

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
 Data File : BP023720.D
 Acq On : 24 Jan 2025 18:40
 Operator : RC/JU
 Sample : PB166118BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	45	rBV	142026	178917	1.18%	0.128%
2	3.705	101	105	130	rBV	1894939	3234474	21.36%	2.308%
3	4.034	158	161	166	rBV	17547	21733	0.14%	0.016%
4	4.499	235	240	244	rBV3	21643	48913	0.32%	0.035%
5	5.517	408	413	420	rBV5	11436	23149	0.15%	0.017%
6	6.358	552	556	563	rBV4	11732	21959	0.15%	0.016%
7	6.958	649	658	671	rBV	2594310	4123704	27.23%	2.943%
8	7.128	680	687	707	rVB	1782261	3179717	21.00%	2.269%
9	7.328	714	721	733	rBV	2588790	4068385	26.87%	2.903%
10	7.793	791	800	814	rBV	1475471	2414855	15.95%	1.723%
11	8.199	866	869	873	rBV4	9848	15405	0.10%	0.011%
12	8.481	909	917	934	rBV	3220585	5122105	33.83%	3.655%
13	8.934	985	994	1006	rBV	2096225	3492890	23.07%	2.493%
14	9.652	1107	1116	1132	rBV	1432517	2424567	16.01%	1.730%
15	10.181	1197	1206	1224	rBV	2987975	4919187	32.49%	3.510%
16	10.563	1254	1271	1285	rBV	2037925	3391288	22.40%	2.420%
17	10.693	1285	1293	1318	rBV	2938428	4830056	31.90%	3.447%
18	12.146	1535	1540	1550	rVB	47250	80508	0.53%	0.057%
19	13.387	1744	1751	1760	rVB5	12027	28423	0.19%	0.020%
20	13.816	1817	1824	1841	rBV	4798385	7125250	47.05%	5.085%
21	14.104	1865	1873	1881	rBV2	5728605	8803921	58.14%	6.283%
22	14.416	1917	1926	1934	rBV	3186218	4615125	30.48%	3.293%
23	14.598	1950	1957	1976	rBV	2403499	3458576	22.84%	2.468%
24	15.069	2031	2037	2041	rBV8	9574	17817	0.12%	0.013%
25	15.428	2091	2098	2105	rBV	7406993	11079631	73.17%	7.907%
26	15.528	2109	2115	2125	rBV	1490385	1907965	12.60%	1.362%
27	15.669	2135	2139	2144	rVB2	35729	50764	0.34%	0.036%
28	16.110	2209	2214	2220	rBV10	7196	20563	0.14%	0.015%
29	17.004	2361	2366	2370	rBV2	14274	23537	0.16%	0.017%
30	17.216	2395	2402	2412	rBV2	3843221	5697720	37.63%	4.066%
31	17.322	2413	2420	2433	rBV	9325966	12463272	82.30%	8.894%
32	17.592	2462	2466	2472	rBV4	8825	18216	0.12%	0.013%
33	17.922	2517	2522	2528	rBV10	10786	23265	0.15%	0.017%
34	18.151	2556	2561	2569	rBV4	65309	119891	0.79%	0.086%
35	18.463	2611	2614	2620	rVB6	10478	15354	0.10%	0.011%
36	19.233	2740	2745	2750	rBV	90418	132039	0.87%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023720.D
Acq On : 24 Jan 2025 18:40
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Title : SVOA CALIBRATION

37	19.304	2753	2757	2762	rVB	80437	114122	0.75%	0.081%
38	19.481	2784	2787	2792	rBV3	81316	98883	0.65%	0.071%
39	19.681	2815	2821	2840	rVB	11688805	15142892	100.00%	10.806%
40	21.651	3150	3156	3170	rBV2	4101125	6442416	42.54%	4.598%
41	24.816	3684	3694	3717	rVB	5723447	14719827	97.21%	10.505%
42	25.045	3723	3733	3747	rVB2	2321627	6417049	42.38%	4.579%




Sum of corrected areas: 140128330

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023720.D
Acq On : 24 Jan 2025 18:40
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

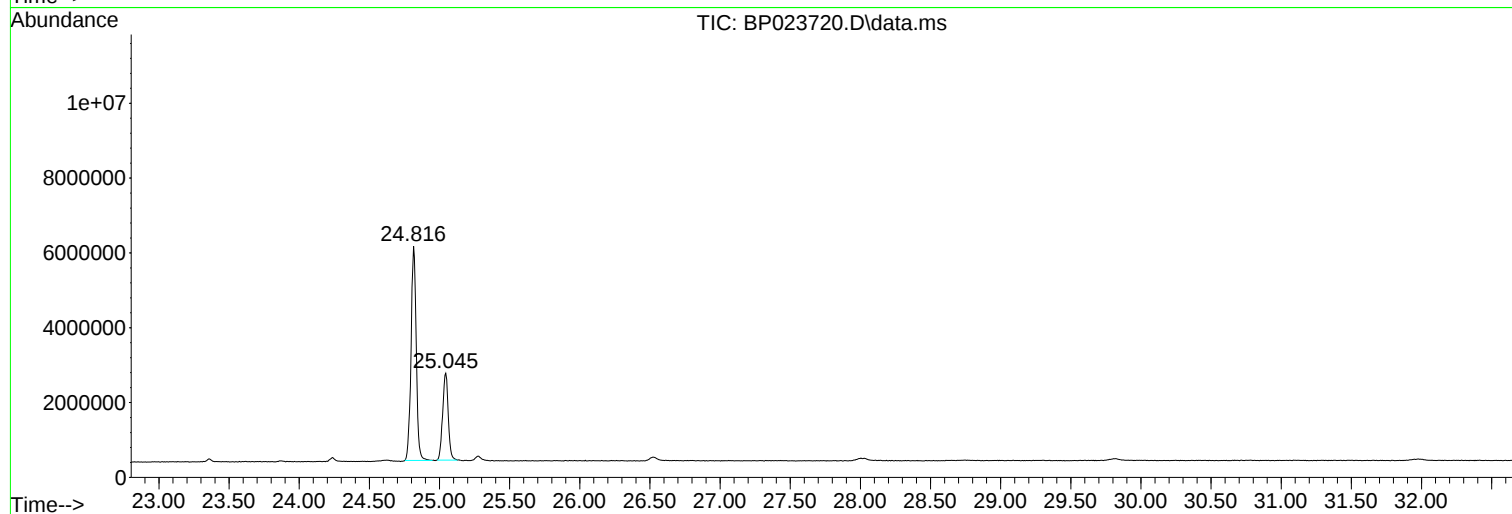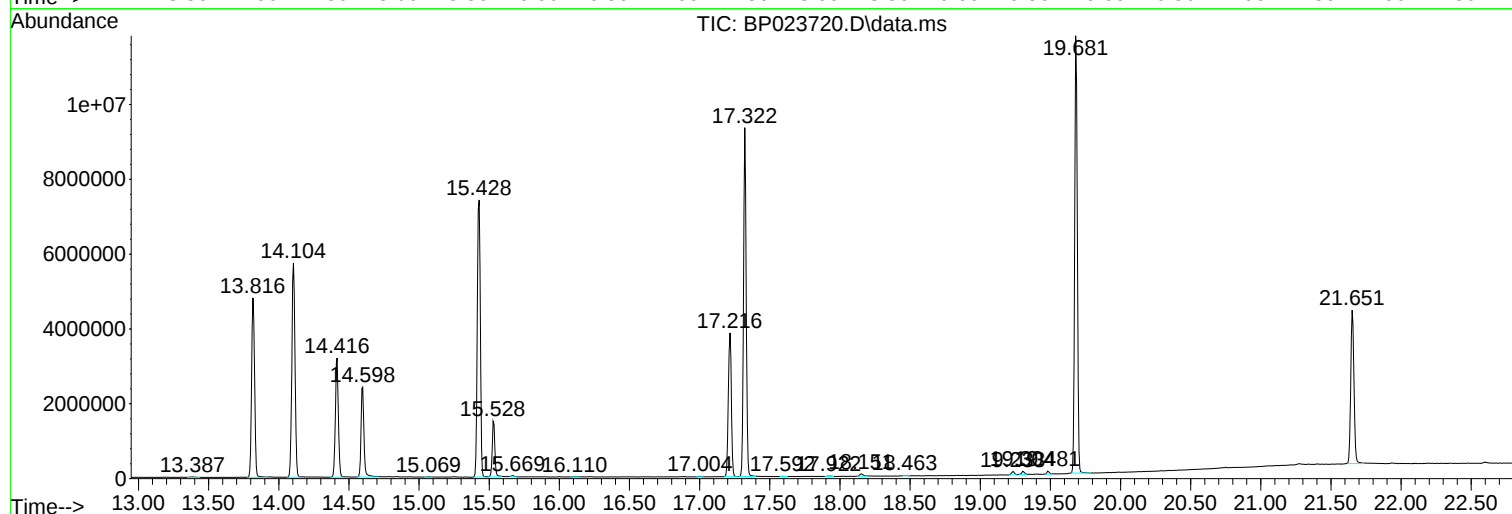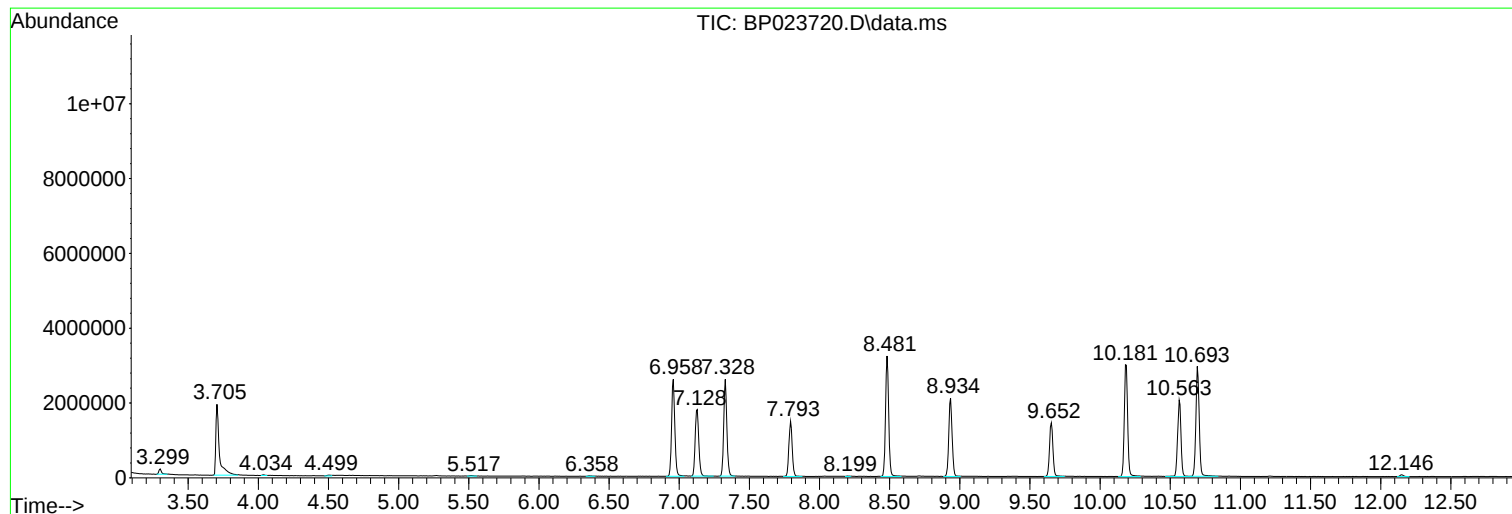

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023720.D
Acq On : 24 Jan 2025 18:40
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023720.D
Acq On : 24 Jan 2025 18:40
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------