
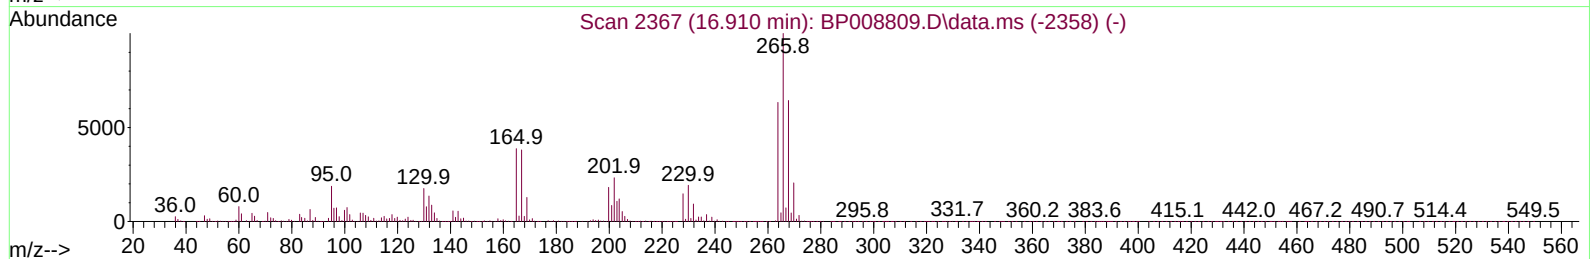
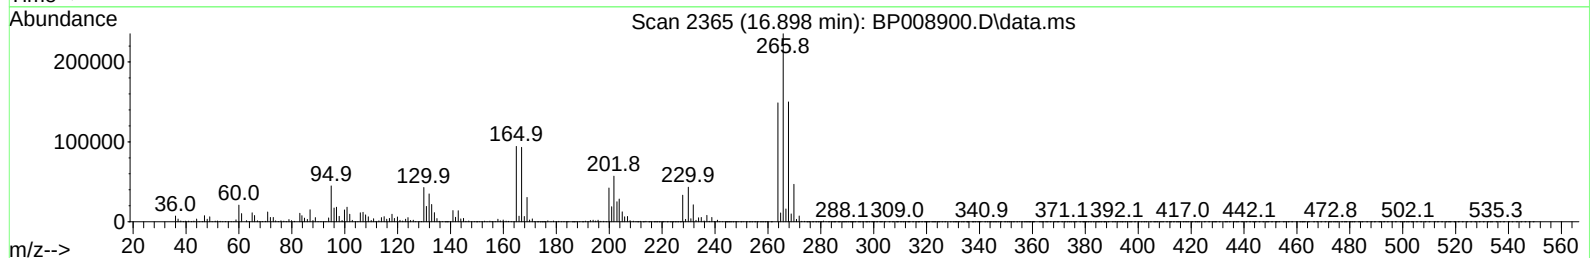


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008900.D
Acq On : 25 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 05:23:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

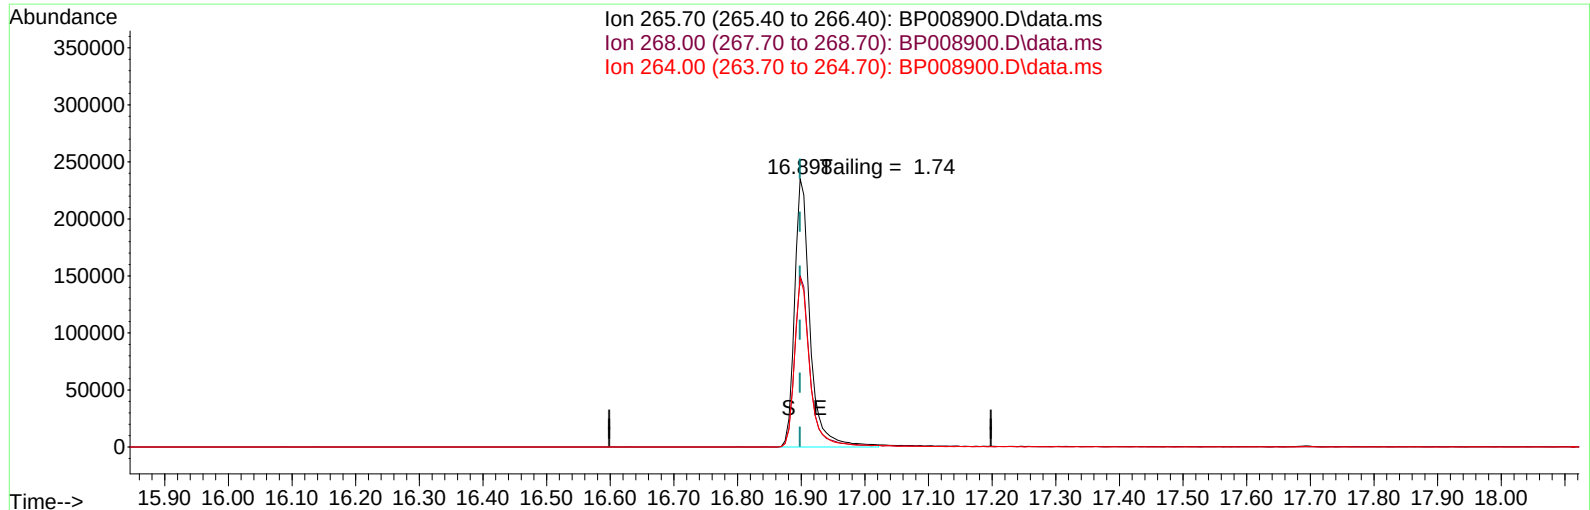

TIC: BP008900.D\data.ms

(70) Pentachlorophenol (C)




16.898min (+ 0.000) 1128008.67 ng

response 404084

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.75
264.00	62.90	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008900.D
 Acq On : 25 Jan 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 05:23:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

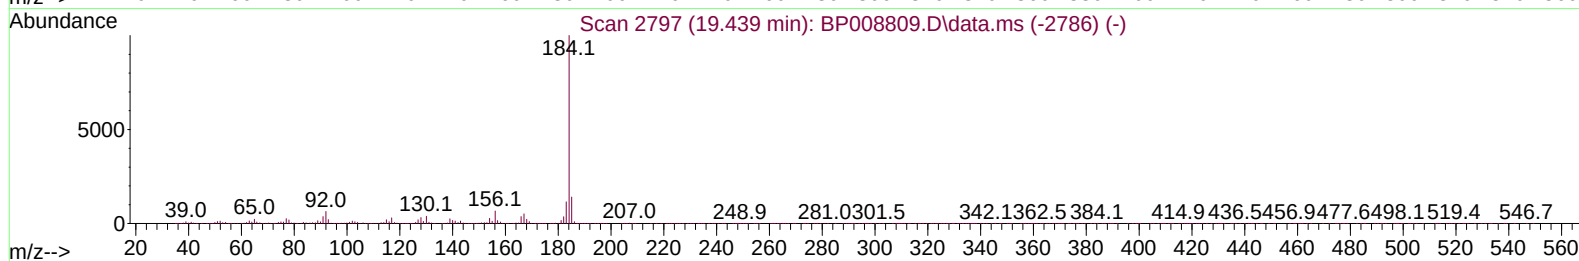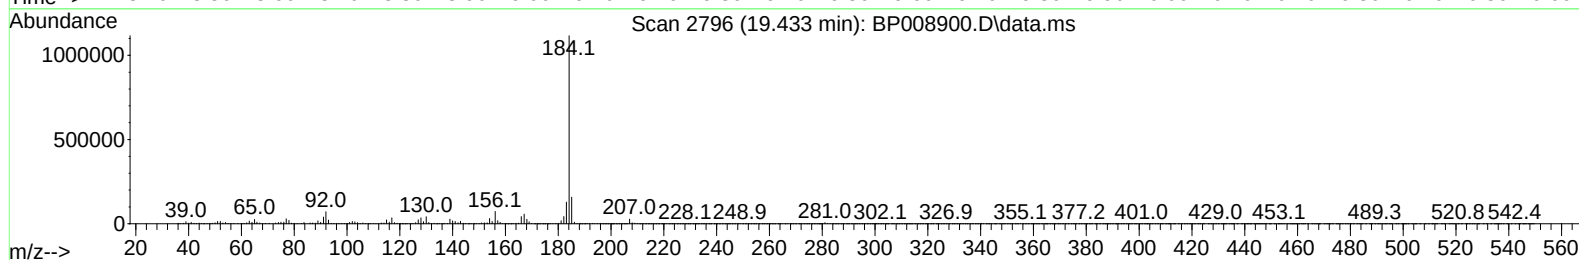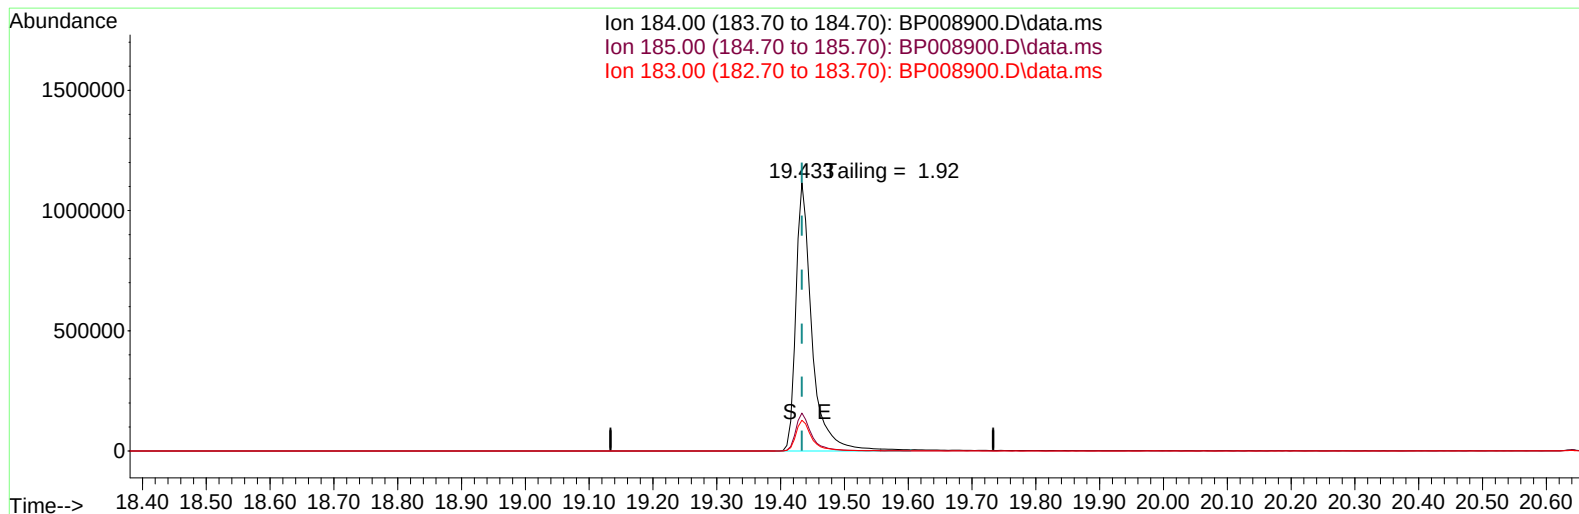

TIC: BP008900.D\data.ms

(77) Benzidine**19.433min (+ 0.000) 480121.21 ng****response 1967548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	11.90	11.48
0.00	0.00	0.00