

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008902.D
 Acq On : 25 Jan 2022 11:51
 Operator : CG/JU
 Sample : PB142179BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142179BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	31	rVB	232895	385134	3.10%	0.600%
2	5.428	408	415	438	rBV	4666460	7202591	58.03%	11.215%
3	7.022	678	686	701	rBV	4114040	6962362	56.10%	10.841%
4	7.840	815	825	837	rBV	959240	1587393	12.79%	2.472%
5	8.999	1014	1022	1045	rBV	2681017	4654698	37.50%	7.248%
6	10.640	1293	1301	1318	rBV	1103888	2075027	16.72%	3.231%
7	13.104	1712	1720	1752	rBV	7293889	11224670	90.44%	17.478%
8	14.481	1947	1954	1968	rBV	1641889	2592692	20.89%	4.037%
9	15.975	2201	2208	2226	rBV	4476757	7211909	58.11%	11.230%
10	17.239	2416	2423	2438	rBV	1766642	2676415	21.56%	4.167%
11	19.798	2853	2858	2868	rBV	10120055	12411333	100.00%	19.326%
12	21.327	3114	3118	3126	rBV	1699855	2384612	19.21%	3.713%
13	23.745	3523	3529	3541	rVB2	1337030	2853441	22.99%	4.443%


Sum of corrected areas: 64222277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008902.D
Acq On : 25 Jan 2022 11:51
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142179BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

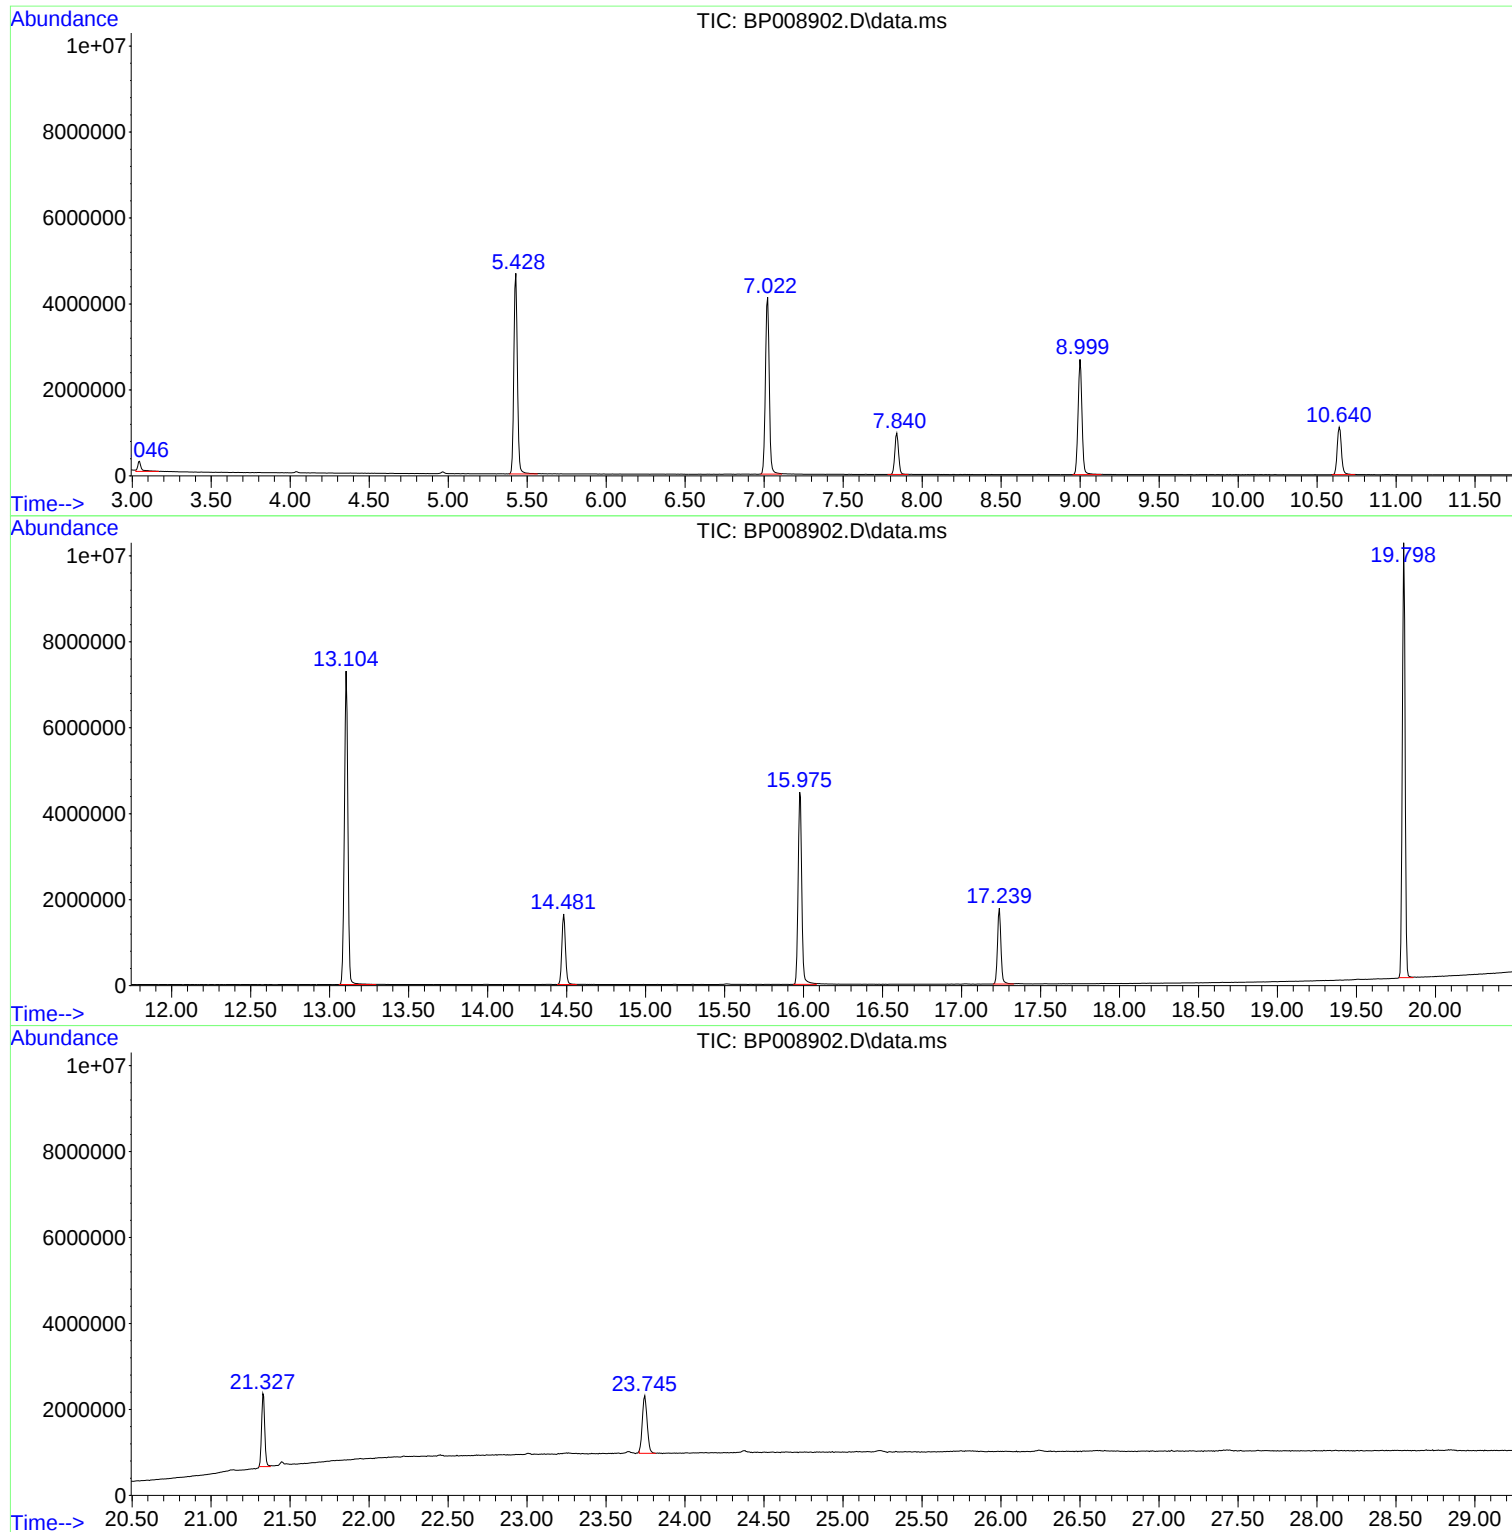

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008902.D
Acq On : 25 Jan 2022 11:51
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142179BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	4.85 ng	385134	1,4-Dichlorobenzene-d4	7.840

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

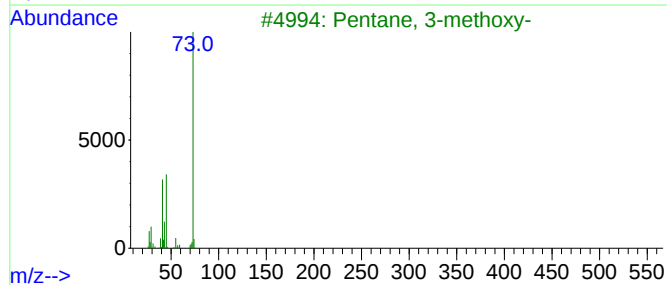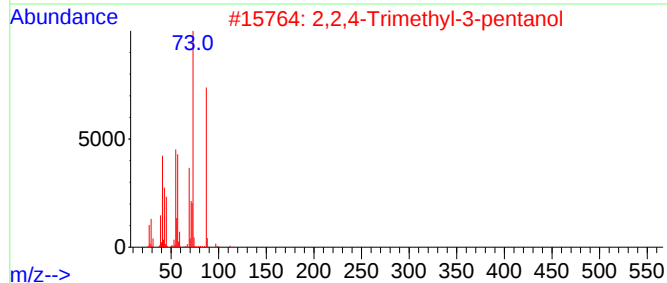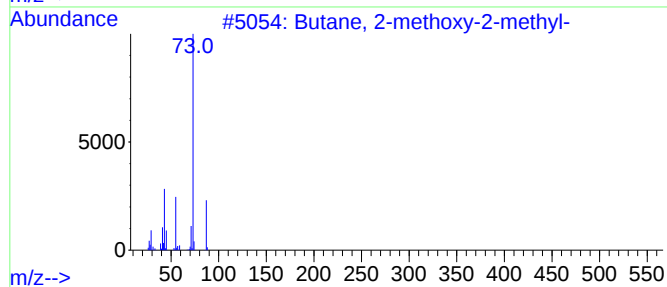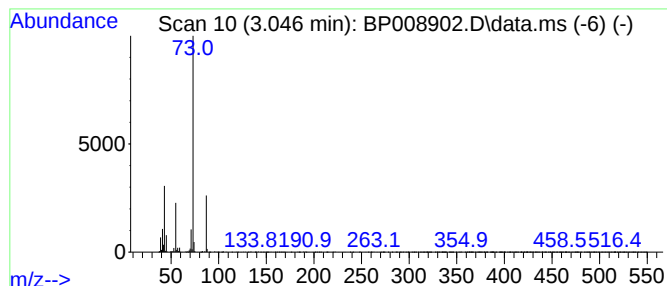

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008902.D
Acq On : 25 Jan 2022 11:51
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142179BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.046	4.8	ng	385134	1	7.840	1587390	20.0