

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008905.D
 Acq On : 25 Jan 2022 13:34
 Operator : CG/JU
 Sample : PB142224BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142224BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	22	rVB	254554	331942	2.29%	0.449%
2	5.428	408	415	436	rBV	5298850	8073585	55.63%	10.932%
3	7.022	678	686	706	rBV	4808705	7957505	54.83%	10.775%
4	7.840	818	825	840	rBV	1070436	1757215	12.11%	2.379%
5	9.005	1014	1023	1045	rBV	2913944	5252913	36.20%	7.113%
6	10.640	1288	1301	1327	rBV	1278359	2394351	16.50%	3.242%
7	13.104	1713	1720	1737	rBV	8635915	13052769	89.94%	17.675%
8	14.481	1946	1954	1971	rBV	2001679	3103142	21.38%	4.202%
9	15.981	2201	2209	2236	rBV	5511426	8912898	61.42%	12.069%
10	17.239	2416	2423	2436	rBV	2157252	3305640	22.78%	4.476%
11	19.804	2853	2859	2869	rBV	11648887	14512373	100.00%	19.651%
12	21.328	3114	3118	3127	rBV	1798346	2562096	17.65%	3.469%
13	23.745	3524	3529	3543	rVB2	1200419	2634230	18.15%	3.567%


Sum of corrected areas: 73850659

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008905.D
Acq On : 25 Jan 2022 13:34
Operator : CG/JU
Sample : PB142224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142224BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

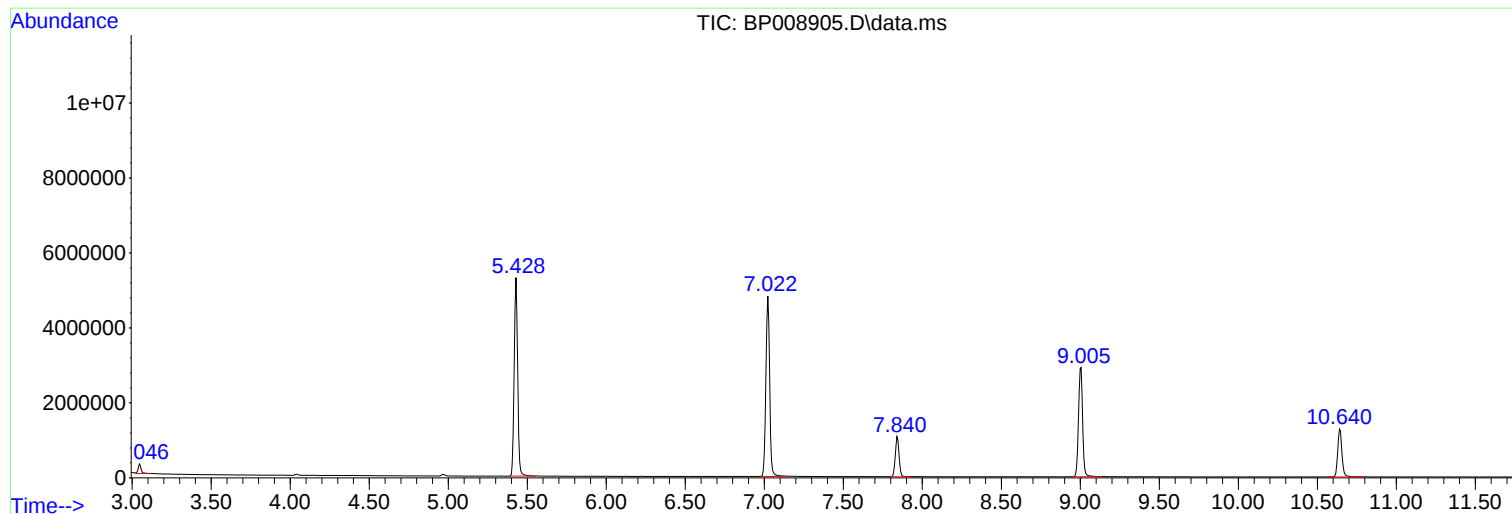

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008905.D
Acq On : 25 Jan 2022 13:34
Operator : CG/JU
Sample : PB142224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142224BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	3.78 ng	331942	1,4-Dichlorobenzene-d4	7.840

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

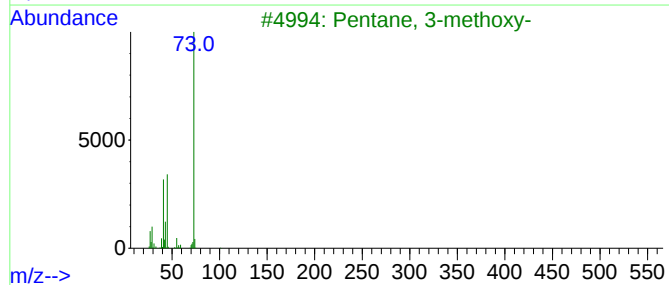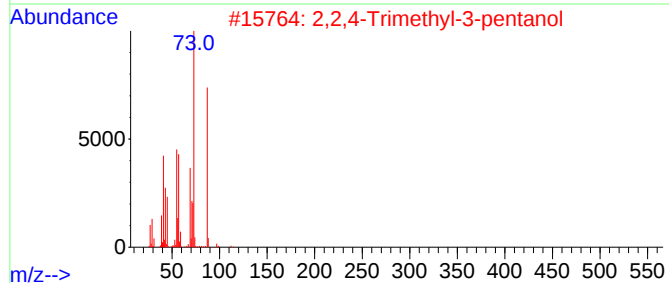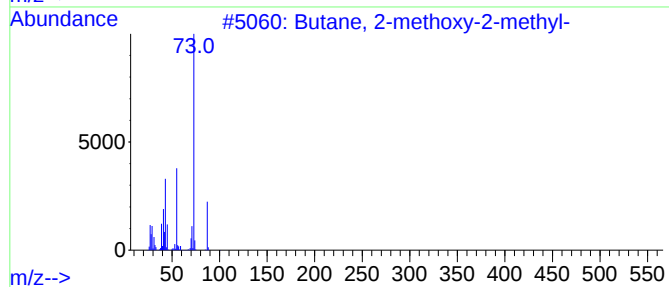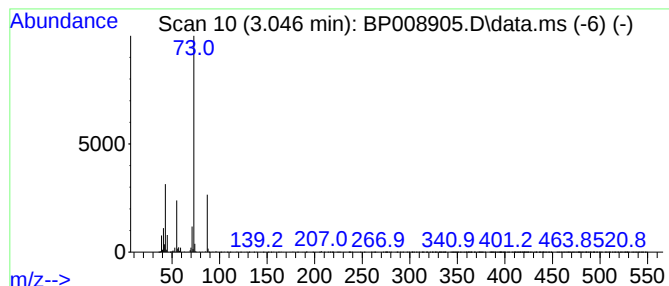

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008905.D
Acq On : 25 Jan 2022 13:34
Operator : CG/JU
Sample : PB142224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142224BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.046	3.8	ng	331942	1	7.840	1757220	20.0