

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008909.D
 Acq On : 25 Jan 2022 16:02
 Operator : CG/JU
 Sample : N1210-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20220027-KEANSBURG-1-COMP-SPLP-LEACHATE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	5	10	19	rVB	1010783	1219476	10.08%	2.103%
2	5.428	409	415	426	rBV	1489541	2246102	18.56%	3.874%
3	7.022	674	686	702	rBV	697365	1430866	11.83%	2.468%
4	7.840	818	825	833	rBV	871860	1415828	11.70%	2.442%
5	8.999	1012	1022	1037	rBV	2337037	4069174	33.63%	7.018%
6	10.640	1293	1301	1309	rBV	1024015	1830658	15.13%	3.157%
7	13.104	1711	1720	1734	rBV	6503242	9882917	81.68%	17.044%
8	13.940	1857	1862	1867	rBV	99041	151115	1.25%	0.261%
9	14.140	1891	1896	1905	rBV4	74805	131796	1.09%	0.227%
10	14.481	1948	1954	1972	rVB	1491493	2363078	19.53%	4.075%
11	15.045	2041	2050	2058	rBV3	35599	130880	1.08%	0.226%
12	15.975	2202	2208	2216	rBV	4378079	6646977	54.93%	11.463%
13	17.057	2389	2392	2402	rVB	126803	206736	1.71%	0.357%
14	17.239	2417	2423	2429	rBV	1754058	2544533	21.03%	4.388%
15	17.528	2469	2472	2483	rBV2	74451	151585	1.25%	0.261%
16	17.916	2534	2538	2542	rVB	364209	428195	3.54%	0.738%
17	18.133	2571	2575	2582	rBV2	397790	585546	4.84%	1.010%
18	19.045	2727	2730	2740	rVB2	518976	695065	5.74%	1.199%
19	19.369	2782	2785	2789	rBV3	139035	209163	1.73%	0.361%
20	19.804	2853	2859	2864	rBV	10052189	12100164	100.00%	20.867%
21	21.045	3066	3070	3077	rBV2	805395	1234159	10.20%	2.128%
22	21.110	3078	3081	3088	rVB	315202	395295	3.27%	0.682%
23	21.333	3114	3119	3126	rBV	1949954	2543463	21.02%	4.386%
24	21.445	3134	3138	3150	rVB	2010882	2749561	22.72%	4.742%
25	23.751	3524	3530	3540	rVB2	1251567	2623699	21.68%	4.525%




Sum of corrected areas: 57986031

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008909.D
Acq On : 25 Jan 2022 16:02
Operator : CG/JU
Sample : N1210-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20220027-KEANSBURG-1-COMP-SPLP-LEACHATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

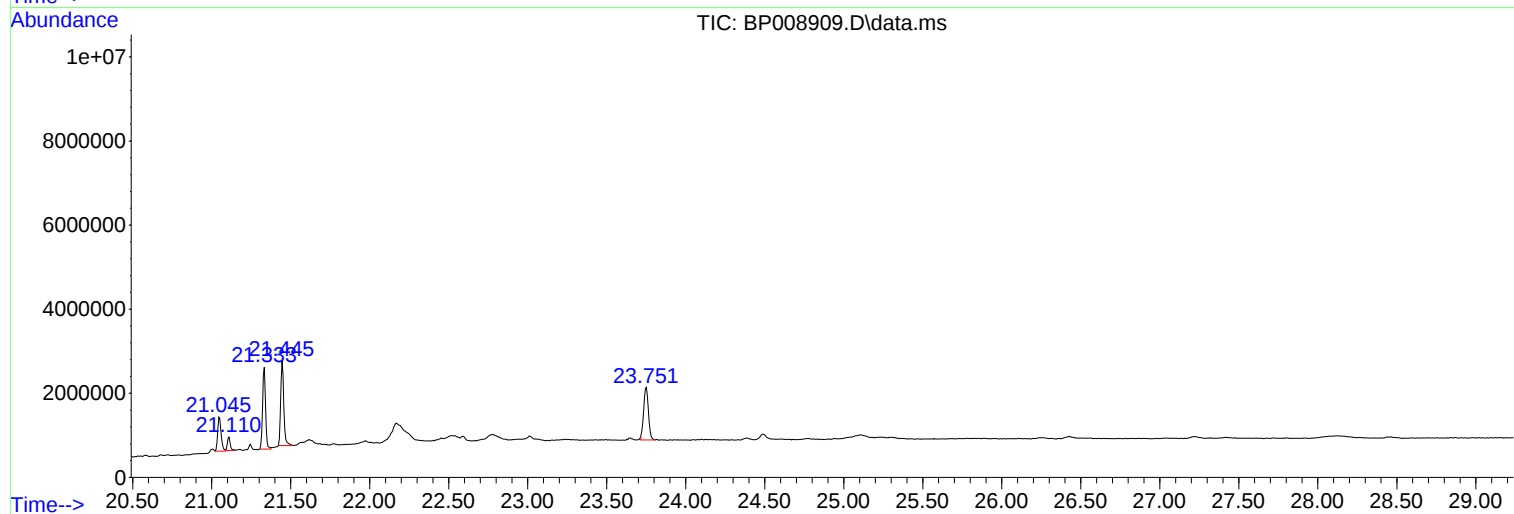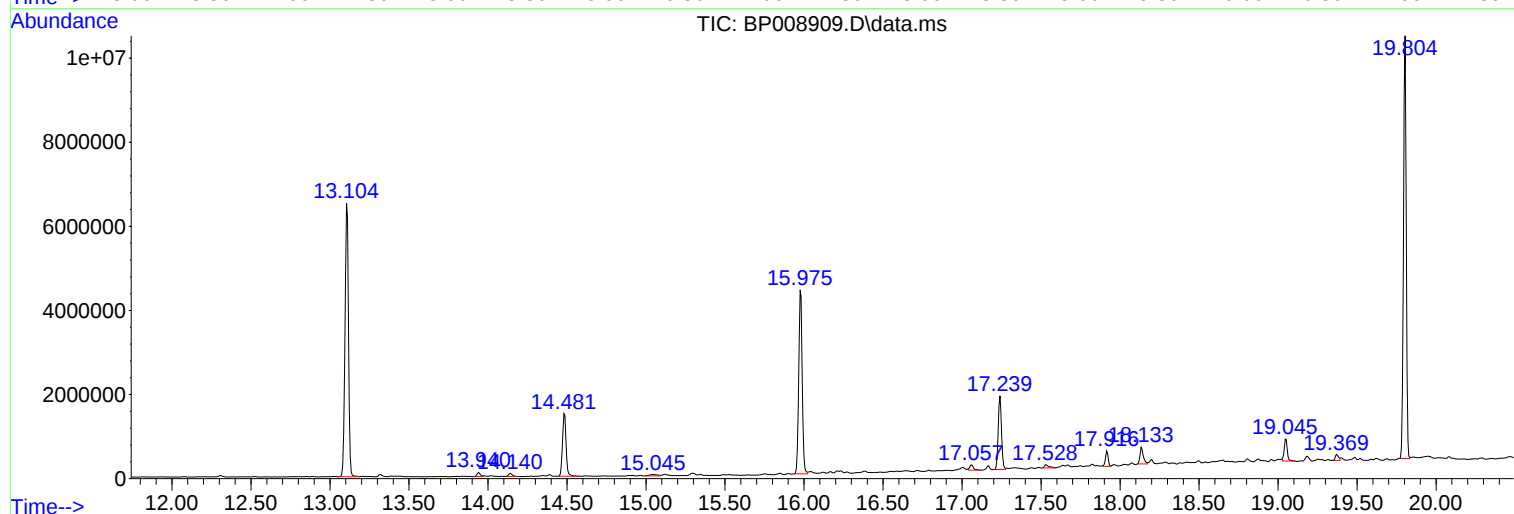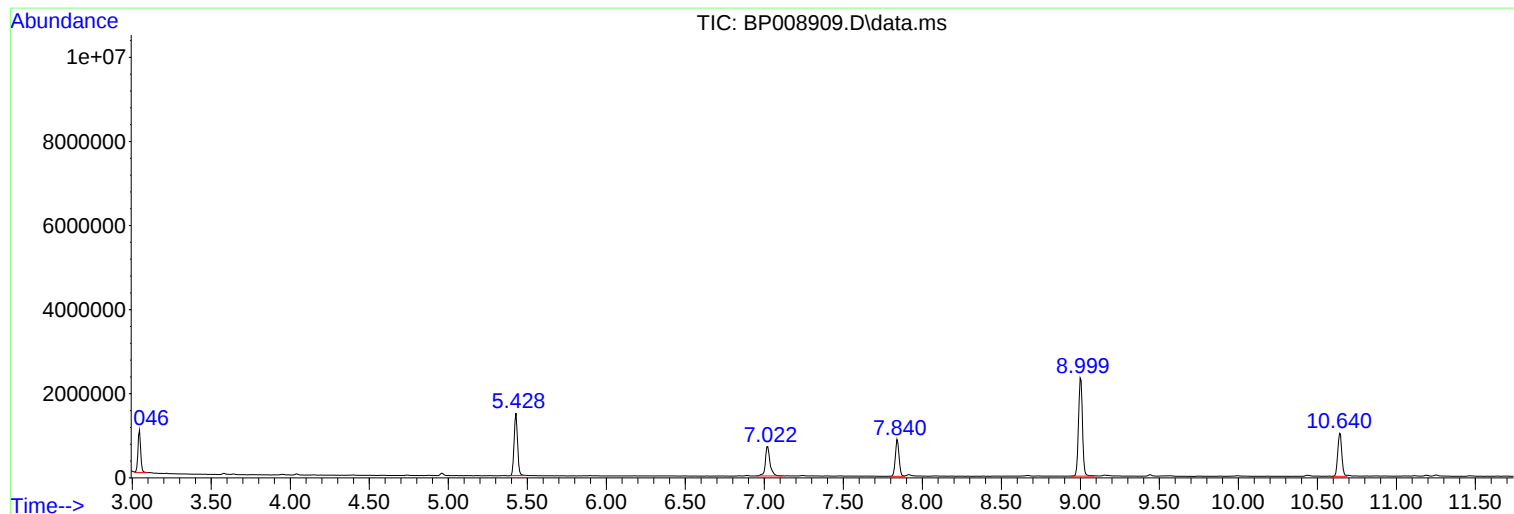

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008909.D
Acq On : 25 Jan 2022 16:02
Operator : CG/JU
Sample : N1210-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20220027-KEANSBURG-1-COMP-SPLP-LEACHATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008909.D
Acq On : 25 Jan 2022 16:02
Operator : CG/JU
Sample : N1210-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20220027-KEANSBURG-1-COMP-SPLP-LEACHATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------