
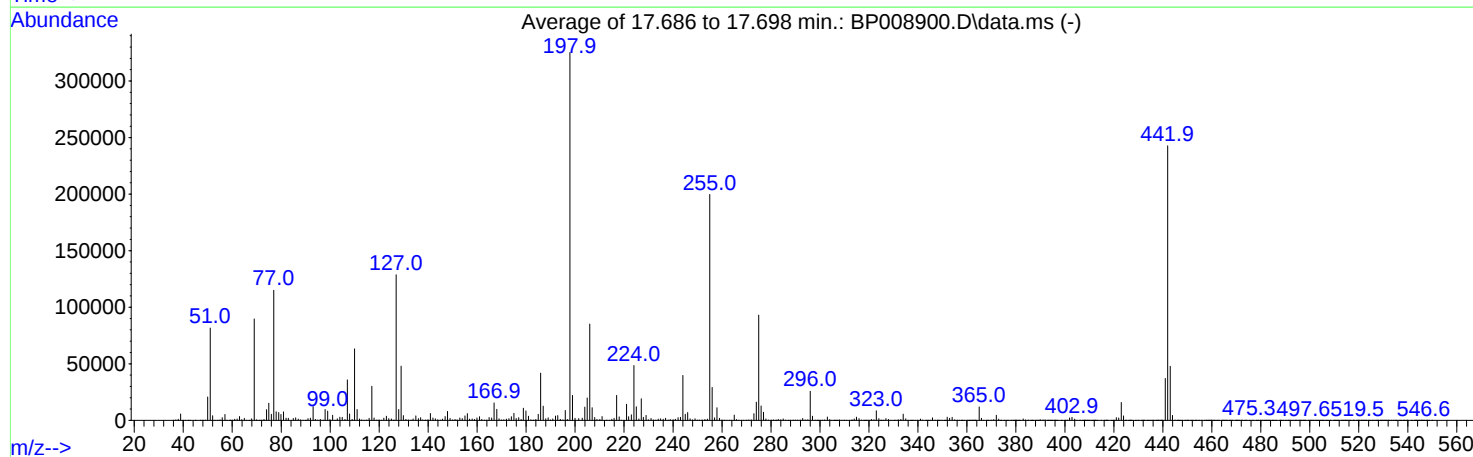


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008900.D
 Acq On : 25 Jan 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 26 01:52:51 2022

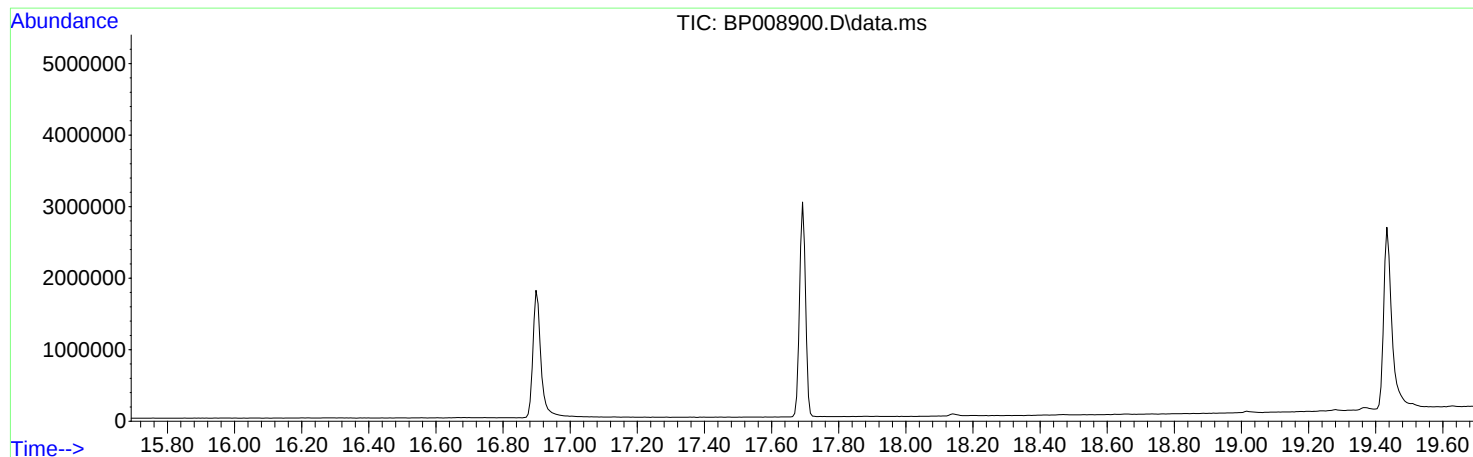




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	81659	PASS
68	69	0.00	2	1.6	1445	PASS
69	198	0.00	100	27.6	89644	PASS
70	69	0.00	2	0.6	579	PASS
127	198	10	80	39.6	128767	PASS
197	198	0.00	2	0.2	656	PASS
198	198	100	100	100.0	325184	PASS
199	198	5	9	6.8	22043	PASS
275	198	10	60	28.6	93080	PASS
365	198	1	100	3.7	11964	PASS
441	198	0.01	100	11.4	37075	PASS
442	442	100	100	100.0	242786	PASS
443	442	15	24	19.7	47770	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
Data File : BP008900.D
Acq On : 25 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 26 05:23:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

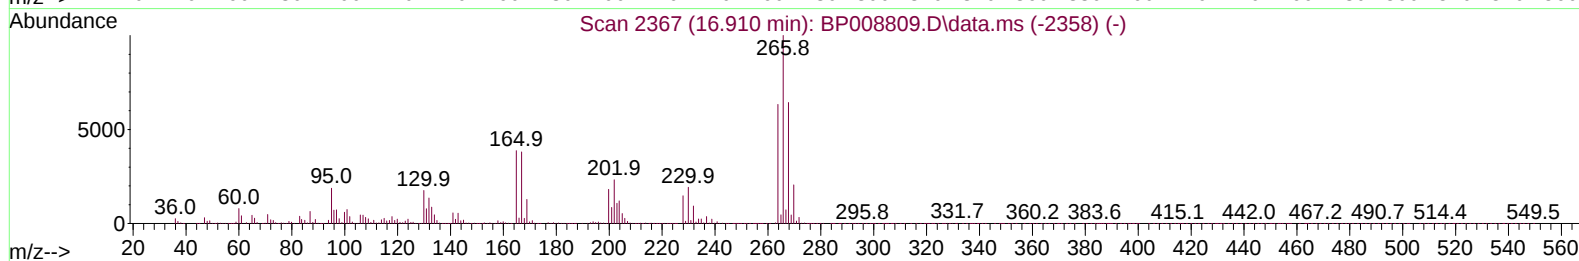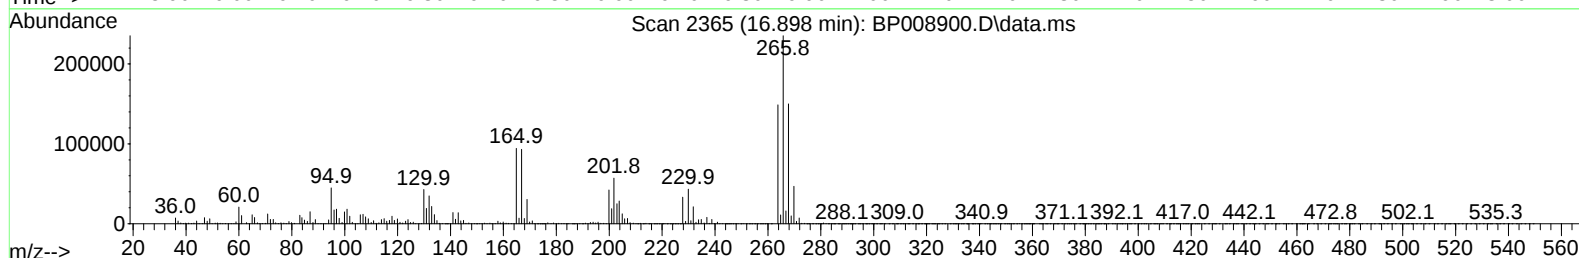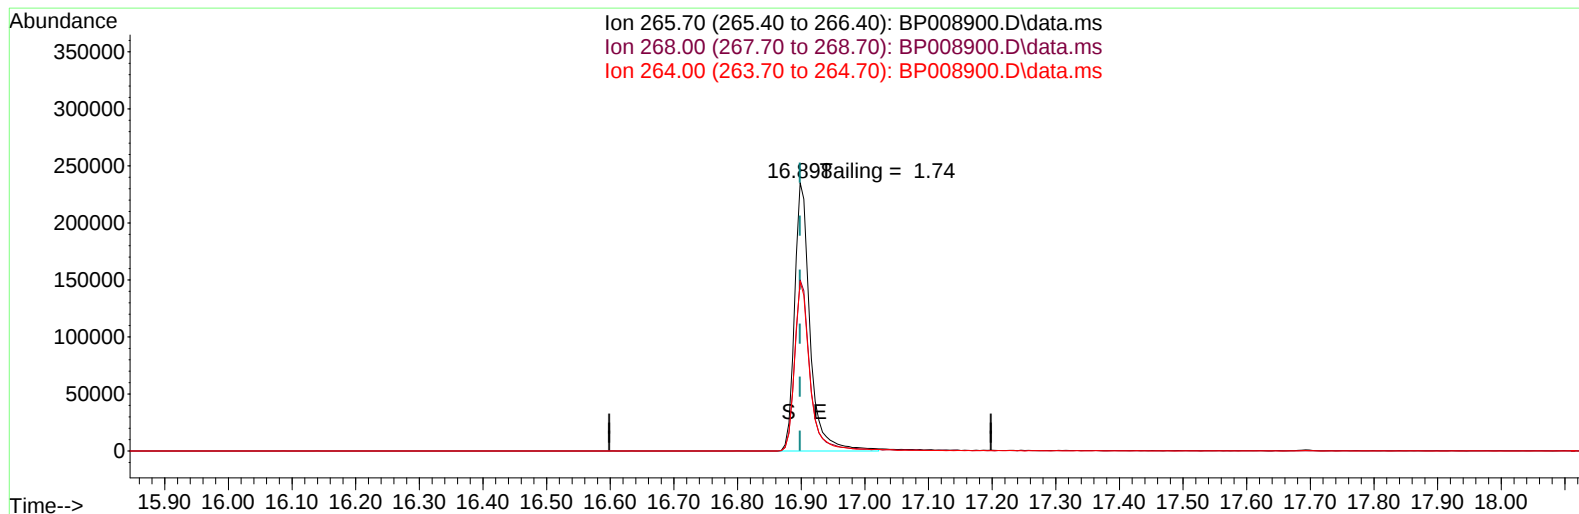

TIC: BP008900.D\data.ms

(70) Pentachlorophenol (C)

16.898min (+ 0.000) 1128008.67 ng




response 404084

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.75
264.00	62.90	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012522\
 Data File : BP008900.D
 Acq On : 25 Jan 2022 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 26 05:23:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

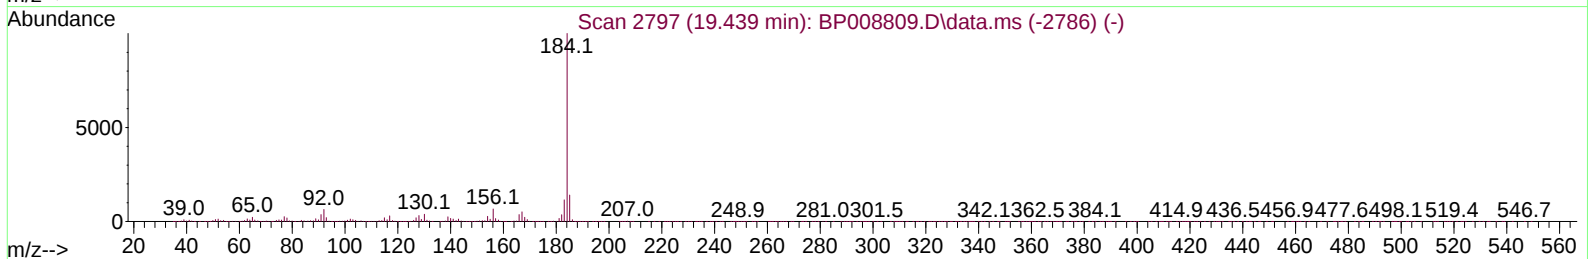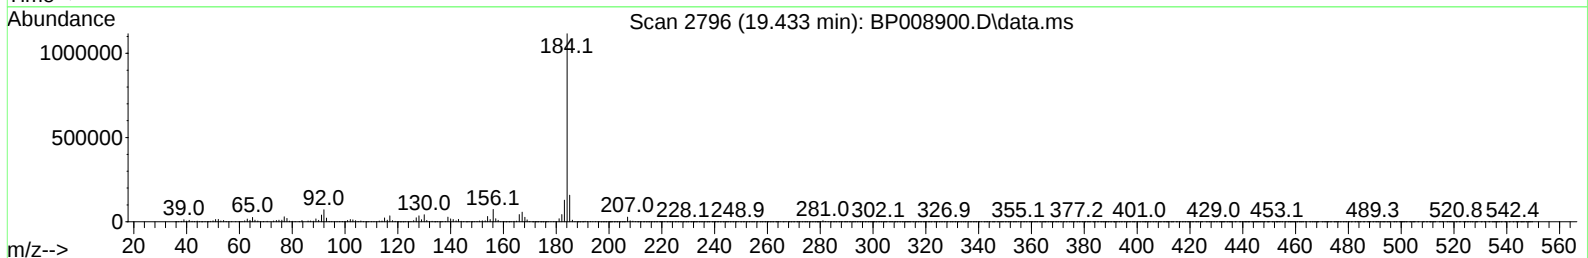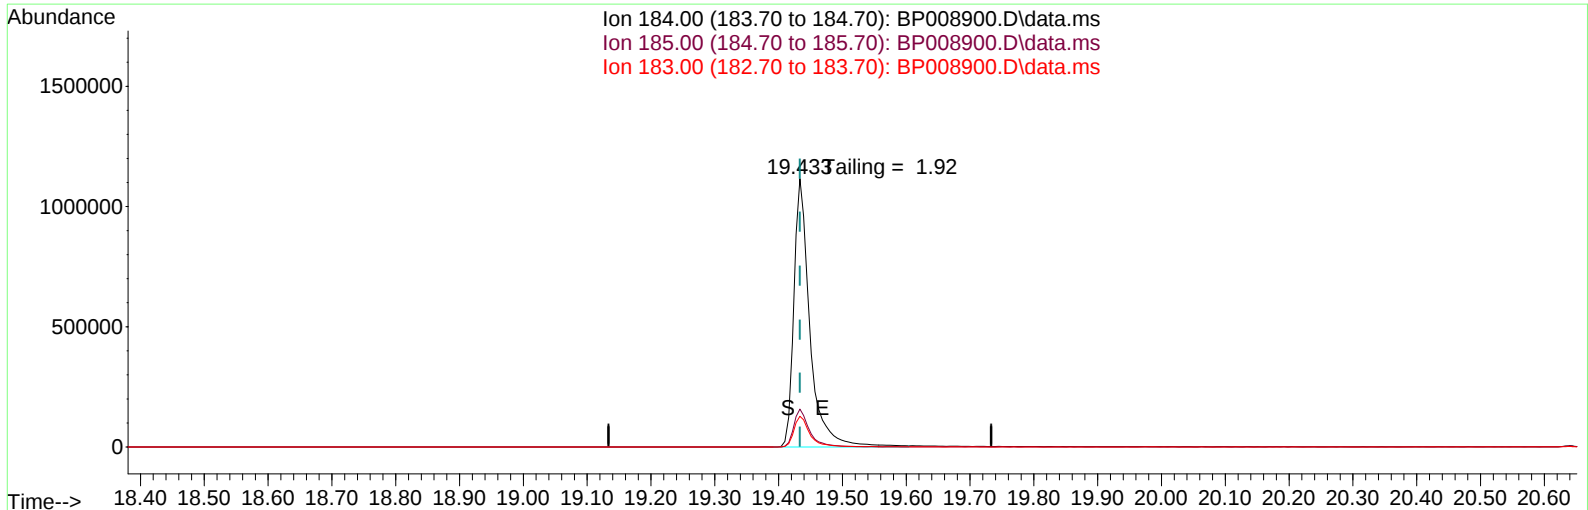

TIC: BP008900.D\data.ms

(77) Benzidine

19.433min (+ 0.000) 480121.21 ng

response 1967548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	11.90	11.48
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2022	BNA_P	<u>BP008900.D</u>
Compound Name	Response	Retention Time
DDT	1135742	20.639
DDD	39382	20.21
DDE	2985	19.716
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42367	1178109	3.60