
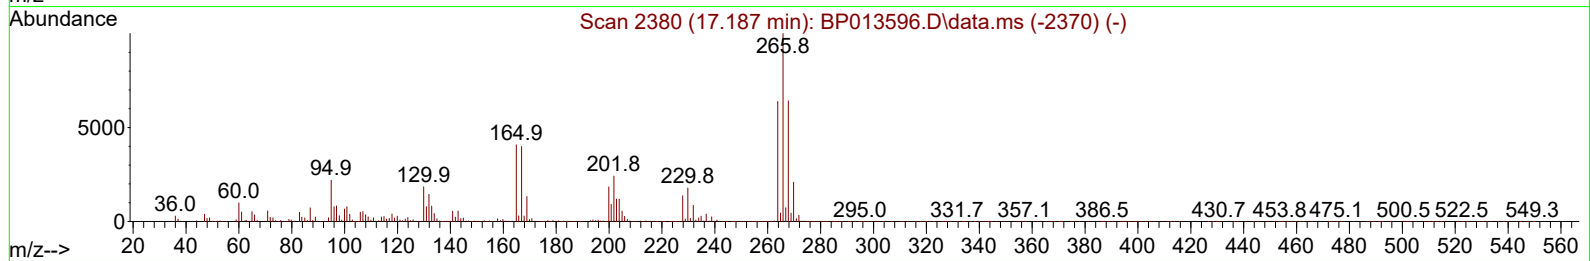
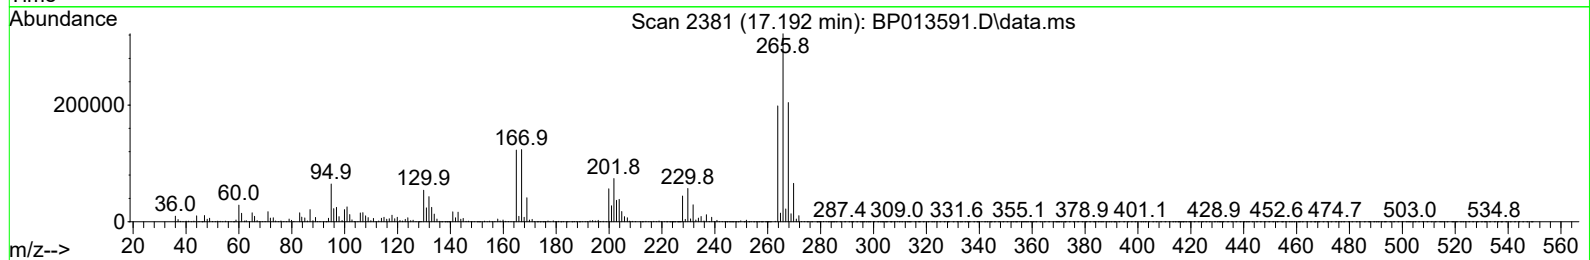


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012623\
 Data File : BP013591.D
 Acq On : 26 Jan 2023 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:14:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 03:27:54 2023
 Response via : Initial Calibration

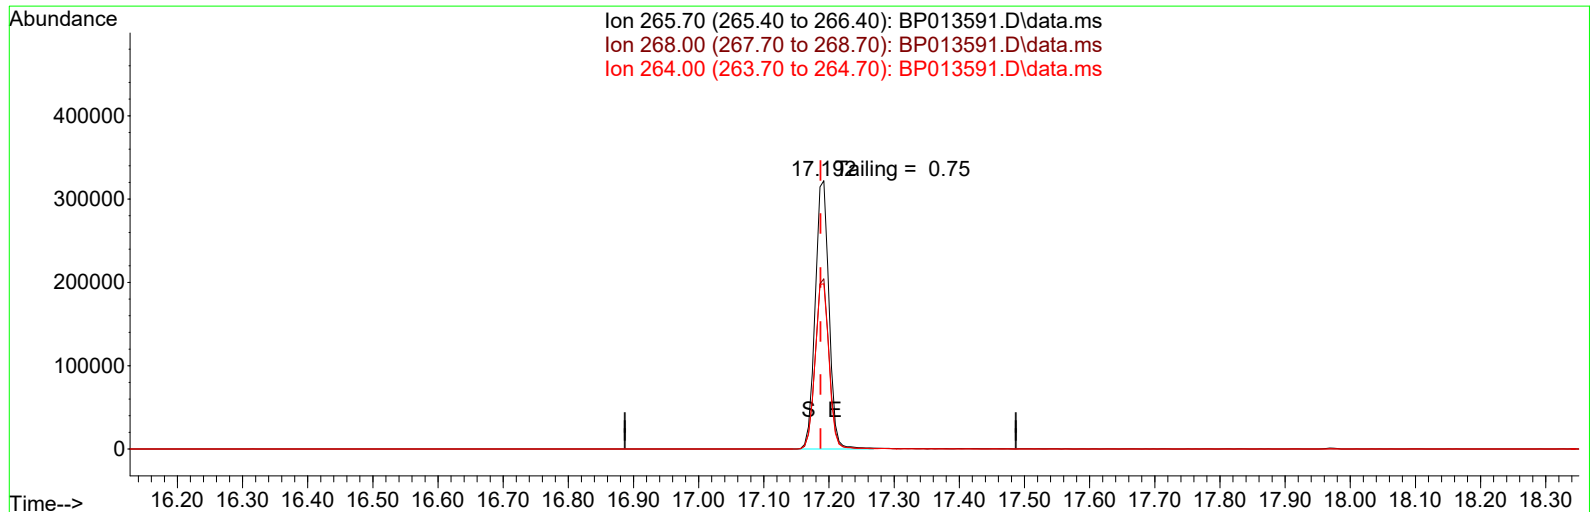

TIC: BP013591.D\data.ms

(70) Pentachlorophenol (C)




17.192min (+ 0.005) 2313826.33 ng

response 475763

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.43
264.00	63.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012623\
Data File : BP013591.D
Acq On : 26 Jan 2023 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:14:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 03:27:54 2023
Response via : Initial Calibration

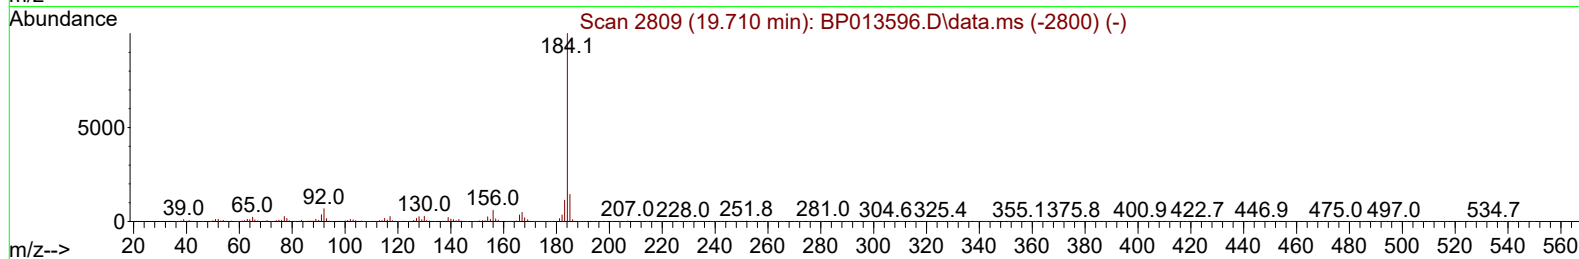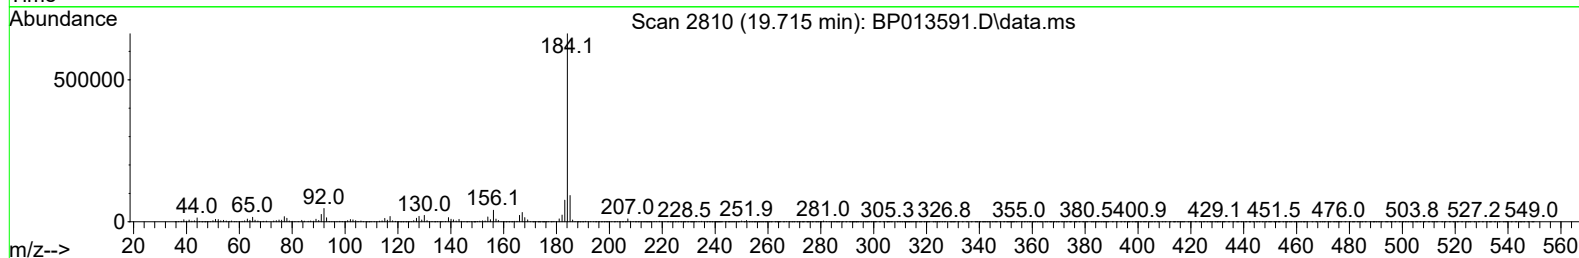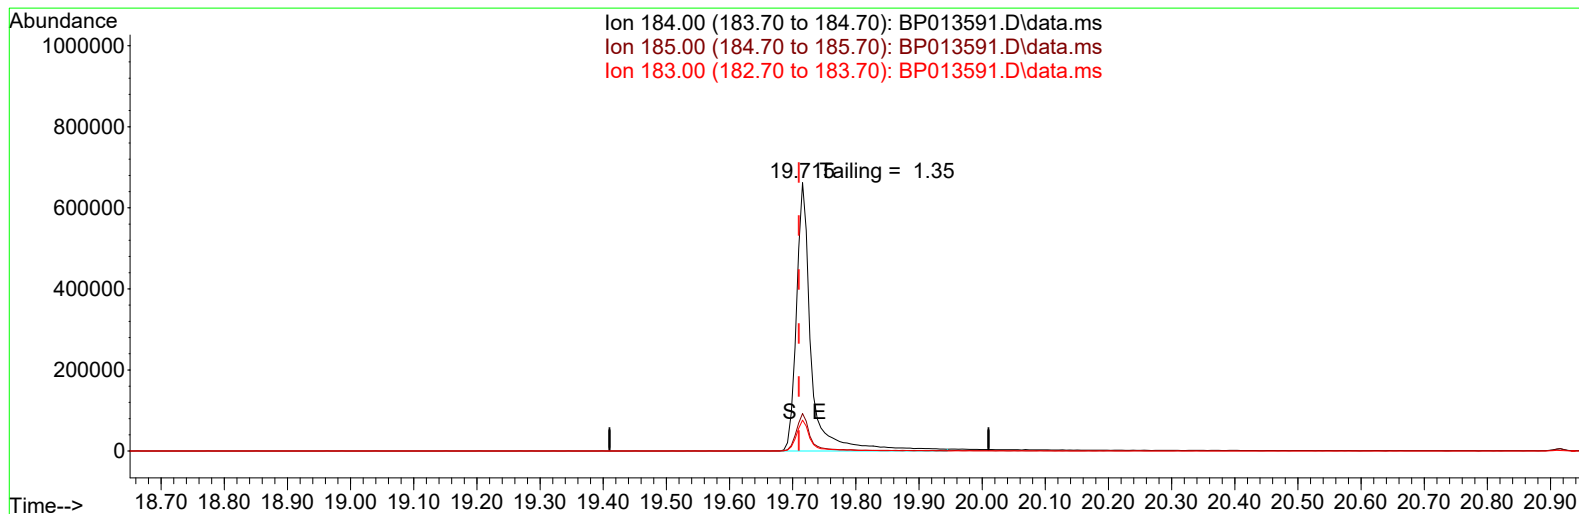

TIC: BP013591.D\data.ms

(77) Benzidine**19.715min (+ 0.005) 261590.70 ng****response 1086074**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.94
183.00	11.30	11.50
0.00	0.00	0.00