


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012623\
Data File : BP013591.D
Acq On : 26 Jan 2023 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 27 03:27:54 2023

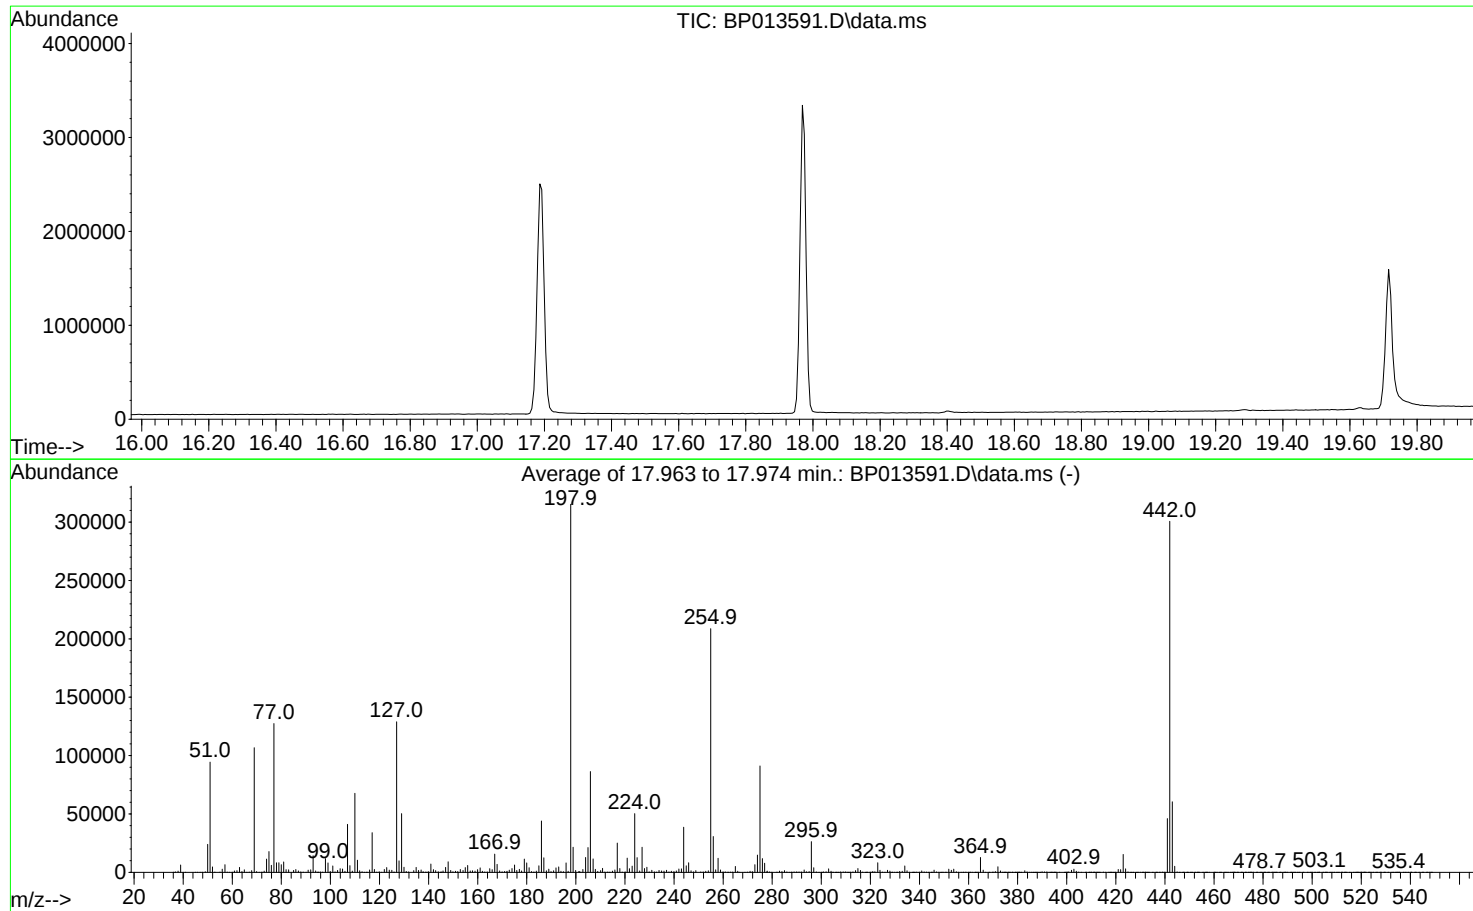




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	94439	PASS
68	69	0.00	2	1.4	1497	PASS
69	198	0.00	100	33.9	106702	PASS
70	69	0.00	2	0.5	575	PASS
127	198	10	80	40.9	128948	PASS
197	198	0.00	2	0.3	861	PASS
198	198	100	100	100.0	315179	PASS
199	198	5	9	6.8	21440	PASS
275	198	10	60	28.9	91065	PASS
365	198	1	100	4.0	12725	PASS
441	198	0.01	100	14.6	45960	PASS
442	442	100	100	100.0	300736	PASS
443	442	15	24	20.1	60392	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012623\
 Data File : BP013591.D
 Acq On : 26 Jan 2023 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 27 05:14:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 03:27:54 2023
 Response via : Initial Calibration

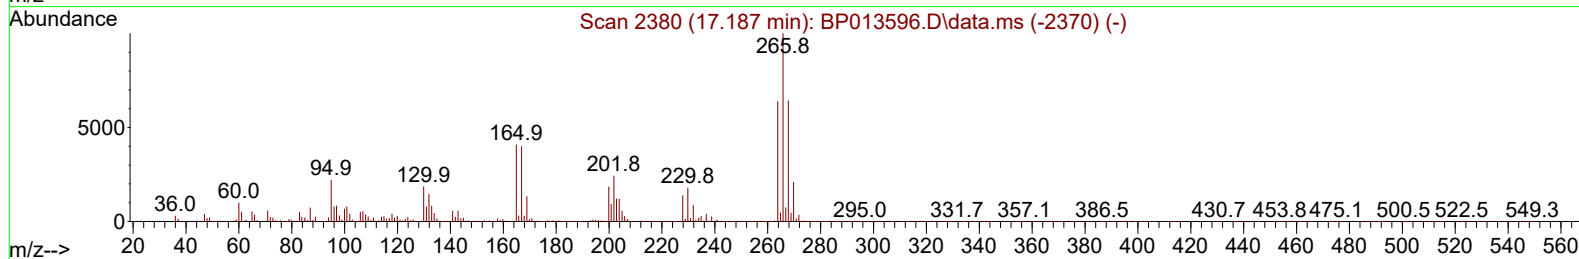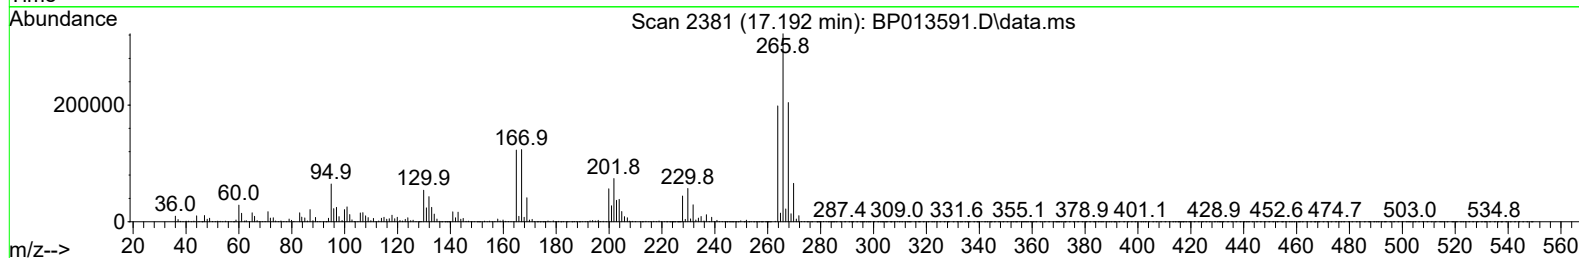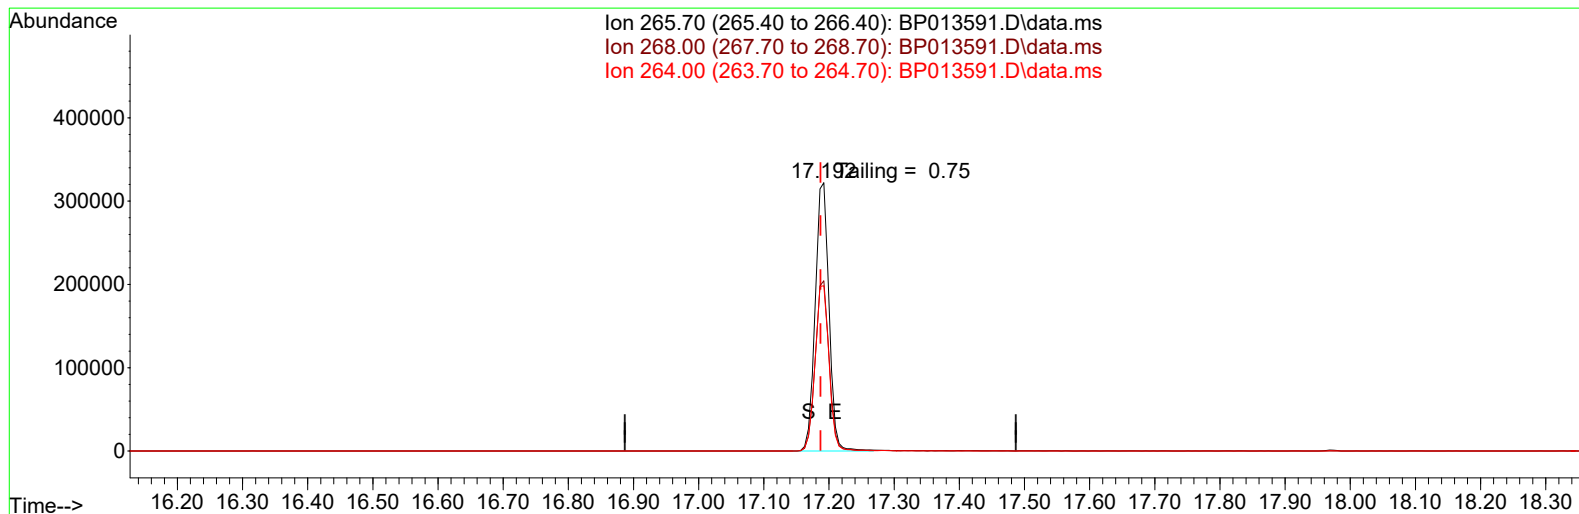

TIC: BP013591.D\data.ms

(70) Pentachlorophenol (C)

17.192min (+ 0.005) 2313826.33 ng




response 475763

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.43
264.00	63.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012623\
 Data File : BP013591.D
 Acq On : 26 Jan 2023 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 27 05:14:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 03:27:54 2023
 Response via : Initial Calibration

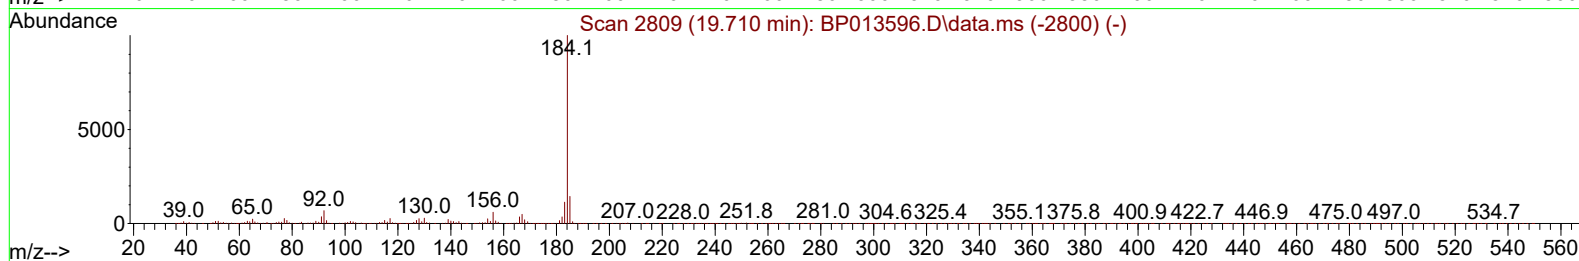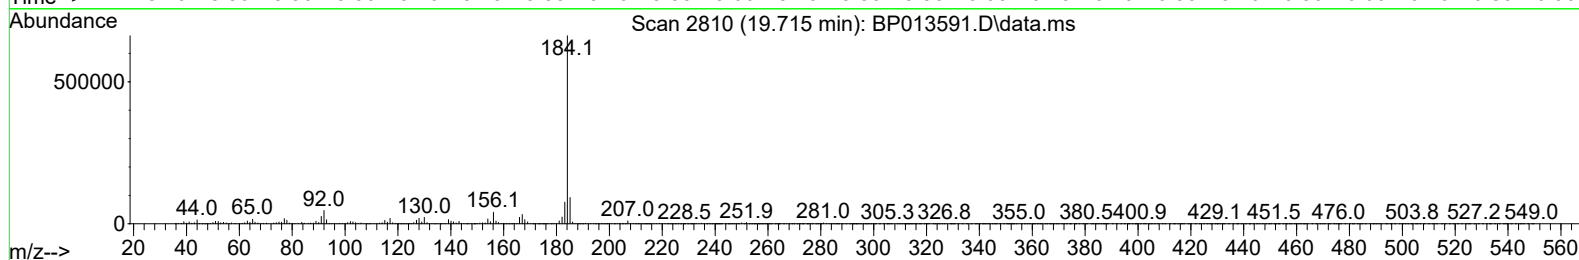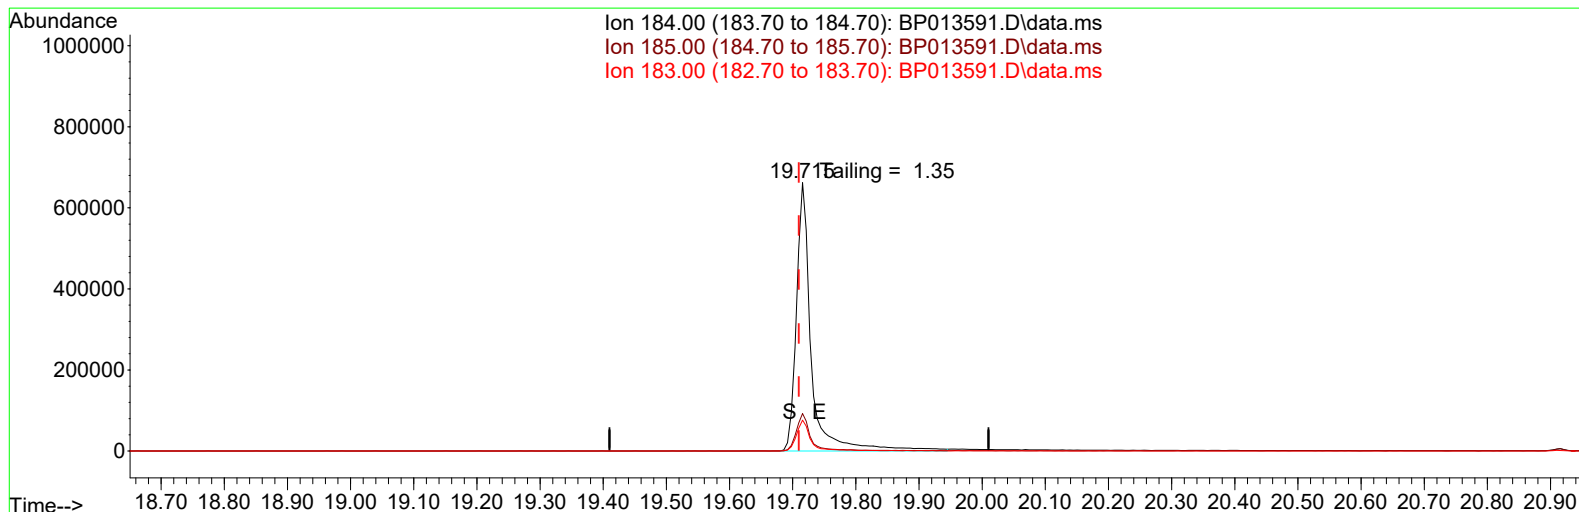

TIC: BP013591.D\data.ms

(77) Benzidine

19.715min (+ 0.005) 261590.70 ng

response 1086074

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.94
183.00	11.30	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/26/2023	BNA_P	<u>BP013591.D</u>
Compound Name	Response	Retention Time
DDT	711904	20.915
DDD	10022	20.539
DDE	1732	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11754	723658	1.62

Instrument :
BNA_P
ClientSampleId :
DFTPP