
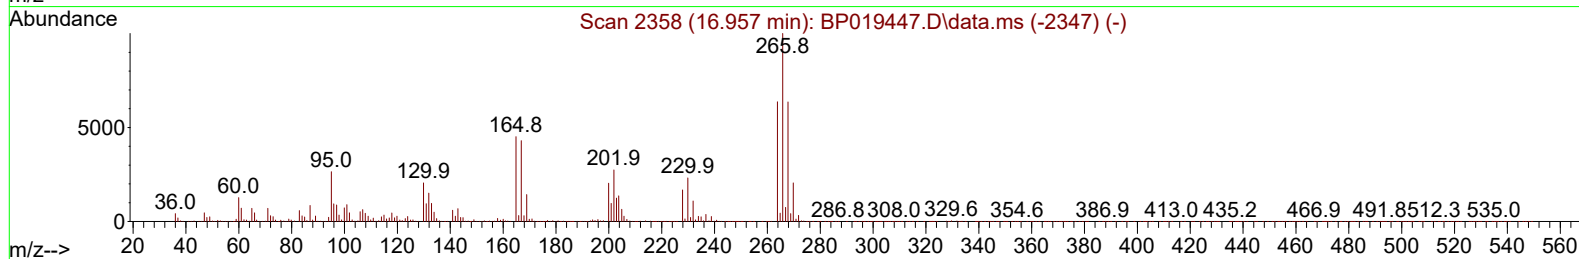
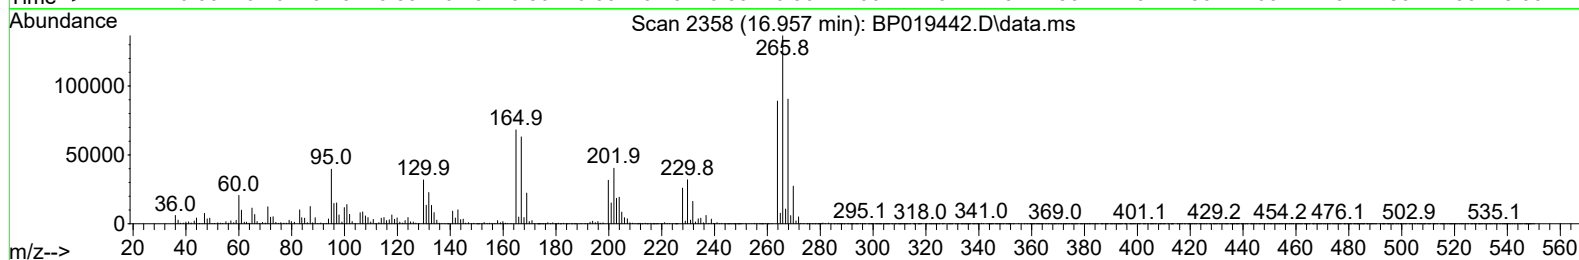


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019442.D
Acq On : 26 Jan 2024 10:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 00:23:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 23:43:31 2024
Response via : Initial Calibration

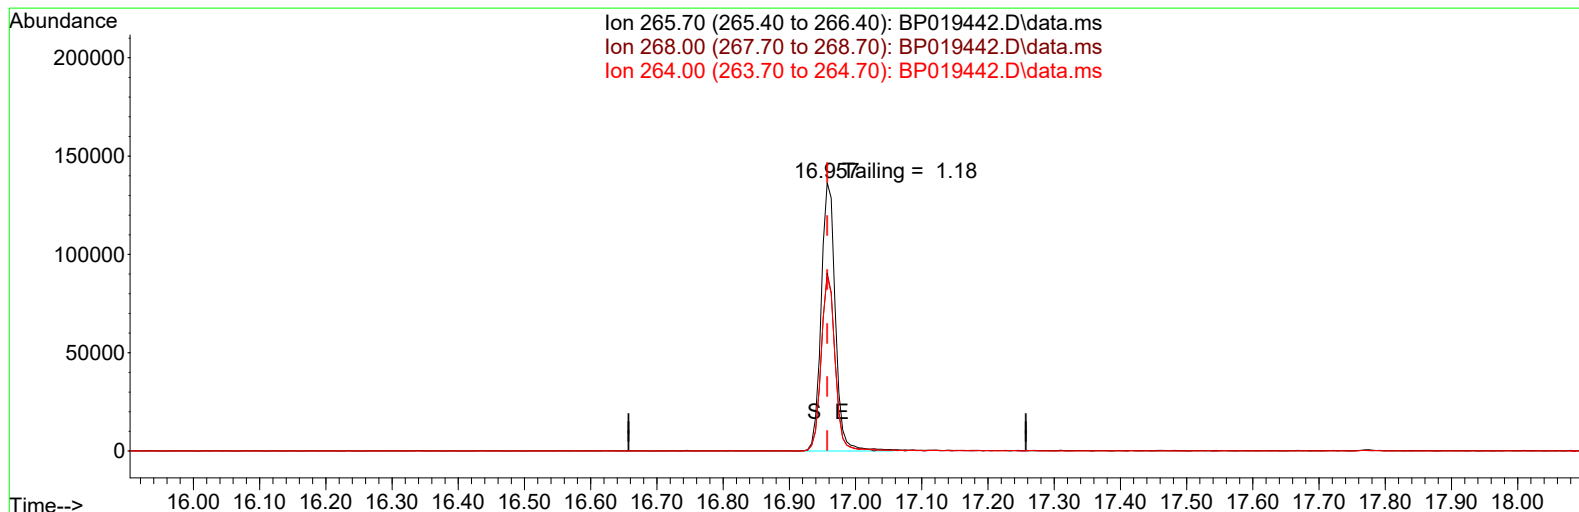

TIC: BP019442.D\data.ms

(70) Pentachlorophenol (C)




16.957min (-0.000) 1531485.39 ng

response 203799

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	66.33
264.00	63.70	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019442.D
Acq On : 26 Jan 2024 10:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 00:23:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 23:43:31 2024
Response via : Initial Calibration

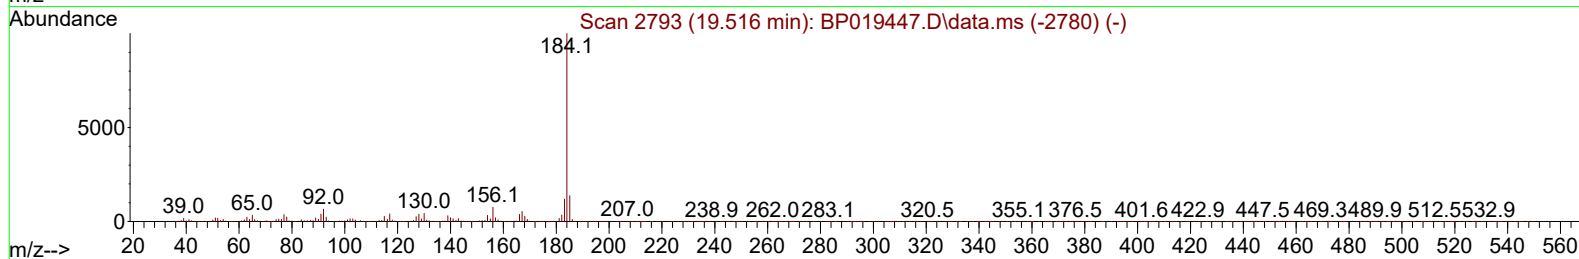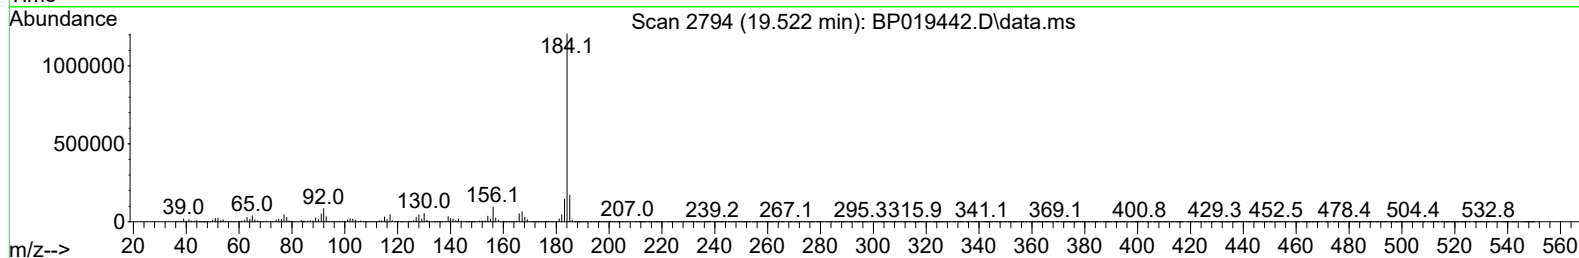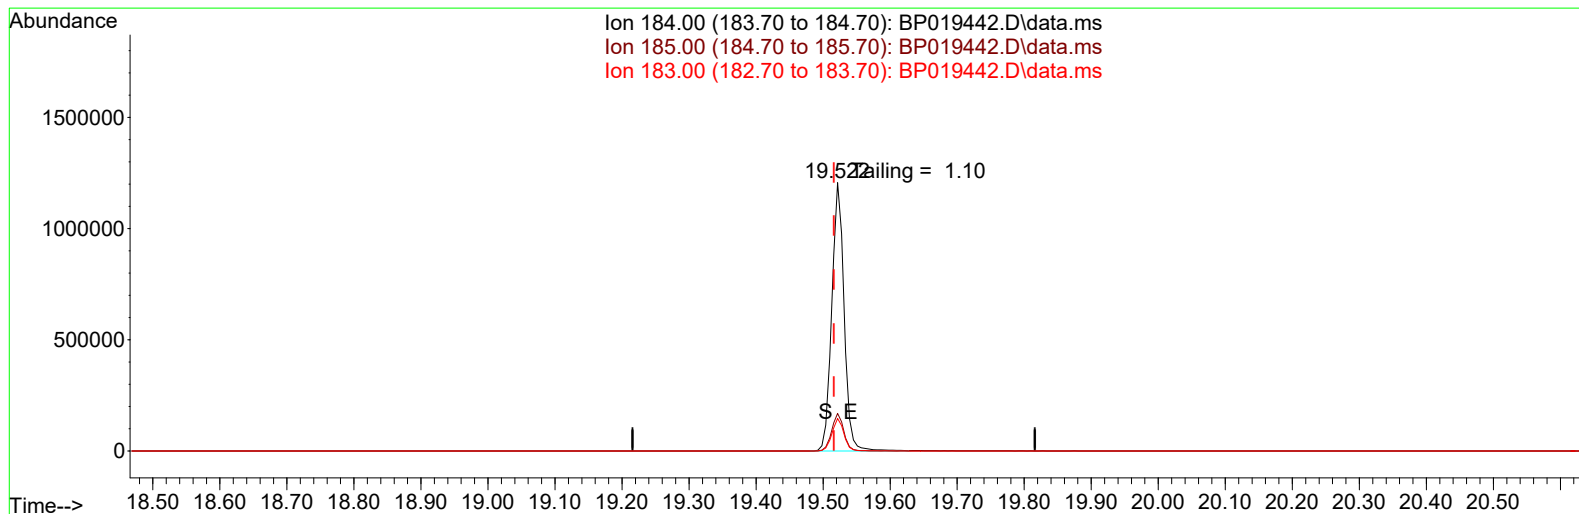

TIC: BP019442.D\data.ms

(77) Benzidine**19.522min (+ 0.006) 636000.23 ng****response 1542458**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	11.80	12.12
0.00	0.00	0.00