

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
 Data File : BP019457.D
 Acq On : 26 Jan 2024 20:44
 Operator : MA/JU
 Sample : P1240-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 72-11985

Quant Time: Jan 27 00:18:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 23:43:31 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	65977	20.000	ng	-0.01
21) Naphthalene-d8	10.716	136	262656	20.000	ng	-0.01
39) Acenaphthene-d10	14.545	164	170795	20.000	ng	-0.01
64) Phenanthrene-d10	17.304	188	390669	20.000	ng	-0.01
76) Chrysene-d12	21.398	240	386243	20.000	ng	-0.01
86) Perylene-d12	23.827	264	439967	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	450196	107.350	ng	-0.01
7) Phenol-d6	7.081	99	614923	99.267	ng	-0.01
23) Nitrobenzene-d5	9.081	82	410985	70.471	ng	-0.02
42) 2,4,6-Tribromophenol	16.039	330	211000	95.396	ng	-0.01
45) 2-Fluorobiphenyl	13.181	172	820984	63.710	ng	-0.01
79) Terphenyl-d14	19.874	244	1404758	59.629	ng	-0.01
Target Compounds						Qvalue
71) Phenanthrene	17.351	178	46781	2.250	ng	99
75) Fluoranthene	19.316	202	86074	3.184	ng	100
78) Pyrene	19.669	202	72706	2.604	ng	99
84) Bis(2-ethylhexyl)phtha...	21.339	149	172914	9.847	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019457.D
Acq On : 26 Jan 2024 20:44
Operator : MA/JU
Sample : P1240-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11985

Quant Time: Jan 27 00:18:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 23:43:31 2024
Response via : Initial Calibration




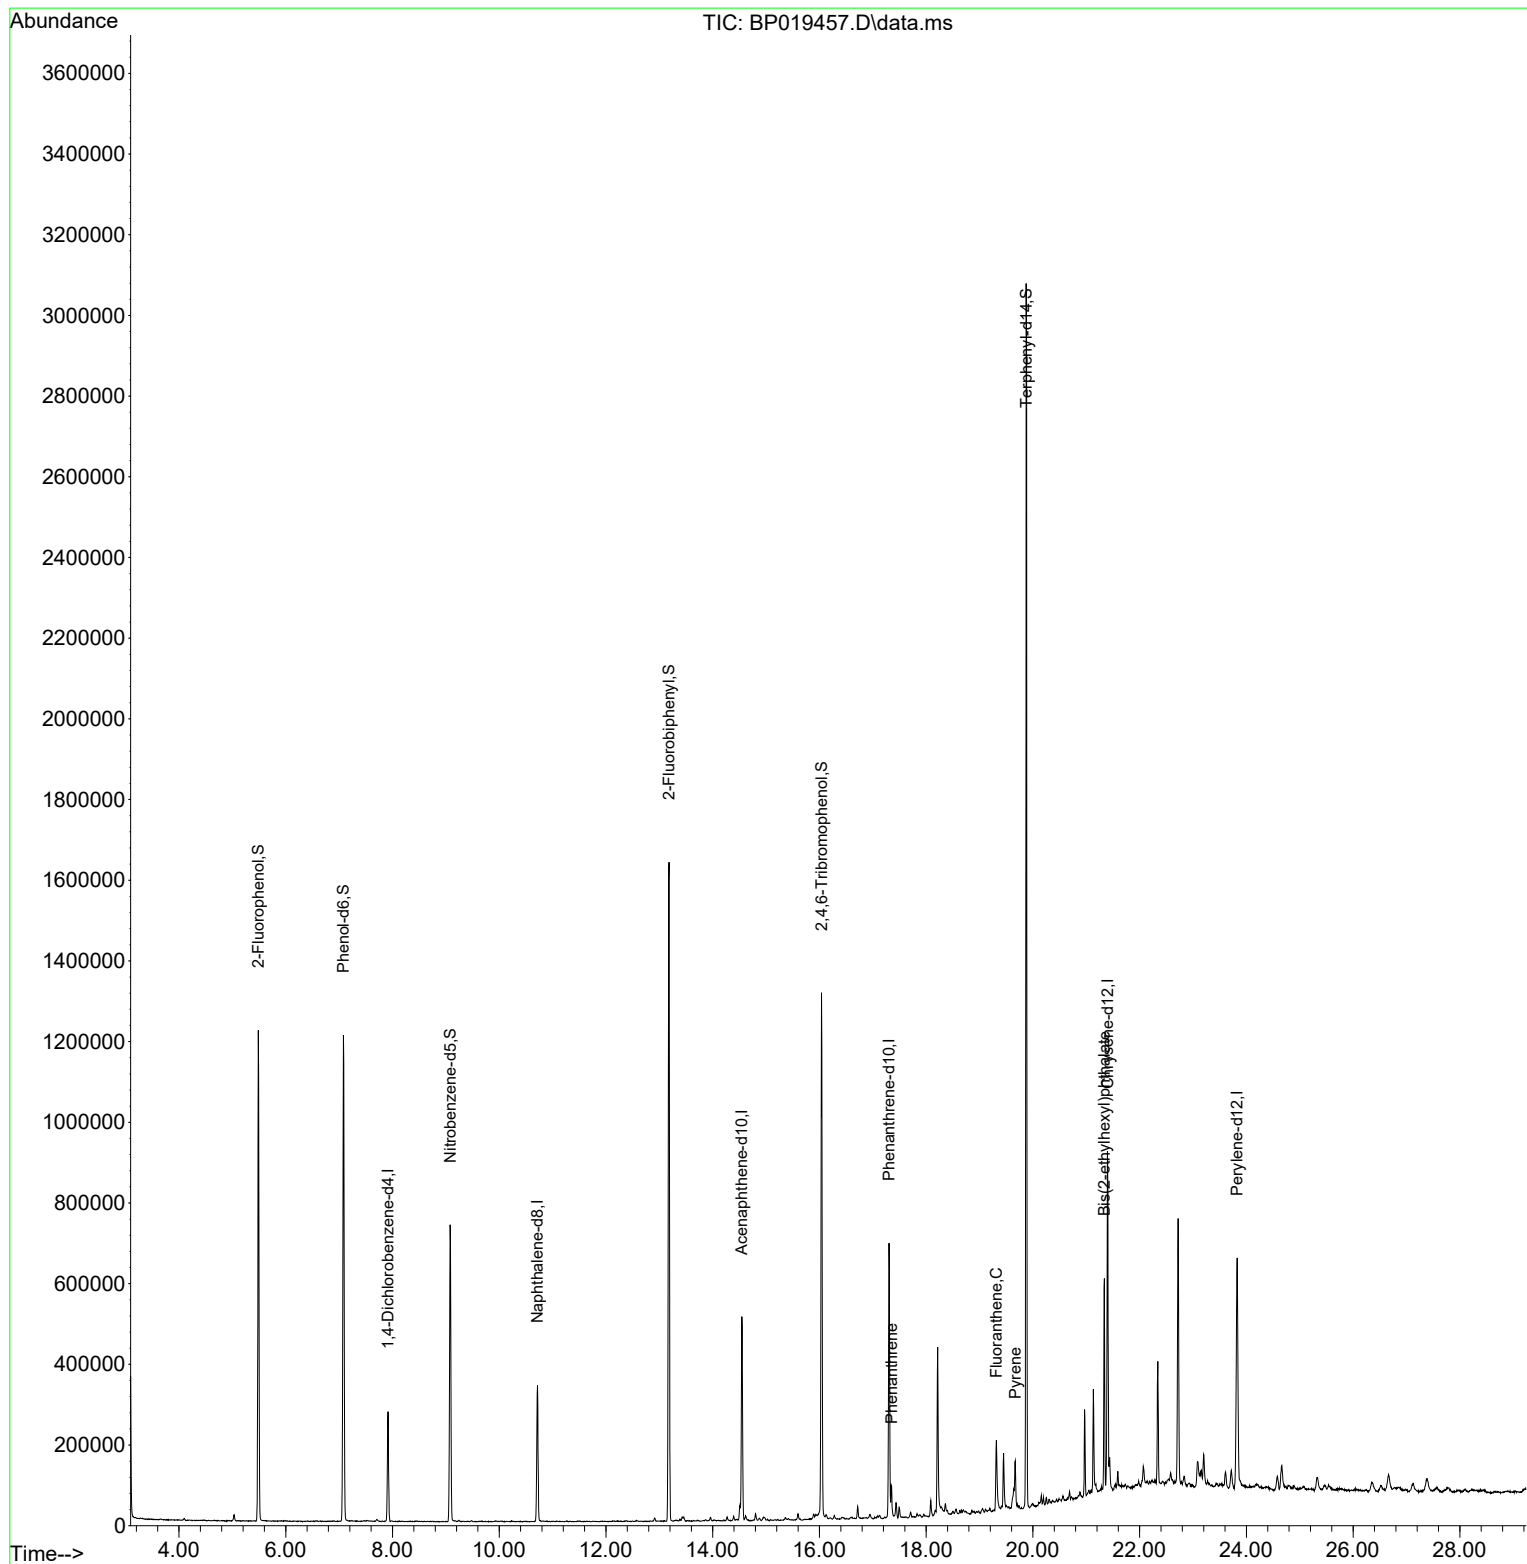




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.916 min Scan# 81
Delta R.T. -0.012 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44




Instrument :
BNA_P
ClientSampleId :
72-11985


Tgt Ion:152 Resp: 65977
Ion Ratio Lower Upper
152 100
150 161.0 123.5 185.3
115 69.7 55.1 82.7

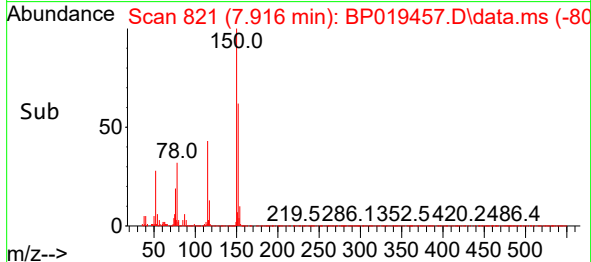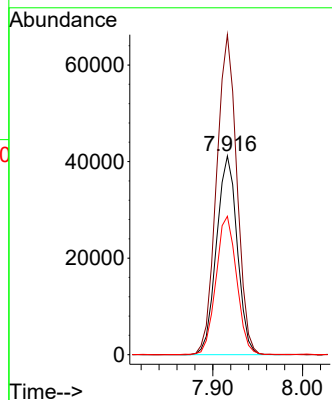

#5
2-Fluorophenol
Concen: 107.350 ng
RT: 5.487 min Scan# 408
Delta R.T. -0.012 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44

Tgt Ion:112 Resp: 450196
Ion Ratio Lower Upper
112 100
64 66.9 53.1 79.7
63 38.4 29.4 44.0


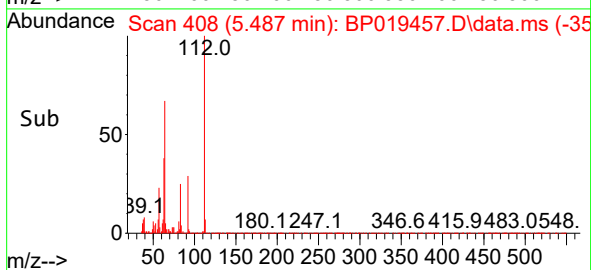
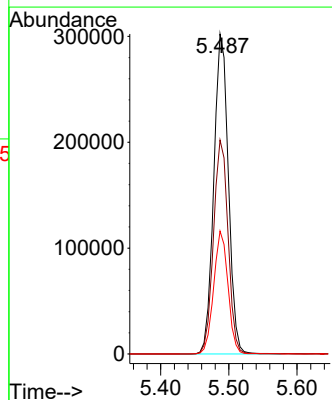
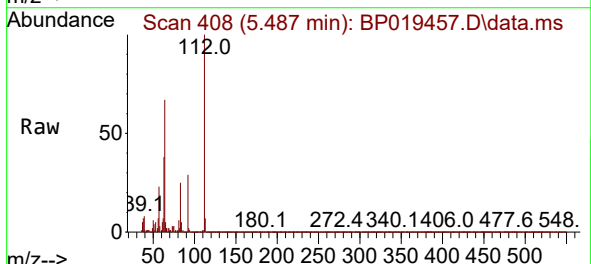




#7
Phenol-d6
Concen: 99.267 ng
RT: 7.081 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44




Instrument :
BNA_P
ClientSampleId :
72-11985


Tgt Ion: 99 Resp: 614923
Ion Ratio Lower Upper
99 100
42 21.7 16.4 24.6
71 44.8 34.6 52.0

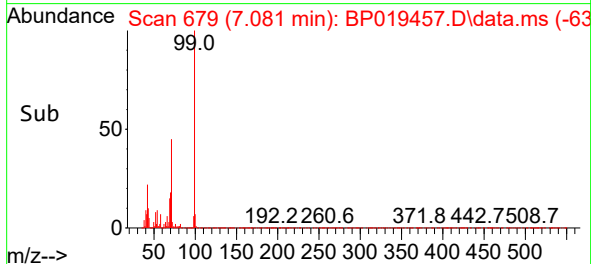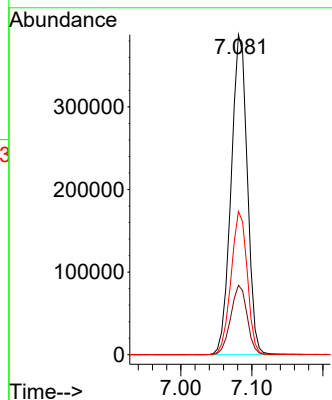

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.716 min Scan# 1297
Delta R.T. -0.012 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44

Tgt Ion: 136 Resp: 262656
Ion Ratio Lower Upper
136 100
137 10.4 8.8 13.2
54 9.3 7.8 11.6
68 5.9 5.2 7.8


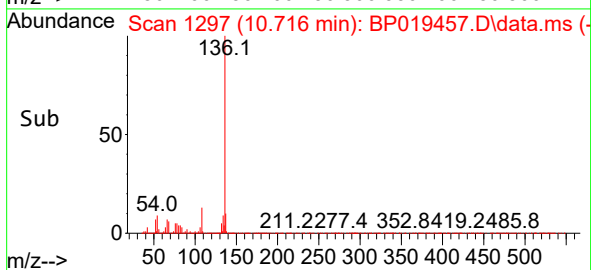
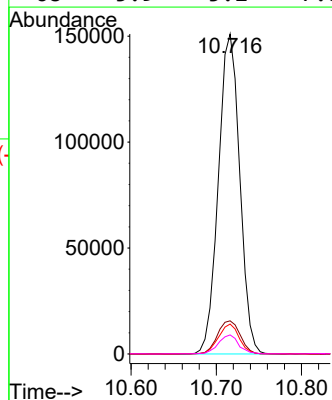
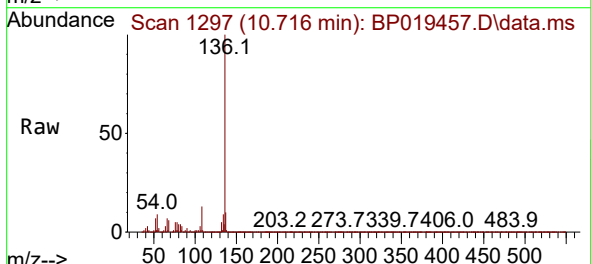




#23
Nitrobenzene-d5
Concen: 70.471 ng
RT: 9.081 min Scan# 1019
Delta R.T. -0.018 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44




Instrument :
BNA_P
ClientSampleId :
72-11985


Tgt Ion: 82 Resp: 410985
Ion Ratio Lower Upper
82 100
128 35.9 28.2 42.2
54 53.5 41.1 61.7

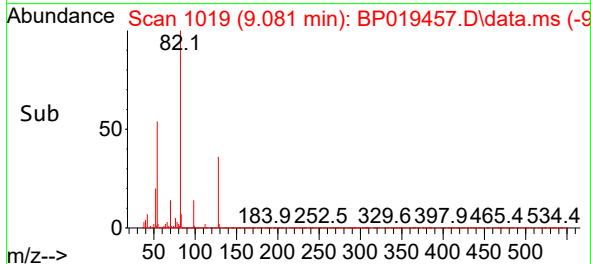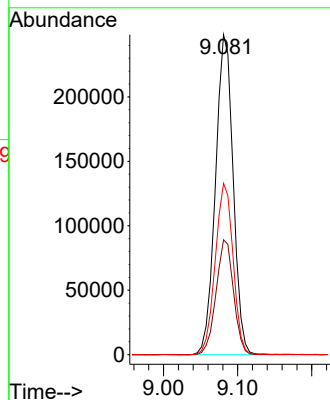

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.545 min Scan# 1948
Delta R.T. -0.012 min
Lab File: BP019457.D
Acq: 26 Jan 2024 20:44

Tgt Ion: 164 Resp: 170795
Ion Ratio Lower Upper
164 100
162 104.0 80.8 121.2
160 45.0 35.0 52.6

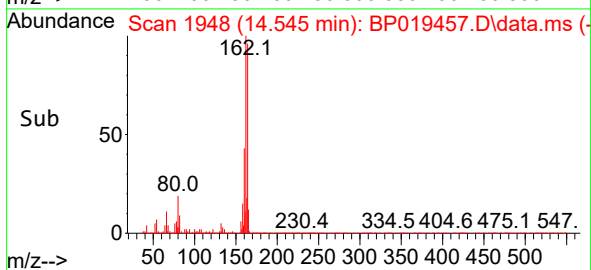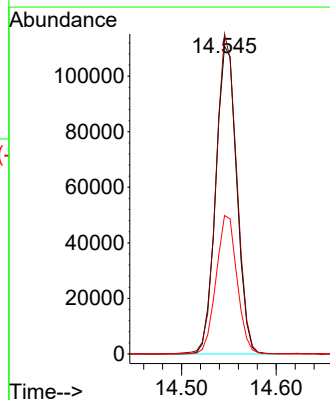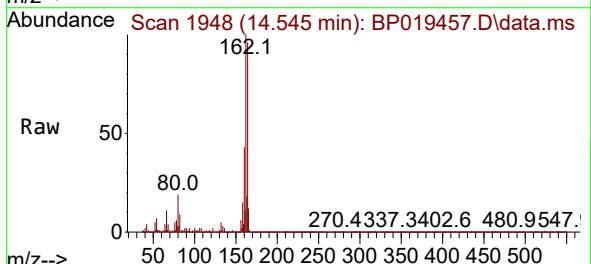



#42

2,4,6-Tribromophenol

Concen: 95.396 ng

RT: 16.039 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Instrument :

BNA_P

ClientSampleId :

72-11985





Tgt Ion:330 Resp: 211000

Ion Ratio Lower Upper

330 100

332 96.9 77.1 115.7

141 39.8 30.9 46.3

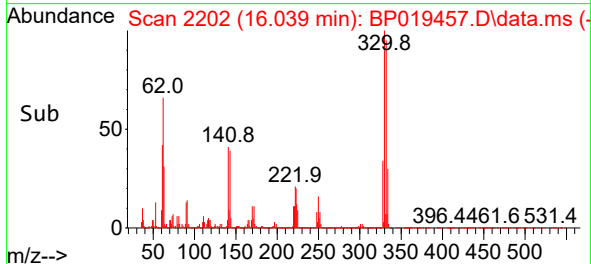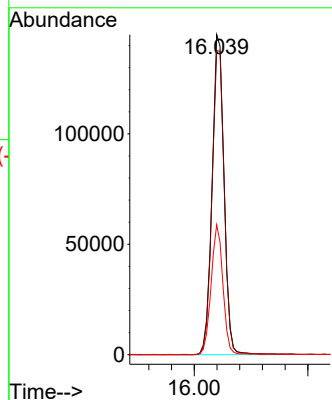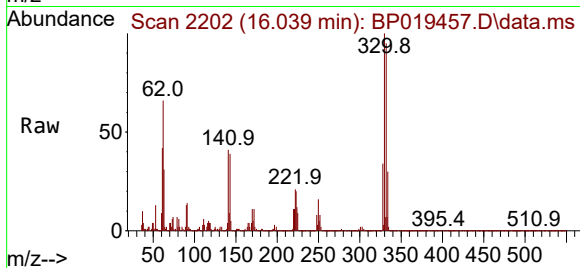

#45

2-Fluorobiphenyl

Concen: 63.710 ng

RT: 13.181 min Scan# 1716

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44




Tgt Ion:172 Resp: 820984


Ion Ratio Lower Upper

172 100

171 34.3 27.9 41.9

170 23.7 18.7 28.1

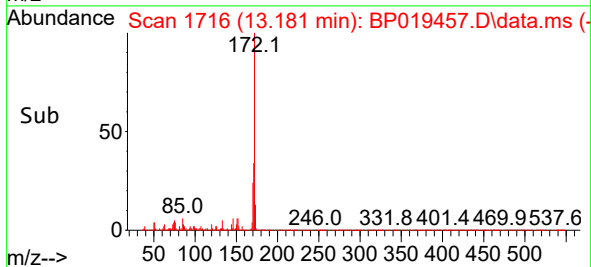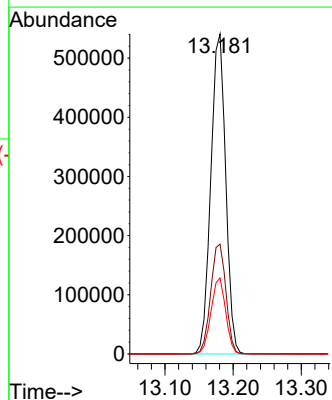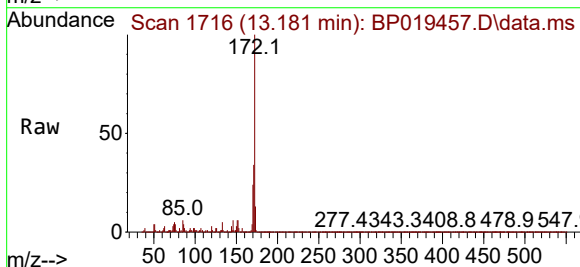



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.304 min Scan# 2419

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Instrument :

BNA_P

ClientSampleId :

72-11985





Tgt Ion:188 Resp: 390669

Ion Ratio Lower Upper

188 100

94 8.3 6.2 9.2

80 9.6 8.1 12.1

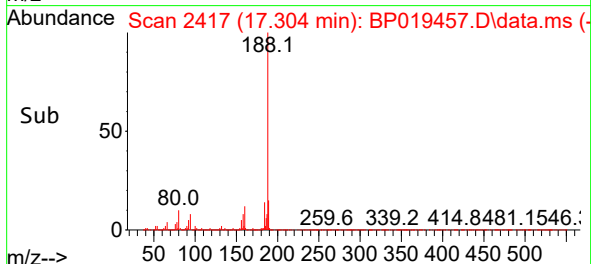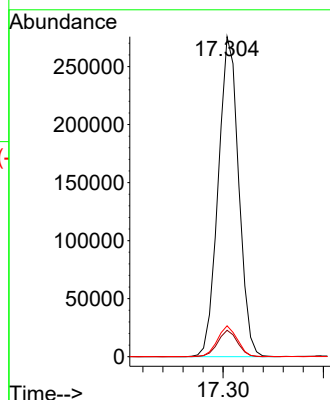

#71

Phenanthrene

Concen: 2.250 ng

RT: 17.351 min Scan# 2425

Delta R.T. -0.006 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44




Tgt Ion:178 Resp: 46781


Ion Ratio Lower Upper

178 100

176 19.4 15.0 22.4

179 15.3 12.2 18.4

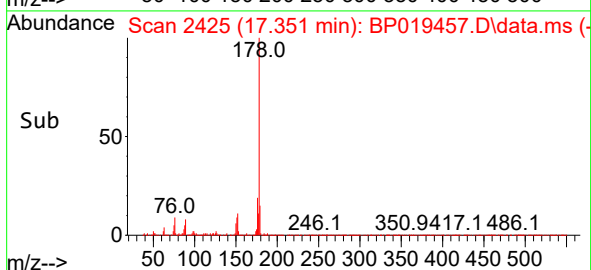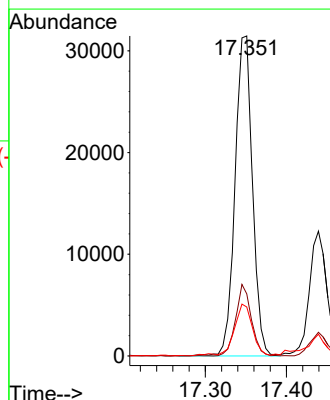



#75

Fluoranthene

Concen: 3.184 ng

RT: 19.316 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Instrument :

BNA_P

ClientSampleId :

72-11985





Tgt Ion:202 Resp: 86074

Ion Ratio Lower Upper

202 100

101 9.2 0.0 29.1

203 17.1 0.0 37.0

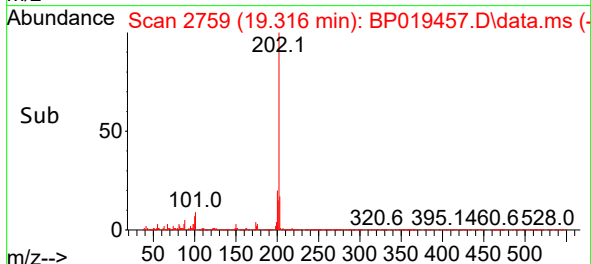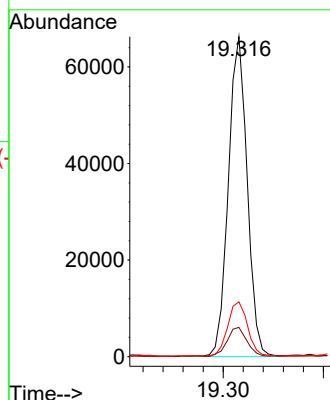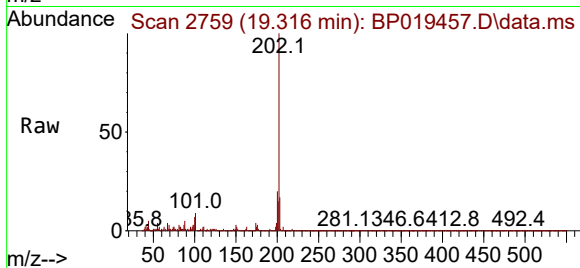

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.398 min Scan# 3113

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44




Tgt Ion:240 Resp: 386243


Ion Ratio Lower Upper

240 100

120 8.2 6.9 10.3

236 26.2 19.8 29.8

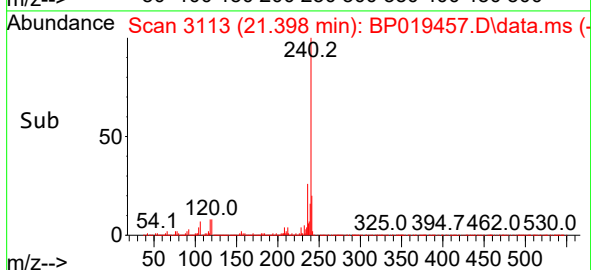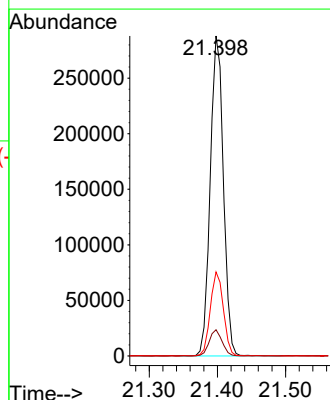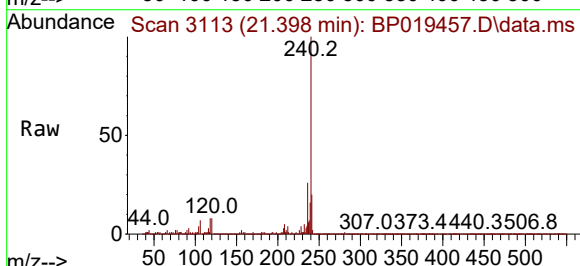



#78

Pyrene

Concen: 2.604 ng

RT: 19.669 min Scan# 2819

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Instrument :

BNA_P

ClientSampleId :

72-11985





Tgt Ion:202 Resp: 72706

Ion Ratio Lower Upper

202 100

200 20.3 16.5 24.7

203 17.0 13.9 20.9

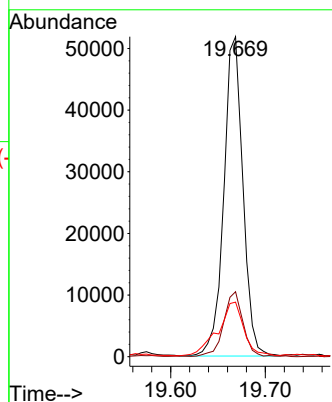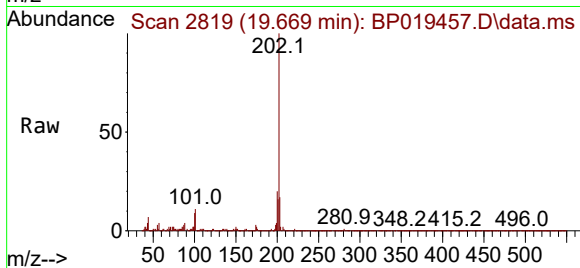

#79

Terphenyl-d14

Concen: 59.629 ng

RT: 19.874 min Scan# 2854

Delta R.T. -0.012 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44




Tgt Ion:244 Resp: 1404758


Ion Ratio Lower Upper

244 100

212 7.8 5.8 8.8

122 9.0 6.6 10.0

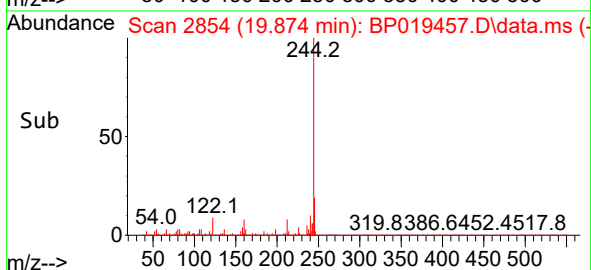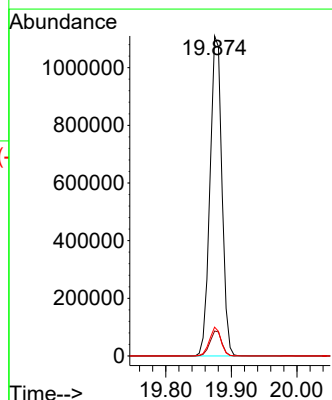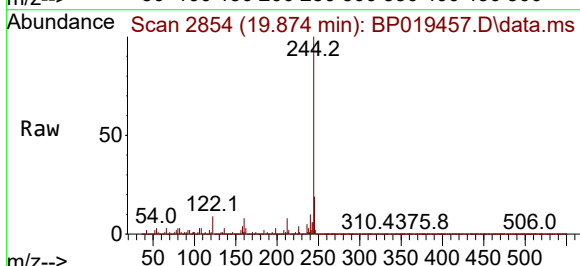



#84

Bis(2-ethylhexyl)phthalate

Concen: 9.847 ng

RT: 21.339 min Scan# 3104

Delta R.T. -0.006 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Instrument :

BNA_P

ClientSampleId :

72-11985





Tgt Ion:149 Resp: 172914

Ion Ratio Lower Upper

149 100

167 27.5 22.0 33.0

279 4.8 3.7 5.5

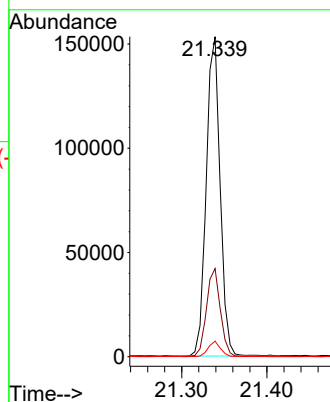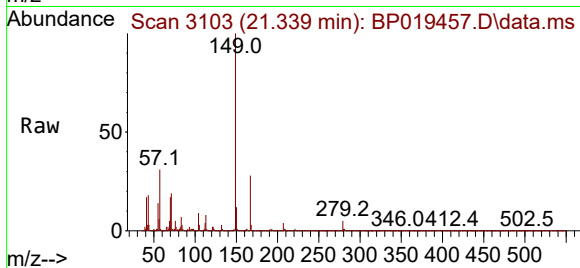

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.827 min Scan# 3526

Delta R.T. -0.018 min

Lab File: BP019457.D

Acq: 26 Jan 2024 20:44

Tgt Ion:264 Resp: 439967

Ion Ratio Lower Upper

264 100

260 23.9 18.6 28.0

265 20.8 16.4 24.6

