

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019452.D
Acq On : 26 Jan 2024 16:00
Operator : MA/JU
Sample : PB158491BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158491BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	403	410	421	rBV	1605055	2354547	36.18%	8.729%
2	7.092	672	681	691	rBV	1627763	2584989	39.72%	9.584%
3	7.922	815	822	831	rBV	344932	555649	8.54%	2.060%
4	9.092	1011	1021	1029	rBV	962148	1608898	24.72%	5.965%
5	10.722	1291	1298	1309	rVB	463380	783530	12.04%	2.905%
6	13.186	1708	1717	1725	rBV	2570463	3836735	58.96%	14.224%
7	14.557	1942	1950	1957	rBV	719825	1145959	17.61%	4.249%
8	16.045	2196	2203	2221	rBV	2053491	3018002	46.38%	11.189%
9	17.310	2411	2418	2425	rBV	1036719	1491570	22.92%	5.530%
10	19.886	2849	2856	2861	rBV	5101597	6507311	100.00%	24.125%
11	21.404	3109	3114	3121	rBV	1223489	1599056	24.57%	5.928%
12	23.833	3519	3527	3536	rVB	714469	1486851	22.85%	5.512%




Sum of corrected areas: 26973097

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019452.D
Acq On : 26 Jan 2024 16:00
Operator : MA/JU
Sample : PB158491BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158491BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

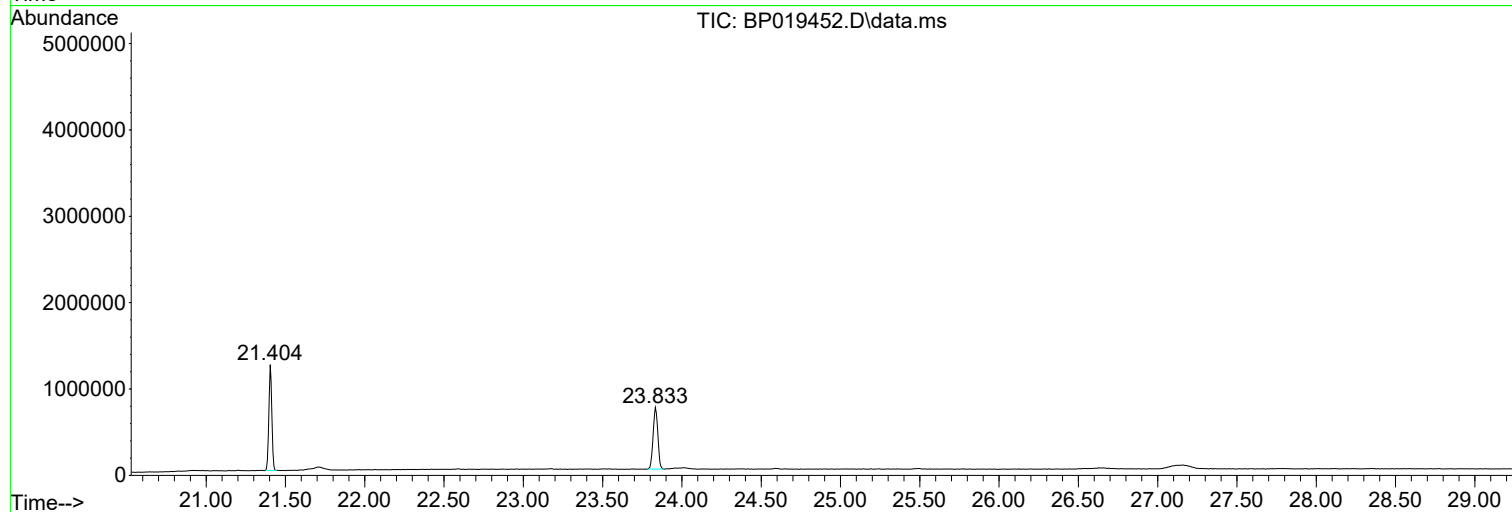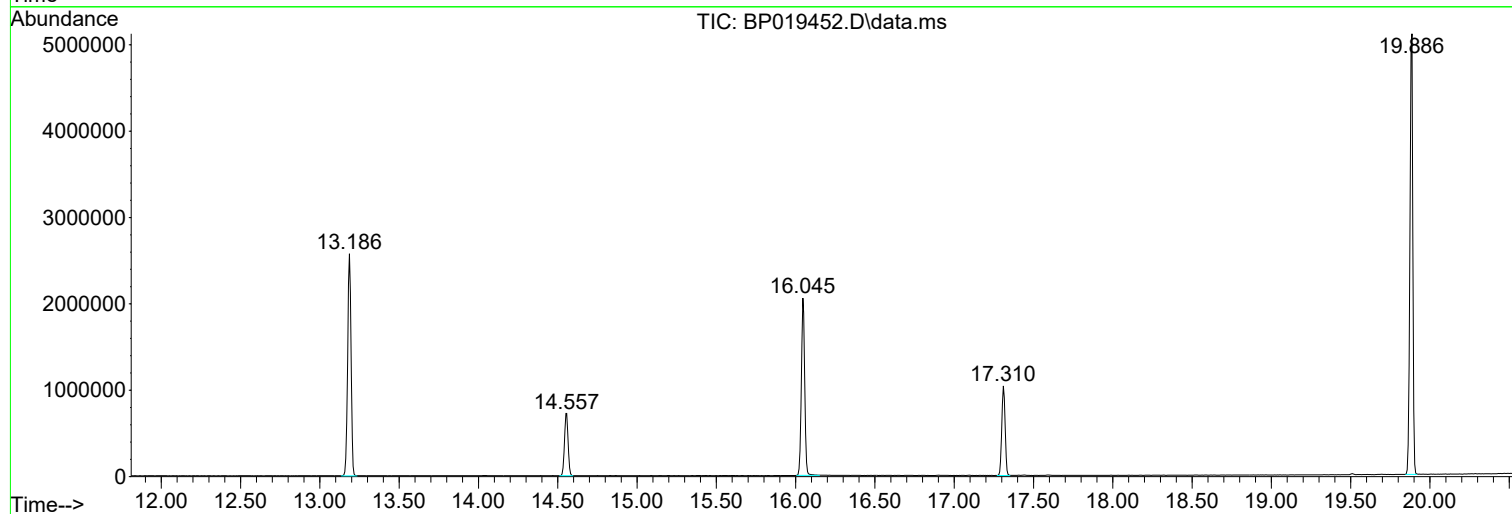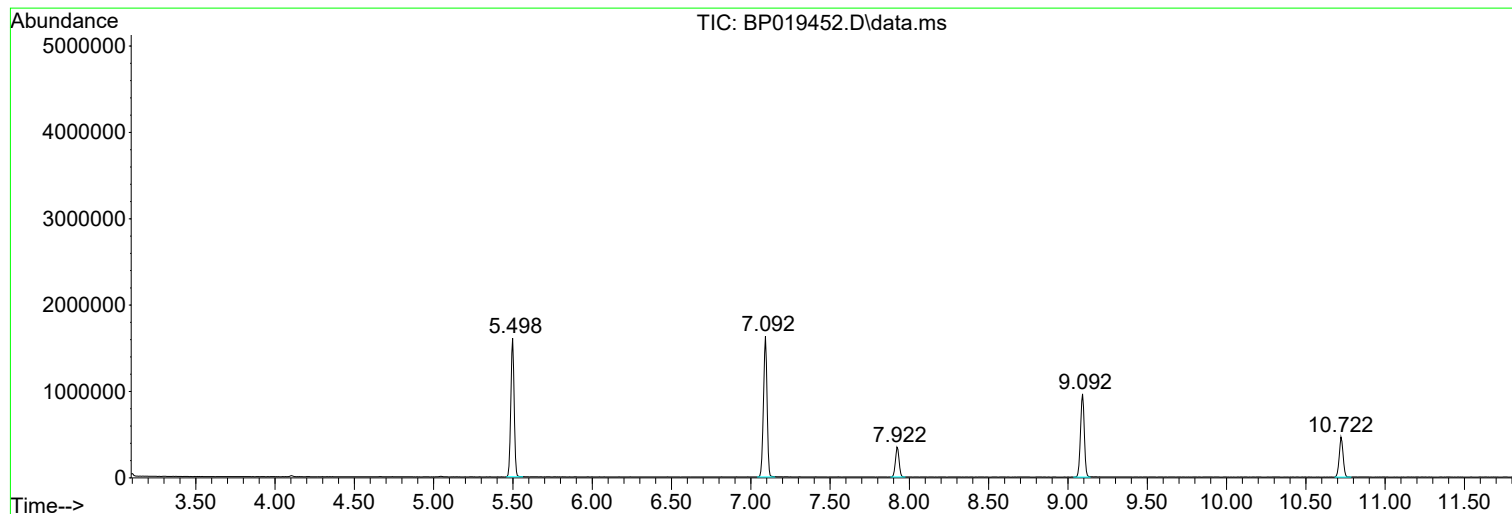

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019452.D
Acq On : 26 Jan 2024 16:00
Operator : MA/JU
Sample : PB158491BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158491BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019452.D
Acq On : 26 Jan 2024 16:00
Operator : MA/JU
Sample : PB158491BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158491BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------