
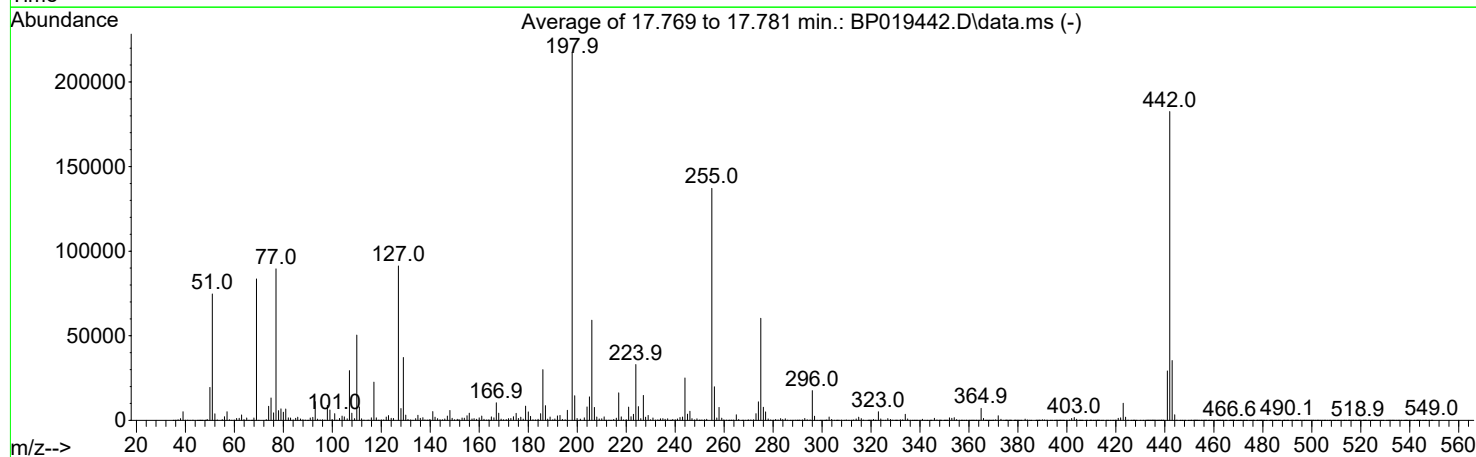


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019442.D
Acq On : 26 Jan 2024 10:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 26 23:43:31 2024

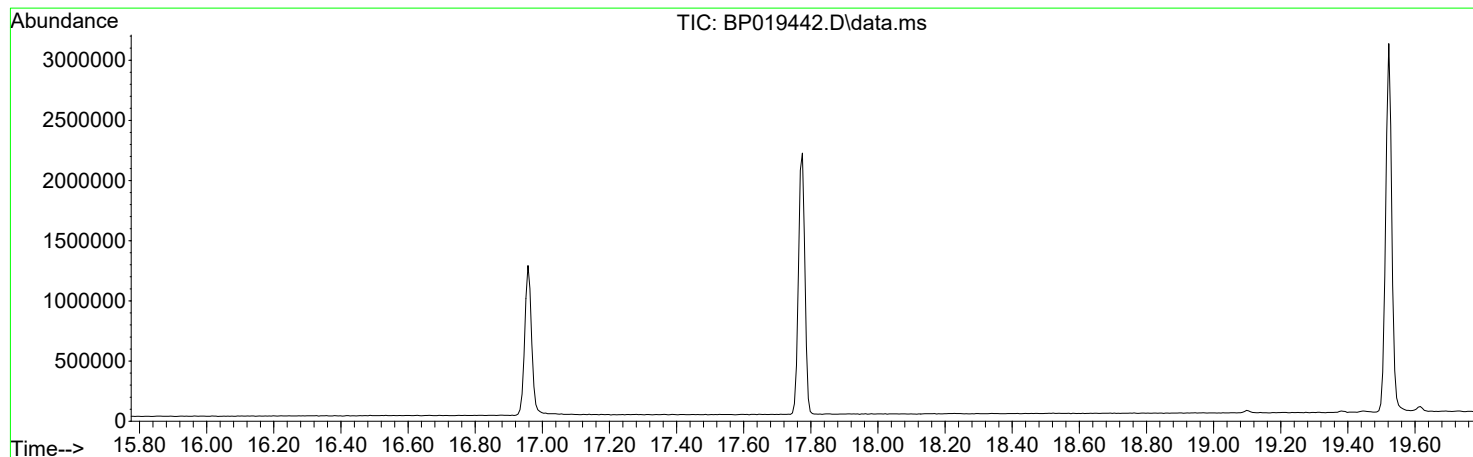

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	34.4	74731	PASS
68	69	0.00	2	1.7	1442	PASS
69	198	0.00	100	38.5	83643	PASS
70	69	0.00	2	0.1	122	PASS
127	198	10	80	42.0	91284	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	217431	PASS
199	198	5	9	6.7	14572	PASS
275	198	10	60	27.7	60308	PASS
365	198	1	100	3.3	7138	PASS
441	198	0.01	100	13.4	29213	PASS
442	442	100	100	100.0	182558	PASS
443	442	15	24	19.4	35387	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/26/2024	BNA_P	<u>BP019442.D</u>
Compound Name	Response	Retention Time
DDT	681656	20.727
DDD	6415	20.345
DDE	0	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6415	688071	0.93

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019442.D
Acq On : 26 Jan 2024 10:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 29 00:23:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 23:43:31 2024
Response via : Initial Calibration

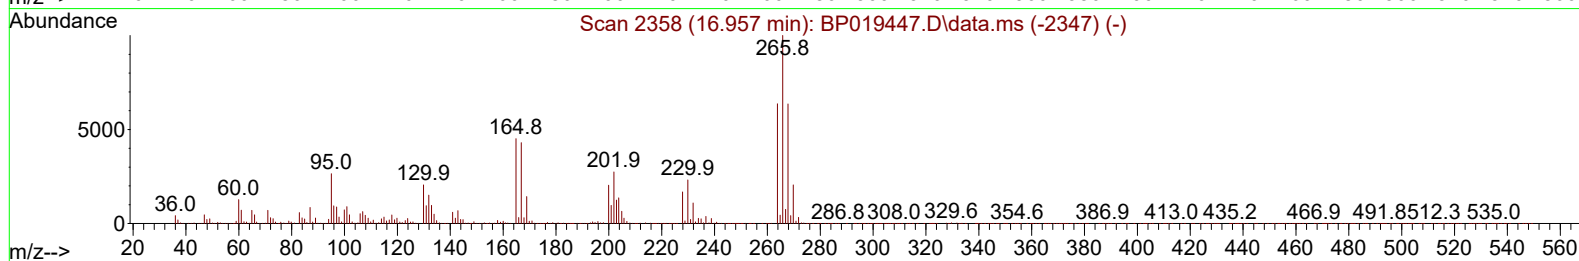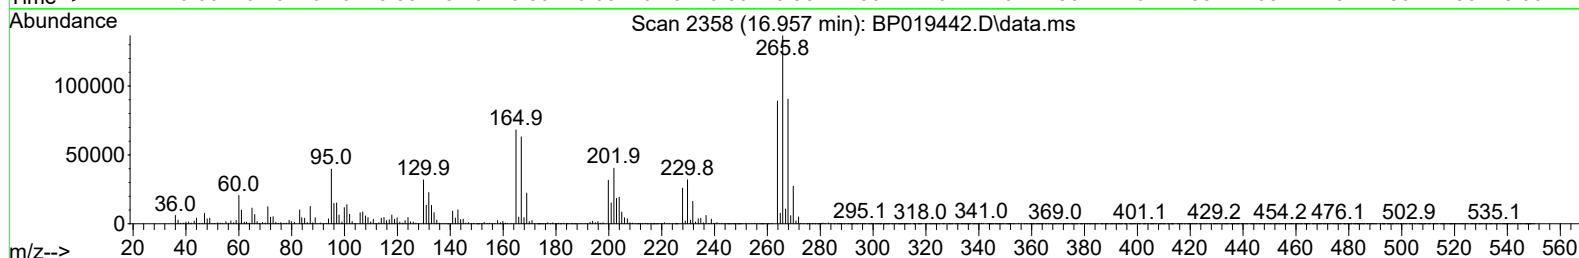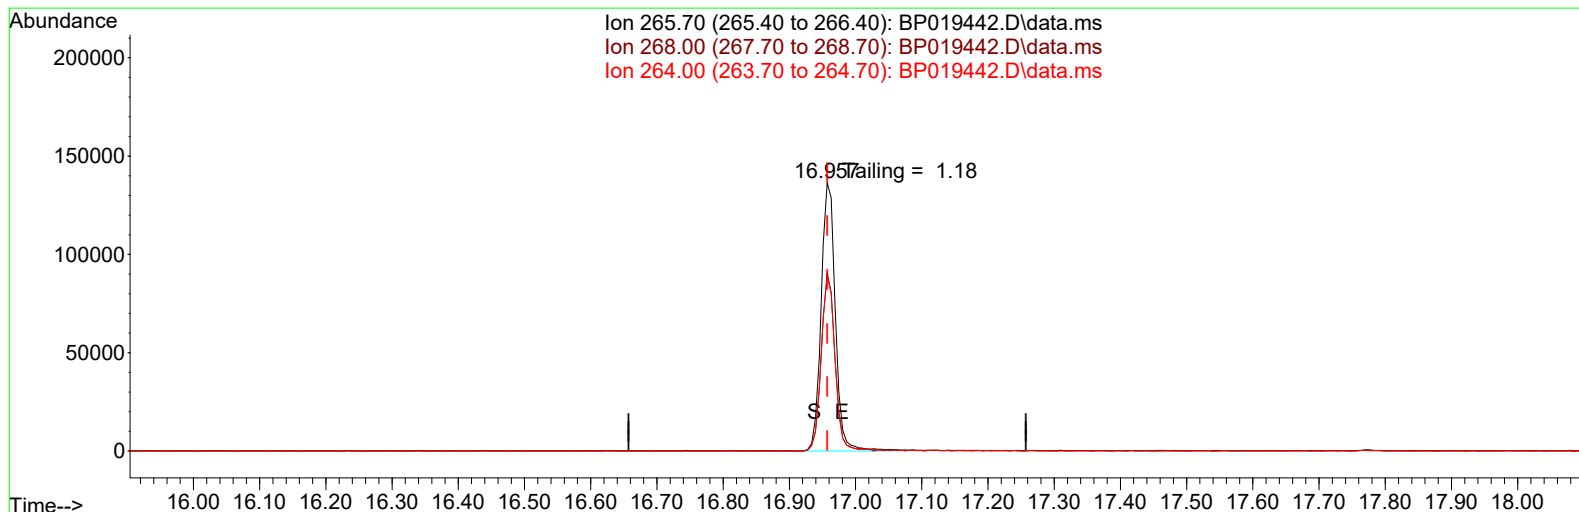

TIC: BP019442.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.000) 1531485.39 ng




response 203799

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	66.33
264.00	63.70	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012624\
Data File : BP019442.D
Acq On : 26 Jan 2024 10:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 29 00:23:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 23:43:31 2024
Response via : Initial Calibration

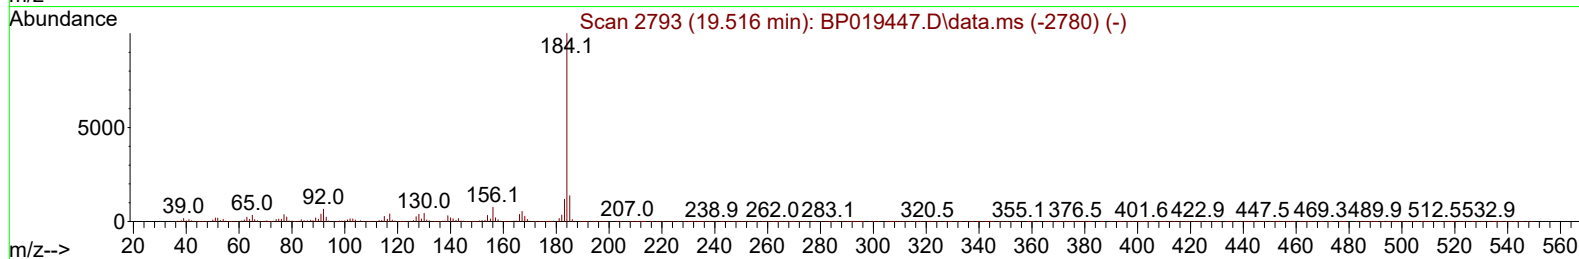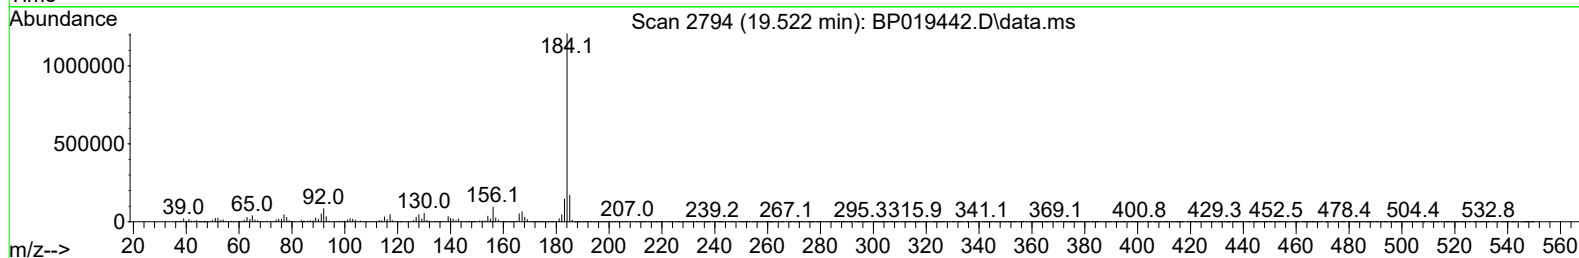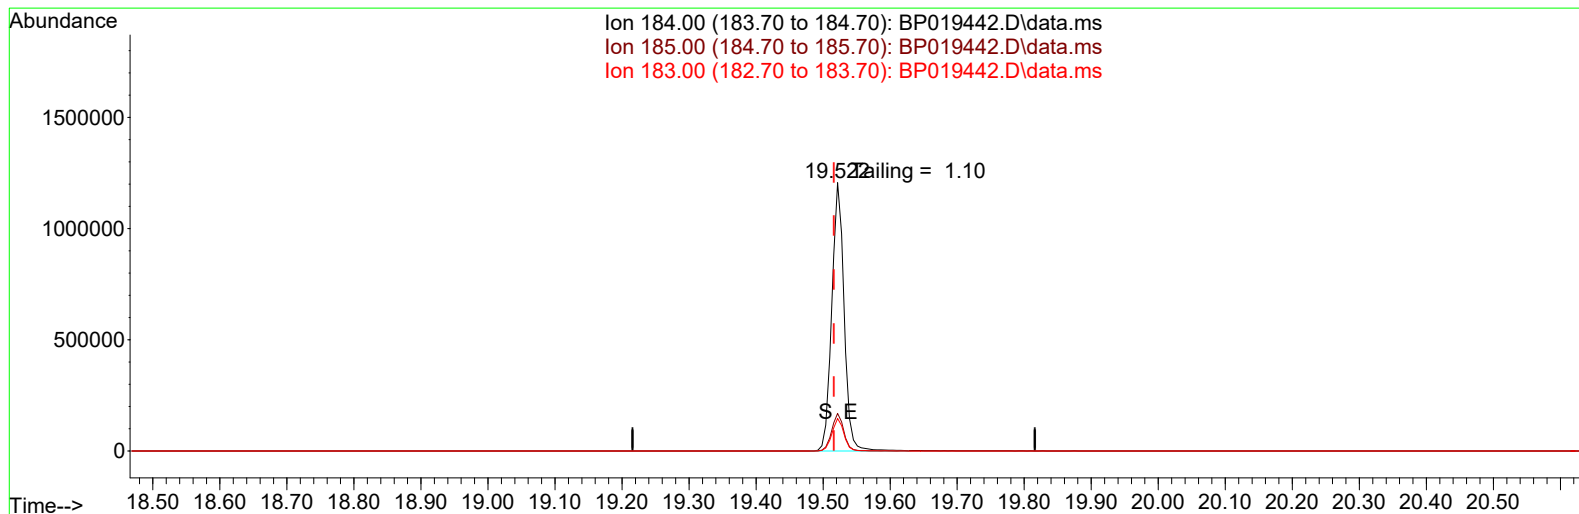

TIC: BP019442.D\data.ms

(77) Benzidine

19.522min (+ 0.006) 636000.23 ng

response 1542458

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	11.80	12.12
0.00	0.00	0.00