


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012720\
 Data File : BP001689.D
 Acq On : 27 Jan 2020 12:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 24 22:23:46 2020

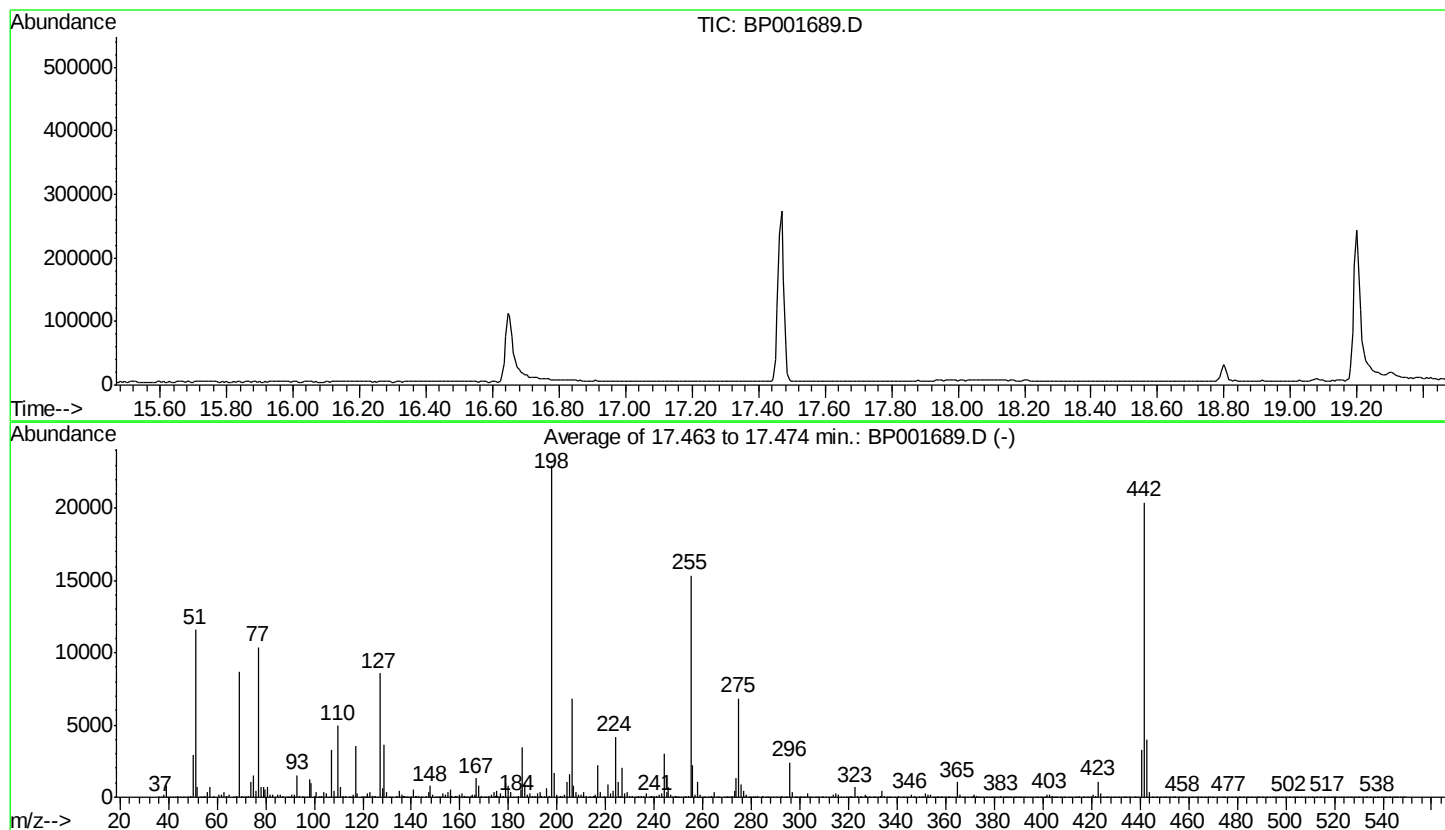

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	11599	PASS
68	69	0.00	2	1.1	97	PASS
69	198	0.00	100	38.0	8724	PASS
70	69	0.00	2	0.7	59	PASS
127	198	10	80	37.3	8573	PASS
197	198	0.00	2	0.1	16	PASS
198	198	100	100	100.0	22960	PASS
199	198	5	9	7.2	1660	PASS
275	198	10	60	29.8	6834	PASS
365	198	1	100	4.6	1061	PASS
441	198	0.01	100	14.2	3249	PASS
442	198	50	100	88.9	20408	PASS
443	442	15	24	19.7	4015	PASS