

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012721\
 Data File : BP004636.D
 Acq On : 26 Jan 2021 17:32
 Operator : CG/JU
 Sample : SSTD02079
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079

Quant Time: Jan 27 04:13:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP012721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 27 04:11:03 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	43536	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	162255	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	133542	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.19	188	330661	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	356644	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	337239	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	6806	6.50	ng/uL	0.00
5) Phenol-d5	6.96	99	59640	15.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	34894	16.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	44392	14.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	46639	15.49	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	20545	14.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	26548	17.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	61338	21.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	57242	17.78	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	196673	18.40	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	233884	17.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	28082	14.54	ng/ul	0.00
58) Fluorene-d10	15.43	176	175743	18.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	37069	17.38	ng/ul	0.00
71) Anthracene-d10	17.29	188	291364	17.84	ng/ul	0.00
79) Pyrene-d10	19.53	212	349811	18.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	339742	18.29	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.30	88	7276	6.801	ng/uL 100
4) Benzaldehyde	6.93	77	45077	24.296	ng/ul 100
6) Phenol	6.98	94	62440	16.420	ng/ul 100
8) Bis(2-Chloroethyl)ether	7.22	93	45726	15.025	ng/ul 100
10) 2-Chlorophenol	7.36	128	45179	14.615	ng/ul 100
11) 2-Methylphenol	8.23	108	48377	16.627	ng/ul 100
12) 2,2'-oxybis(1-Chloropropan	8.32	45	26909	7.841	ng/ul 98
14) Acetophenone	8.62	105	81194	18.386	ng/ul 100
15) N-Nitroso-di-n-propylamine	8.60	70	44775	20.055	ng/ul 100
16) 4-Methylphenol	8.56	108	51296	16.497	ng/ul 100
17) Hexachloroethane	8.87	117	22042	16.600	ng/ul 100
20) Nitrobenzene	8.99	77	68493	21.180	ng/ul 100
21) Isophorone	9.52	82	118760	19.651	ng/ul 100
23) 2-Nitrophenol	9.70	139	26342	16.477	ng/ul 100
24) 2,4-Dimethylphenol	9.76	107	65195	21.661	ng/ul 100
25) Bis(2-Chloroethoxy)methane	10.00	93	63731	16.881	ng/ul 100
27) 2,4-Dichlorophenol	10.23	162	59871	21.894	ng/ul 100
28) Naphthalene	10.63	128	154542	16.954	ng/ul 100
30) 4-Chloroaniline	10.75	127	60162	19.682	ng/ul 100
31) Hexachlorobutadiene	10.92	225	52471	26.956	ng/ul 100
32) Caprolactam	11.51	113	7500	8.418	ng/ul 100
33) 4-Chloro-3-methylphenol	11.87	107	59348	21.536	ng/ul 100
34) 2-Methylnaphthalene	12.25	142	125301	19.927	ng/ul 100

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP012721\
 Data File : BP004636.D
 Acq On : 26 Jan 2021 17:32
 Operator : CG/JU
 Sample : SSTD02079
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079

Quant Time: Jan 27 04:13:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP012721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 27 04:11:03 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.47	142	122608	16.750	ng/ul	100
37) 1,2,4,5-Tetrachlorobenzene	12.62	216	97097	20.414	ng/ul	100
38) Hexachlorocyclopentadiene	12.60	237	65039	23.939	ng/ul	100
39) 2,4,6-Trichlorophenol	12.86	196	58656	19.913	ng/ul	100
40) 2,4,5-Trichlorophenol	12.93	196	62525	20.097	ng/ul	100
41) 1,1'-Biphenyl	13.27	154	184165	16.882	ng/ul	100
42) 2-Chloronaphthalene	13.31	162	150608	17.301	ng/ul	100
43) 2-Nitroaniline	13.51	65	40439	18.354	ng/ul	100
45) Dimethylphthalate	13.90	163	196534	18.352	ng/ul	100
46) 2,6-Dinitrotoluene	14.01	165	38580	17.289	ng/ul	100
48) Acenaphthylene	14.16	152	207209	15.978	ng/ul	100
49) 3-Nitroaniline	14.34	138	29516	15.674	ng/ul	100
50) Acenaphthene	14.50	153	153087	16.849	ng/ul	100
51) 2,4-Dinitrophenol	14.54	184	24439	20.072	ng/ul	100
53) 4-Nitrophenol	14.65	109	37101	27.375	ng/ul	100
54) Dibenzofuran	14.84	168	237064	18.530	ng/ul	100
55) 2,4-Dinitrotoluene	14.80	165	54585	17.057	ng/ul	100
56) 2,3,4,6-Tetrachlorophenol	15.06	232	60793	22.089	ng/ul	100
57) Diethylphthalate	15.27	149	188931	17.935	ng/ul	100
59) Fluorene	15.49	166	197582	19.059	ng/ul	100
60) 4-Chlorophenyl-phenylether	15.49	204	120174	21.674	ng/ul	100
61) 4-Nitroaniline	15.50	138	34984	17.673	ng/ul	100
64) 4,6-Dinitro-2-methylphenol	15.56	198	38407	17.056	ng/ul	100
65) N-Nitrosodiphenylamine	15.70	169	172226	17.337	ng/ul	100
66) 4-Bromophenyl-phenylether	16.39	248	78680	19.655	ng/ul	100
67) Hexachlorobenzene	16.49	284	88993	19.161	ng/ul	100
68) Atrazine	16.66	200	77531	20.692	ng/ul	100
69) Pentachlorophenol	16.84	266	53144	21.759	ng/ul	100
70) Phenanthrene	17.23	178	334422	17.416	ng/ul	100
72) Anthracene	17.33	178	340769	17.720	ng/ul	100
73) 1,2,3,4-Tetrachlorobenzene	13.23	216	100087	18.696	ng/uL	100
74) Pentachlorobenzene	14.76	250	104398	19.686	ng/uL	100
75) Carbazole	17.60	167	285862	17.980	ng/ul	100
76) Di-n-butylphthalate	18.16	149	312562	15.650	ng/ul	100
77) Fluoranthene	19.20	202	427503	19.626	ng/ul	100
80) Pvrene	19.56	202	439350	18.090	ng/ul	100
81) Butylbenzylphthalate	20.44	149	132943	14.338	ng/ul	100
82) 3,3'-Dichlorobenzidine	21.20	252	152126	20.555	ng/ul	100
83) Benzo(a)anthracene	21.26	228	422334	17.570	ng/ul	100
84) Bis(2-ethylhexyl)phthalate	21.20	149	194427	14.176	ng/ul	100
85) Chrysene	21.31	228	406965	17.536	ng/ul	100
87) Di-n-octyl phthalate	22.10	149	311686	15.676	ng/ul	100
88) Benzo(b)fluoranthene	22.89	252	425294	19.335	ng/ul	100
89) Benzo(k)fluoranthene	22.94	252	405665	19.008	ng/ul	100
91) Benzo(a)pyrene	23.49	252	359013	17.695	ng/ul	100
92) Indeno(1,2,3-cd)pyrene	25.98	276	460107	17.948	ng/ul	100
93) Dibenzo(a,h)anthracene	26.00	278	388734	18.207	ng/ul	100
94) Benzo(a,h,i)perylene	26.71	276	376955	17.527	ng/ul	100


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012721\
Data File : BP004636.D
Acq On : 26 Jan 2021 17:32
Operator : CG/JU
Sample : SSTD02079
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD02079

Quant Time: Jan 27 04:13:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP012721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 27 04:11:03 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						

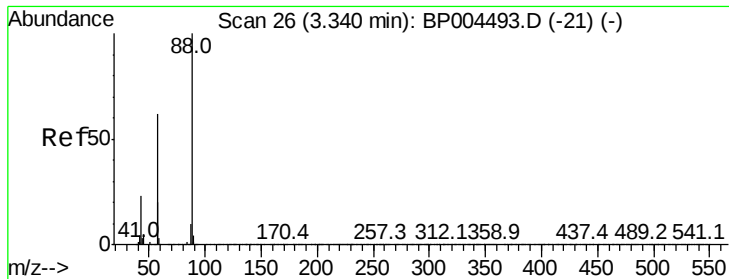

#2

1,4-Dioxane

Concen: 6.801 ng/uL

RT: 3.30 min Scan# 20

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079





Tot Ion: 88 Resp: 7276

Ion	Ratio	Lower	Upper
88	100		
43	41.2	33.0	49.4
58	65.0	52.0	78.0

88 100

43 41.2 33.0 49.4

58 65.0 52.0 78.0

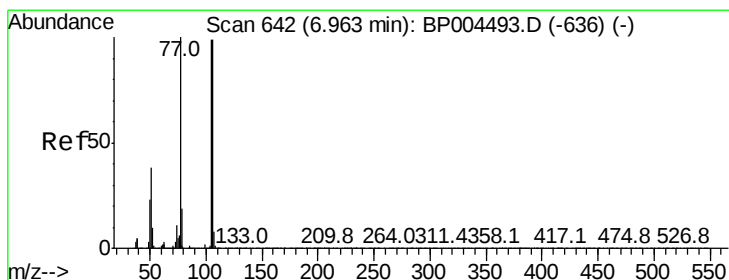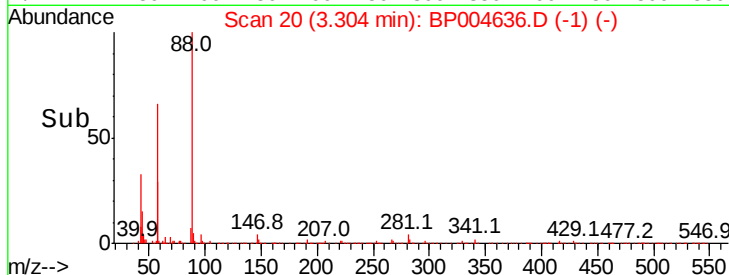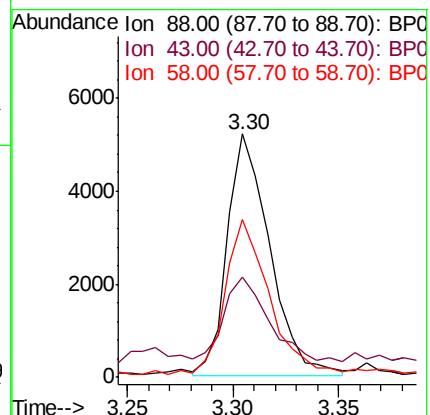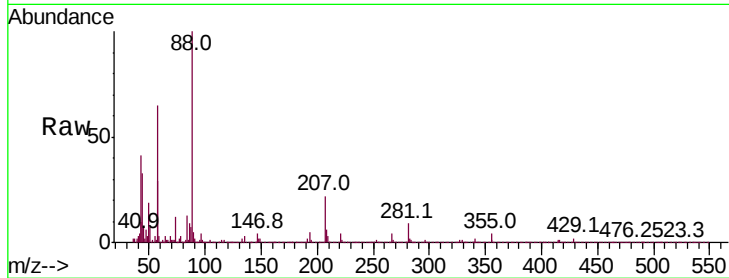

#4

Benzaldehyde

Concen: 24.296 ng/uL

RT: 6.93 min Scan# 637

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32




Tgt Ion: 77 Resp: 45077


Ion	Ratio	Lower	Upper
77	100		
105	83.4	66.7	100.1
106	77.1	61.7	92.5

77 100

105 83.4 66.7 100.1

106 77.1 61.7 92.5

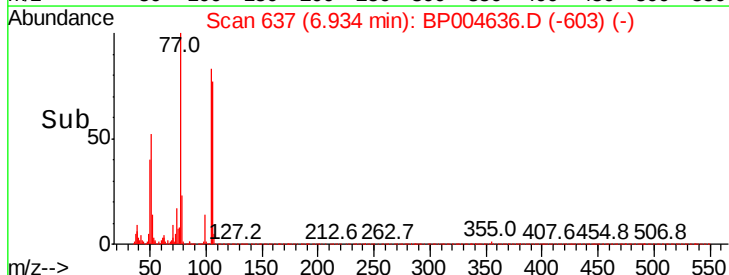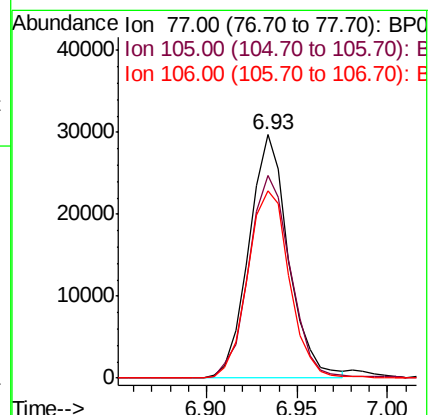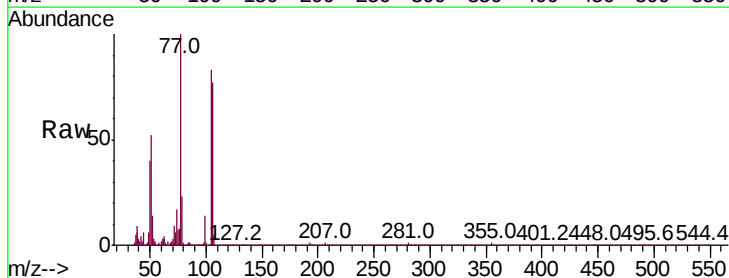



#6

Phenol

Concen: 16.420 ng/ul

RT: 6.98 min Scan# 645

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampled :

SSTD02079




Tot Ion: 94 Resp: 62440

Ion Ratio Lower Upper

94 100

65 37.6 30.1 45.1

66 58.0 46.4 69.6



#8

Bis(2-Chloroethyl)ether

Concen: 15.025 ng/ul

RT: 7.22 min Scan# 685

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32





Tgt Ion: 93 Resp: 45726


Ion Ratio Lower Upper

93 100

63 80.6 64.5 96.7

95 31.7 25.4 38.0





#10

2-Chlorophenol

Concen: 14.615 ng/ul

RT: 7.36 min Scan# 709

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:128 Resp: 45179

Ion Ratio Lower Upper

128 100

64 53.5 42.8 64.2




130 31.8 25.4 38.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 130.00 (129.70 to 130.70): E

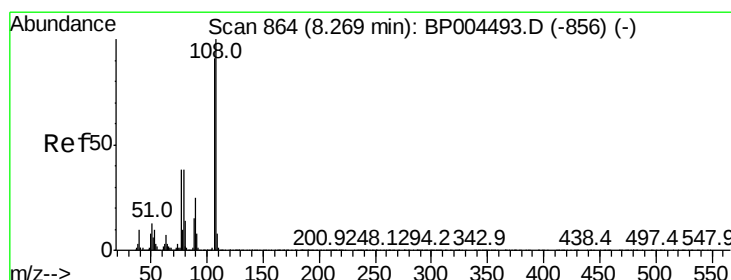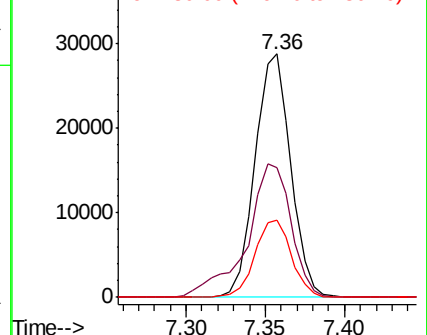

#11

2-Methylphenol

Concen: 16.627 ng/ul

RT: 8.23 min Scan# 858

Delta R.T. 0.00 min

Lab File: BP004636.D


Acq: 26 Jan 2021 17:32

Tgt Ion:108 Resp: 48377

Ion Ratio Lower Upper



108 100


107 92.9 74.3 111.5



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E




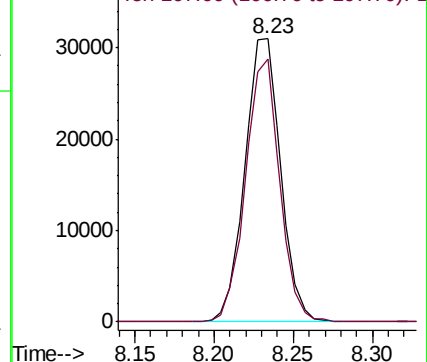




#12
2,2'-oxvbis(1-Chloropropane)
Concen: 7.841 ng/ul
RT: 8.32 min Scan# 872
Delta R.T. -0.01 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion: 45 Resp: 26909
Ion Ratio Lower Upper
45 100
77 18.0 15.5 23.3
79 14.4 12.1 18.1

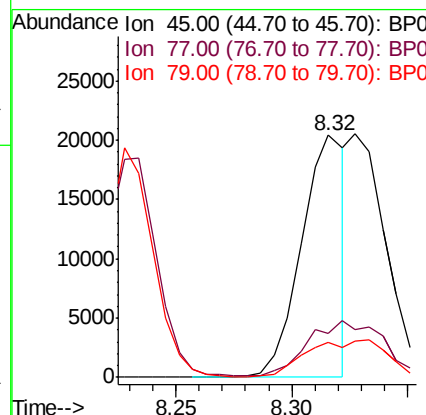

#14
Acetophenone
Concen: 18.386 ng/ul
RT: 8.62 min Scan# 923
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion: 105 Resp: 81194
Ion Ratio Lower Upper
105 100
77 88.8 71.0 106.6
51 32.9 26.3 39.5

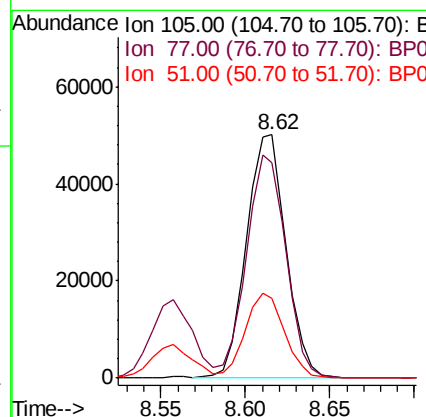







#15
N-Nitroso-di-n-propylamine
Concen: 20.055 ng/ul
RT: 8.60 min Scan# 920
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Instrument :
BNA_P
ClientSampleId :
SSTD02079

Tot Ion:	70	Resp:	44775
Ion	Ratio	Lower	Upper
70	100		
42	60.6	48.5	72.7
101	9.3	7.4	11.2
130	17.9	14.3	21.5




Abundance Ion 70.00 (69.70 to 70.70): BP0
Ion 42.00 (41.70 to 42.70): BP0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E


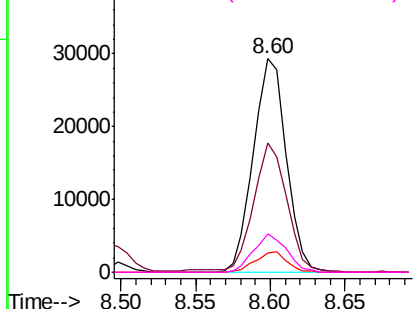



#16
4-Methylphenol
Concen: 16.497 ng/ul
RT: 8.56 min Scan# 913
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:	108	Resp:	51296
Ion	Ratio	Lower	Upper
108	100		
107	103.9	83.1	124.7



Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E



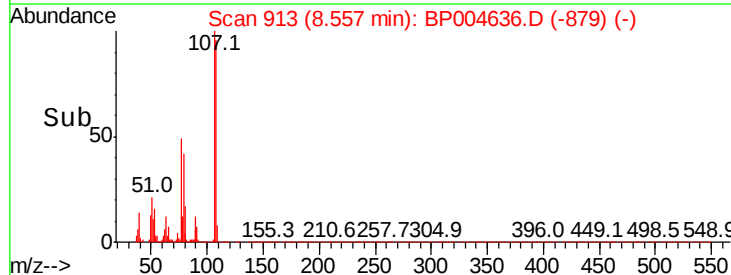
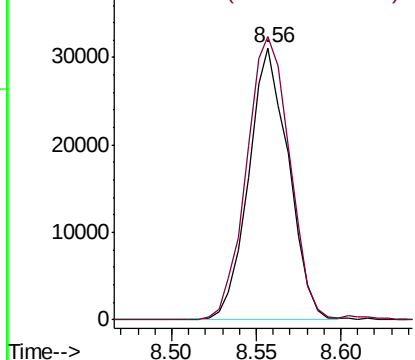




#17
Hexachloroethane
Concen: 16.600 ng/ul
RT: 8.87 min Scan# 966
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:117 Resp: 22042
Ion Ratio Lower Upper
117 100
201 137.2 109.8 164.6
199 88.3 70.6 106.0

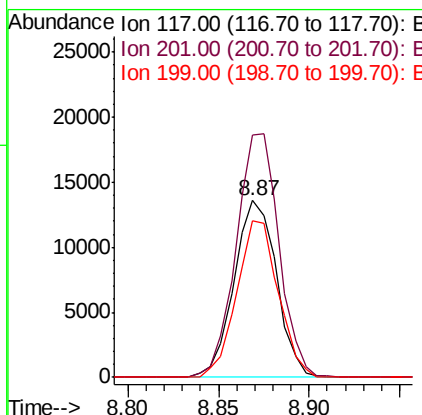

#20
Nitrobenzene
Concen: 21.180 ng/ul
RT: 8.99 min Scan# 986
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion: 77 Resp: 68493
Ion Ratio Lower Upper
77 100
123 36.0 28.8 43.2
65 15.9 12.7 19.1

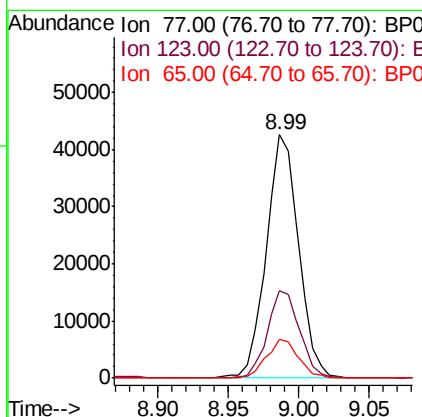



#21

Isophorone

Concen: 19.651 ng/ul

RT: 9.52 min Scan# 1076

Delta R.T. 0.00 min





Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :
BNA_P
ClientSampleId :
SSTD02079

Tot Ion: 82 Resp: 118760

Ion	Ratio	Lower	Upper
82	100		
95	9.9	7.9	11.9
138	16.8	13.4	20.2

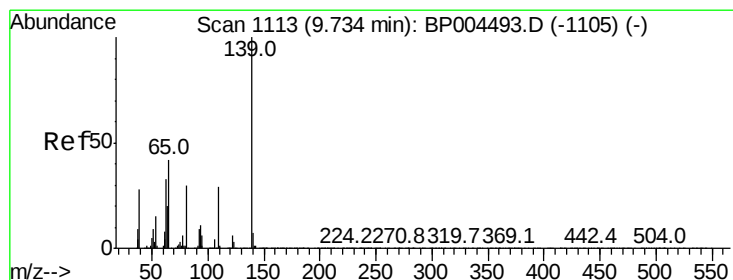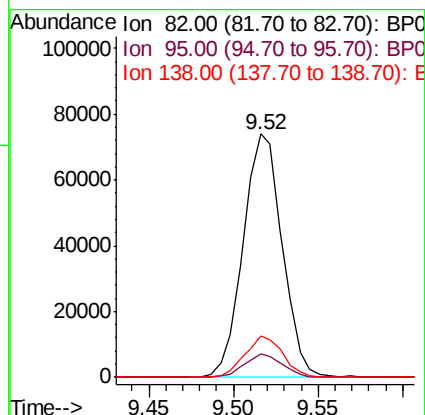

#23

2-Nitrophenol

Concen: 16.477 ng/ul

RT: 9.70 min Scan# 1107




Delta R.T. 0.00 min


Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Tgt Ion: 139 Resp: 26342

Ion	Ratio	Lower	Upper
139	100		
65	74.6	59.7	89.5
109	49.4	39.5	59.3



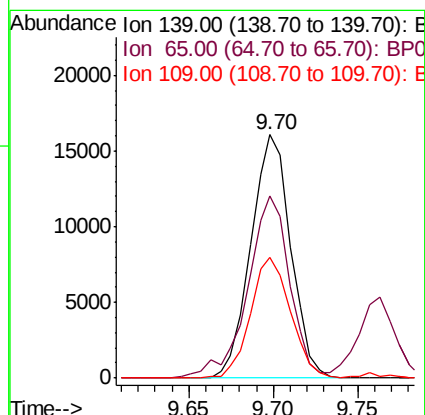
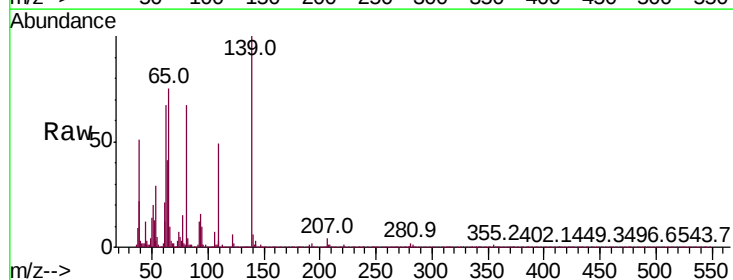




#24
2,4-Dimethylphenol
Concen: 21.661 ng/ul
RT: 9.76 min Scan# 1118
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion	Ratio	Lower	Upper
107	100		
121	43.4	34.7	52.1
122	70.7	56.6	84.8

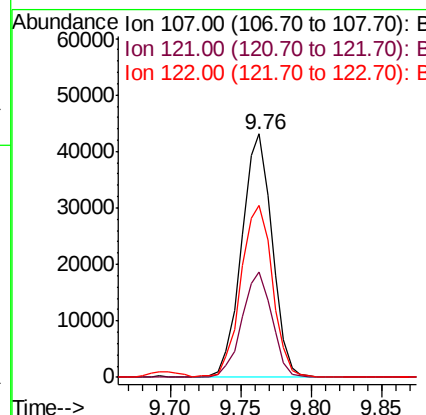

#25
Bis(2-Chloroethoxy)methane
Concen: 16.881 ng/ul
RT: 10.00 min Scan# 1159
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
93	100		
95	30.6	24.5	36.7
123	10.2	8.2	12.2

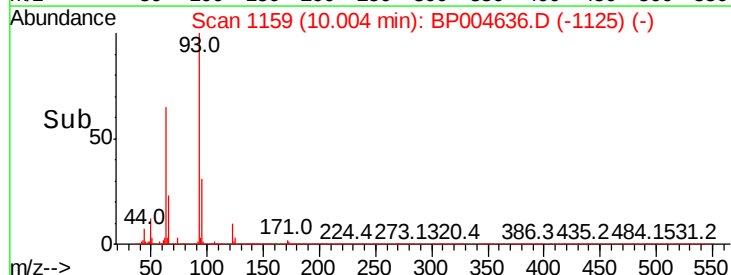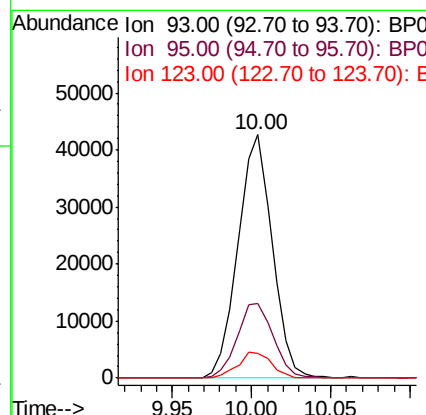



#27

2,4-Dichlorophenol

Concen: 21.894 ng/ul

RT: 10.23 min Scan# 1198

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:162 Resp: 59871

Ion Ratio Lower Upper

162 100

164 64.1 51.3 76.9




98 32.2 25.8 38.6



Abundance Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 98.00 (97.70 to 98.70): BP0

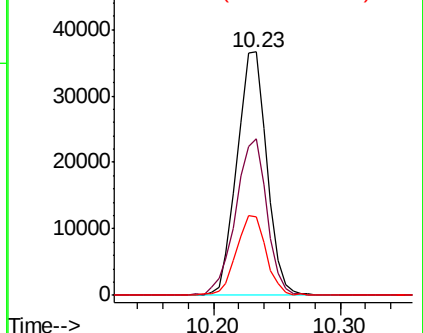

#28

Naphthalene

Concen: 16.954 ng/ul

RT: 10.63 min Scan# 1266

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:128 Resp: 154542

Ion Ratio Lower Upper

128 100

129 10.1 8.1 12.1



127 13.5 10.8 16.2




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E




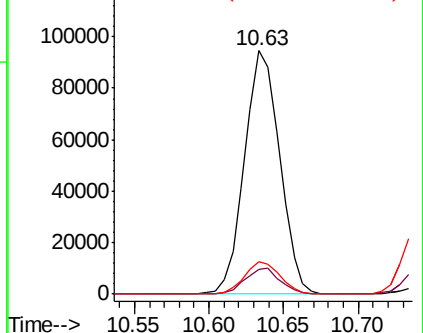




#30
4-Chloroaniline
Concen: 19.682 ng/ul
RT: 10.75 min Scan# 1285
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:127 Resp: 60162
Ion Ratio Lower Upper
127 100
129 31.8 25.4 38.2

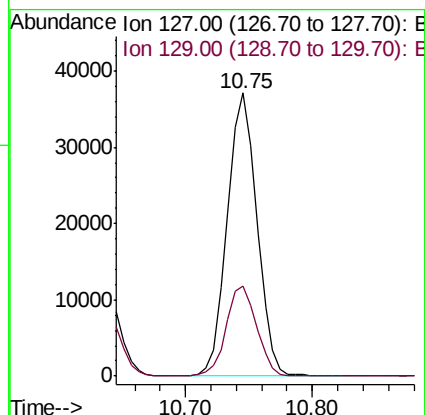

#31
Hexachlorobutadiene
Concen: 26.956 ng/ul
RT: 10.92 min Scan# 1315
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:225 Resp: 52471
Ion Ratio Lower Upper
225 100
223 61.7 49.4 74.0
227 62.0 49.6 74.4



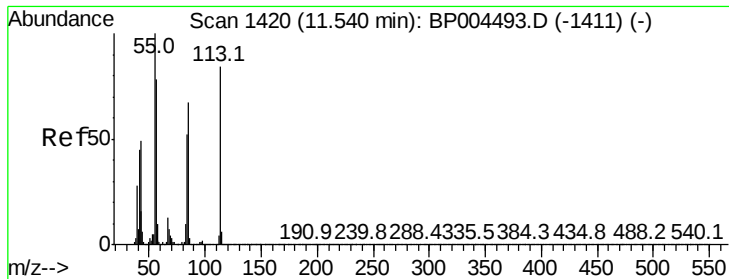

#32

Caprolactam

Concen: 8.418 ng/ul

RT: 11.51 min Scan# 1415

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:113 Resp: 7500

Ion Ratio Lower Upper

113 100

55 146.9 117.5 176.3




56 110.0 88.0 132.0

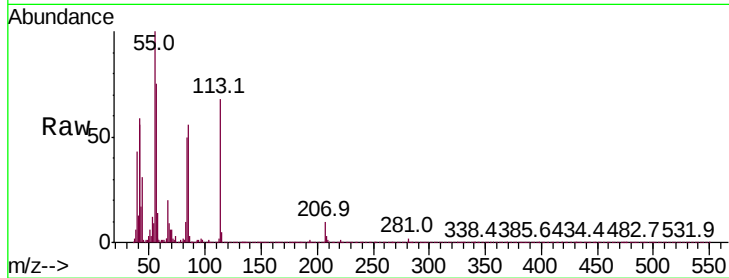

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BP0

Ion 56.00 (55.70 to 56.70): BP0

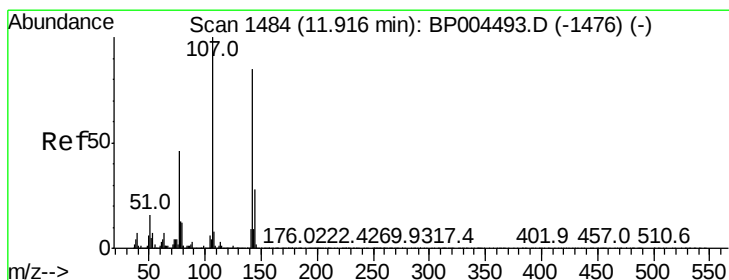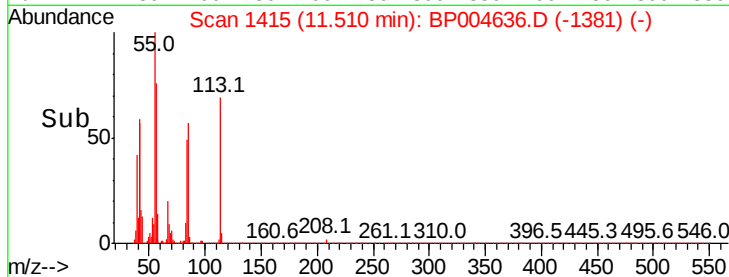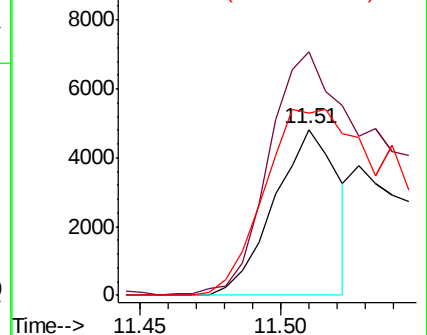

#33

4-Chloro-3-methylphenol

Concen: 21.536 ng/ul

RT: 11.87 min Scan# 1476

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:107 Resp: 59348

Ion Ratio Lower Upper

107 100

144 26.0 20.8 31.2



142 77.4 61.9 92.9

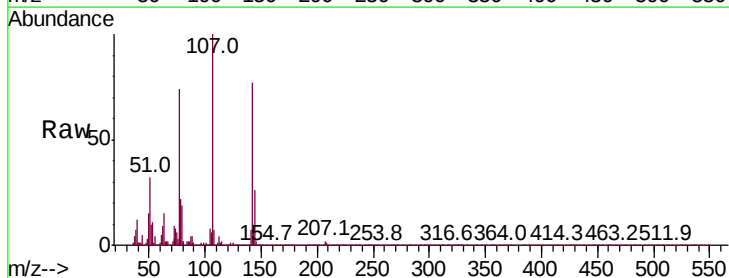


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E



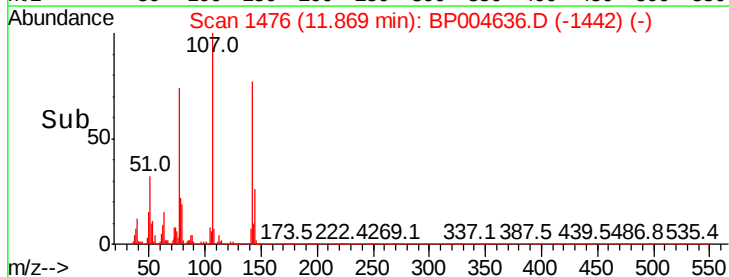
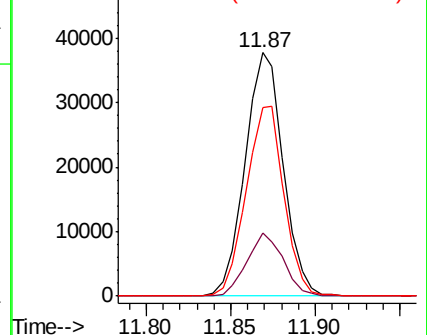




#34
2-Methylnaphthalene
Concen: 19.927 ng/ul
RT: 12.25 min Scan# 1541
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:142 Resp: 125301
Ion Ratio Lower Upper
142 100
141 88.9 71.1 106.7

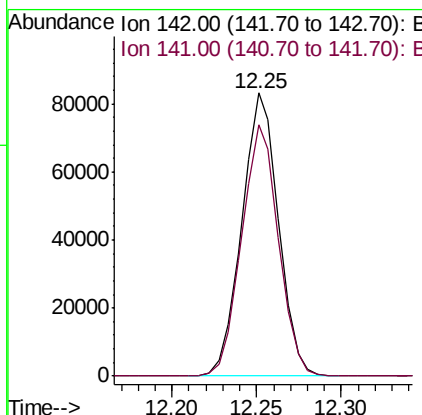

#35
1-Methylnaphthalene
Concen: 16.750 ng/ul
RT: 12.47 min Scan# 1578
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:142 Resp: 122608
Ion Ratio Lower Upper
142 100
141 86.1 68.9 103.3
116 4.8 3.8 5.8

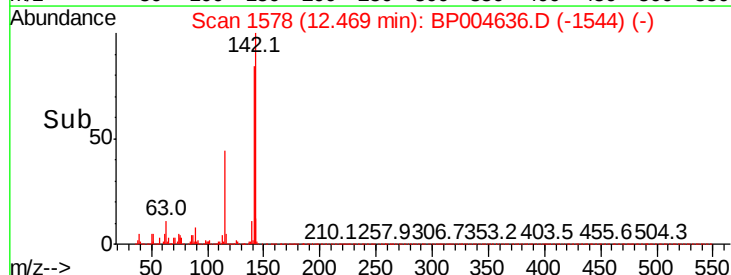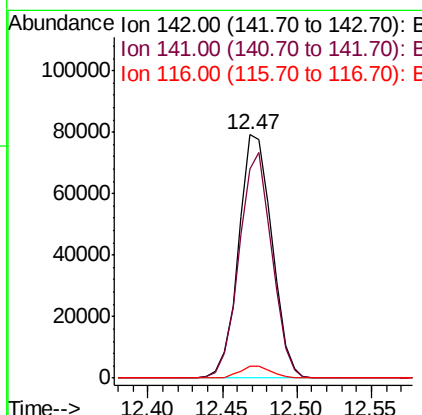



#37

1,2,4,5-Tetrachlorobenzene

Concen: 20.414 ng/ul

RT: 12.62 min Scan# 1604

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079

Tot Ion:216 Resp: 97097



Ion Ratio Lower Upper

216 100

214 74.6 59.7 89.5

179 18.9 15.1 22.7

108 13.6 10.9 16.3





Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

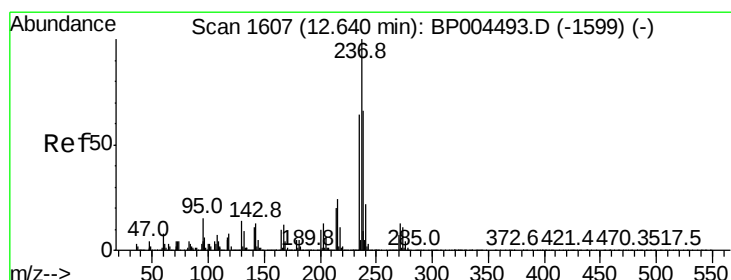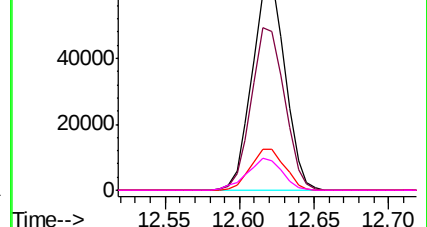

#38

Hexachlorocyclopentadiene

Concen: 23.939 ng/ul

RT: 12.60 min Scan# 1601

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32



Tgt Ion:237 Resp: 65039

Ion Ratio Lower Upper

237 100

235 62.9 50.3 75.5


272 11.7 9.4 14.0




Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E




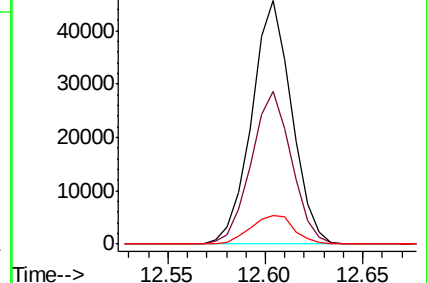




#39
 2,4,6-Trichlorophenol
 Concen: 19.913 ng/ul
 RT: 12.86 min Scan# 1645
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079


Tot Ion	Ratio	Lower	Upper
196	100		
198	89.5	71.6	107.4
200	31.4	25.1	37.7

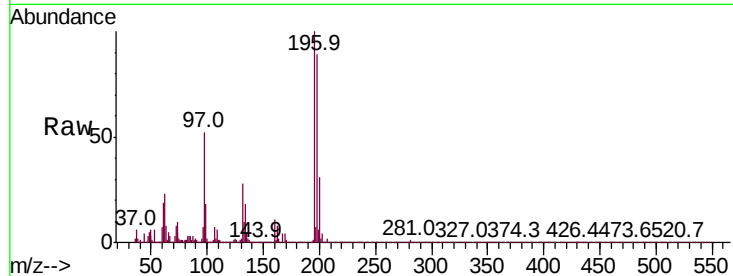

#40
 2,4,5-Trichlorophenol
 Concen: 20.097 ng/ul
 RT: 12.93 min Scan# 1656
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
196	100		
198	95.6	76.5	114.7
200	30.2	24.2	36.2









#41
1,1'-Biphenyl
Concen: 16.882 ng/ul
RT: 13.27 min Scan# 1714
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion	Ratio	Lower	Upper
154	100		
153	39.9	31.9	47.9
76	10.4	8.3	12.5

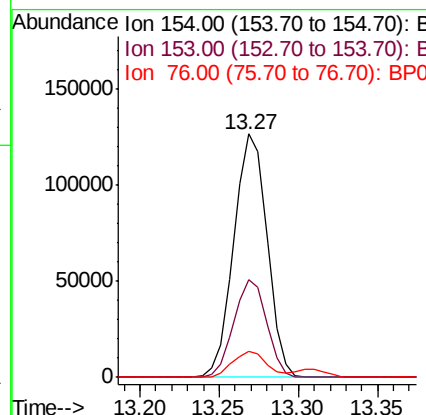

#42
2-Chloronaphthalene
Concen: 17.301 ng/ul
RT: 13.31 min Scan# 1721
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
162	100		
164	31.9	25.5	38.3
127	32.3	25.8	38.8

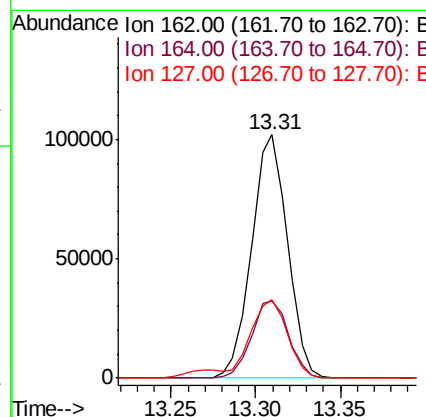



#43

2-Nitroaniline

Concen: 18.354 ng/ul

RT: 13.51 min Scan# 1755

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion: 65 Resp: 40439

Ion Ratio Lower Upper

65 100

92 59.9 47.9 71.9




138 89.4 71.5 107.3

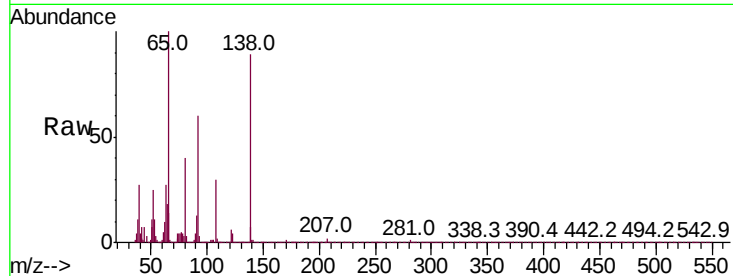

Abundance Ion 65.00 (64.70 to 65.70): BP0

Ion 92.00 (91.70 to 92.70): BP0

Ion 138.00 (137.70 to 138.70): E

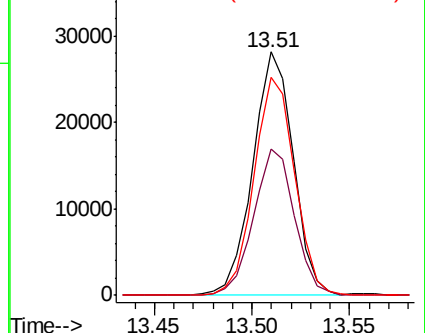

#45

Dimethylphthalate

Concen: 18.352 ng/ul

RT: 13.90 min Scan# 1821

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion: 163 Resp: 196534

Ion Ratio Lower Upper

163 100

194 5.2 4.2 6.2



164 10.0 8.0 12.0




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E




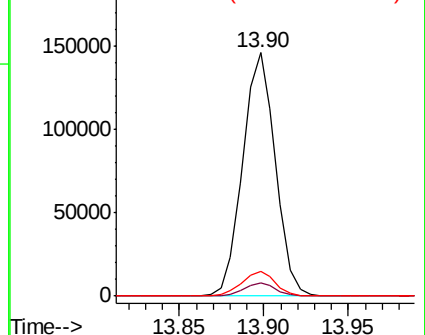




#46
2,6-Dinitrotoluene
Concen: 17.289 ng/ul
RT: 14.01 min Scan# 1840
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion	Ratio	Lower	Upper
165	100		
89	68.0	54.4	81.6
121	18.4	14.7	22.1

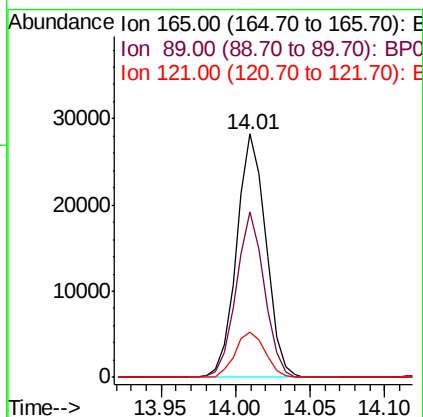

#48
Acenaphthylene
Concen: 15.978 ng/ul
RT: 14.16 min Scan# 1865
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.8	23.6
153	12.8	10.2	15.4

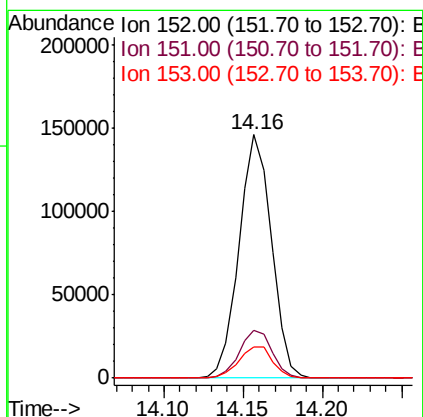



#49

3-Nitroaniline

Concen: 15.674 ng/ul

RT: 14.34 min Scan# 1896

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:138 Resp: 29516

Ion Ratio Lower Upper

138 100

108 11.7 9.4 14.0




92 127.6 102.1 153.1



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BP0

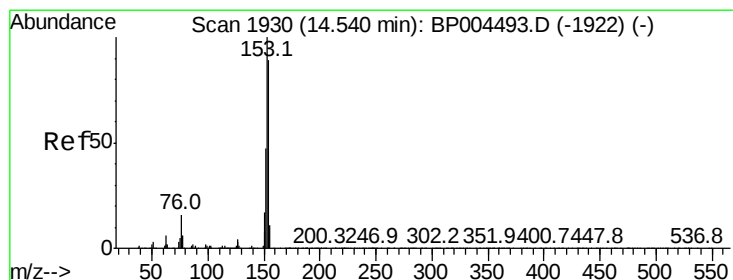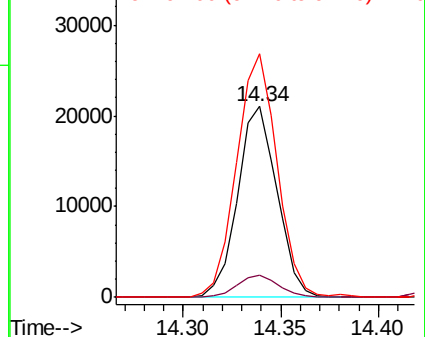

#50

Acenaphthene

Concen: 16.849 ng/ul

RT: 14.50 min Scan# 1924

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:153 Resp: 153087

Ion Ratio Lower Upper

153 100

152 46.1 36.9 55.3



154 90.3 72.2 108.4




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



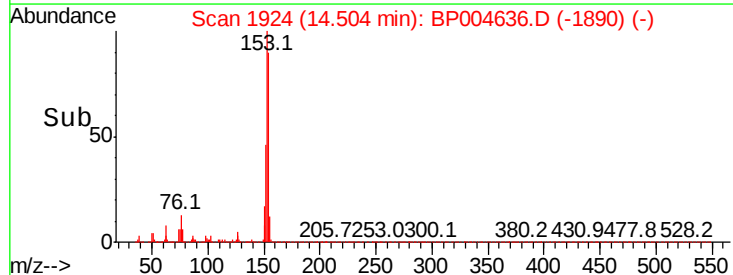
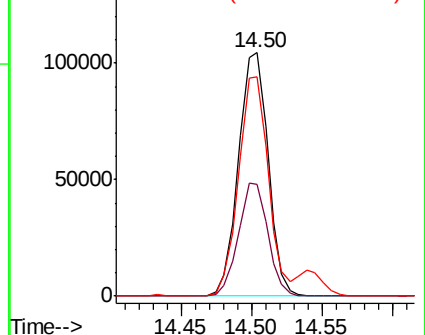




#51
2,4-Dinitrophenol
Concen: 20.072 ng/ul
RT: 14.54 min Scan# 1930
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:184 Resp: 24439
Ion Ratio Lower Upper
184 100
63 63.7 51.0 76.4
154 63.7 51.0 76.4

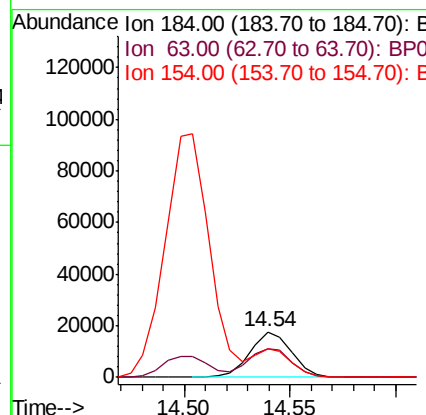

#53
4-Nitrophenol
Concen: 27.375 ng/ul
RT: 14.65 min Scan# 1948
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:109 Resp: 37101
Ion Ratio Lower Upper
109 100
139 78.8 63.0 94.6
65 104.4 83.5 125.3

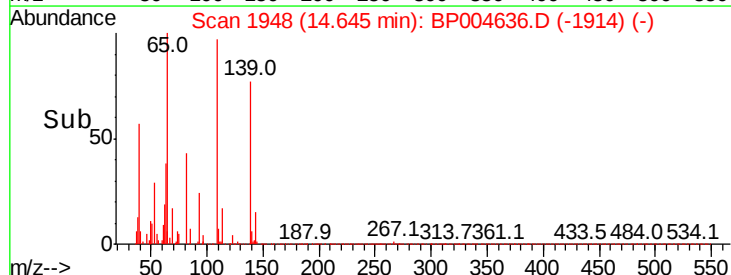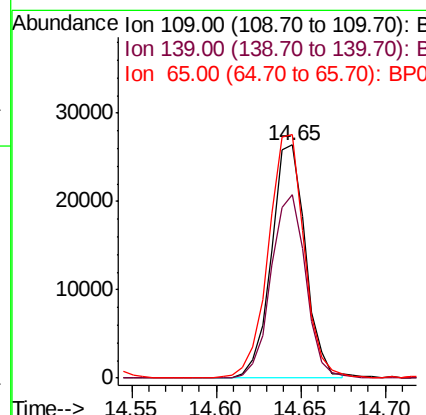



#54

Dibenzofuran

Concen: 18.530 ng/ul

RT: 14.84 min Scan# 1981

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :





SSTD02079

Tot Ion:168 Resp: 237064

Ion Ratio Lower Upper

168 100

139 34.4 27.5 41.3

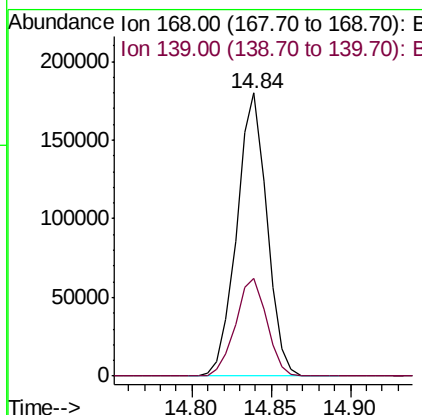

#55

2,4-Dinitrotoluene

Concen: 17.057 ng/ul

RT: 14.80 min Scan# 1974

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32




Tgt Ion:165 Resp: 54585


Ion Ratio Lower Upper

165 100

63 50.7 40.6 60.8

182 2.9 2.3 3.5

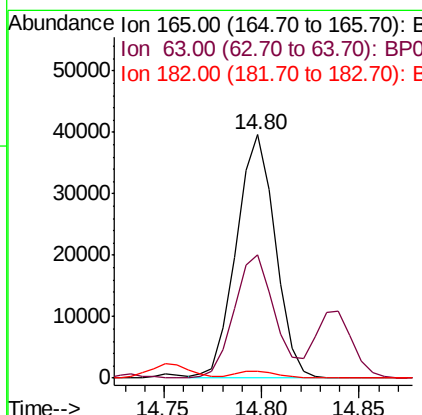


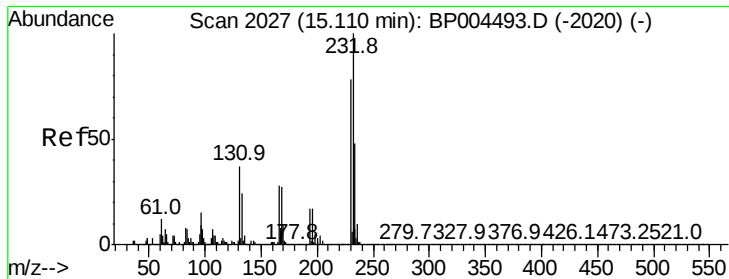




#56
2,3,4,6-Tetrachlorophenol
Concen: 22.089 ng/ul
RT: 15.06 min Scan# 2019
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Instrument :
BNA_P
ClientSampleId :
SSTD02079

Tot Ion:	232	Resp:	60793
Ion	Ratio	Lower	Upper
232	100		
131	34.3	27.4	41.2
130	2.0	1.6	2.4
166	25.7	20.6	30.8

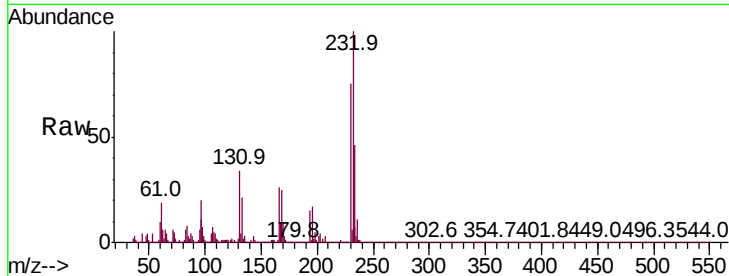


Abundance Ion 232.00 (231.70 to 232.70): E
Ion 131.00 (130.70 to 131.70): E
Ion 130.00 (129.70 to 130.70): E
Ion 166.00 (165.70 to 166.70): E

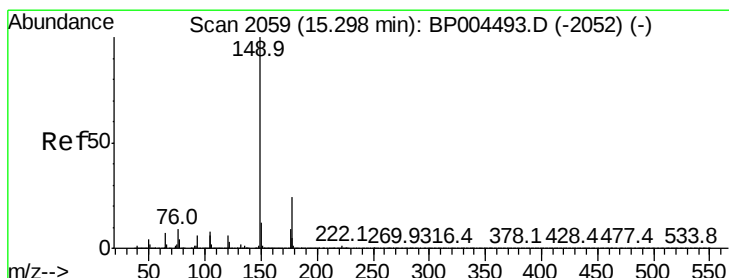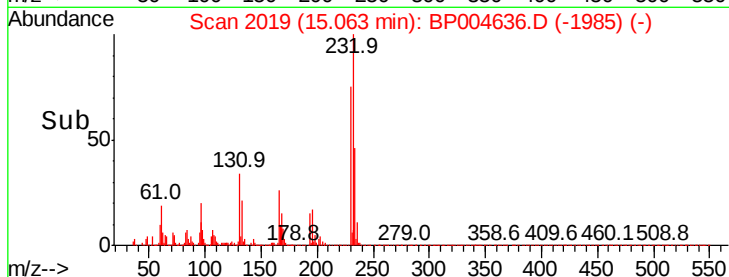
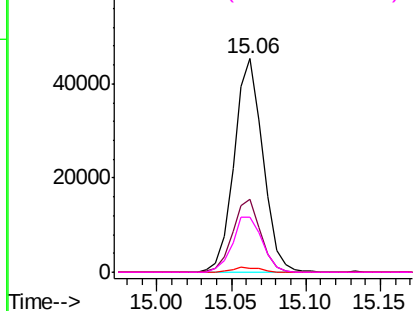



#57
Diethylphthalate
Concen: 17.935 ng/ul
RT: 15.27 min Scan# 2054
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:	149	Resp:	188931
Ion	Ratio	Lower	Upper
149	100		
177	25.5	20.4	30.6
150	12.7	10.2	15.2

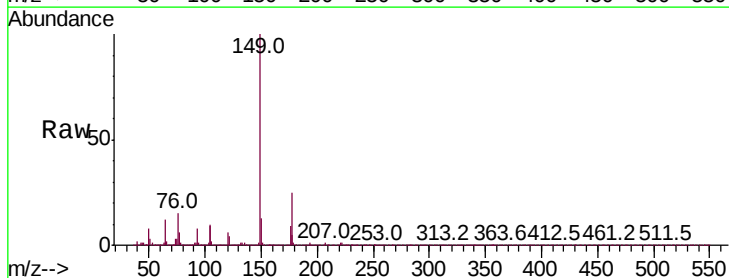

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 177.00 (176.70 to 177.70): E
Ion 150.00 (149.70 to 150.70): E

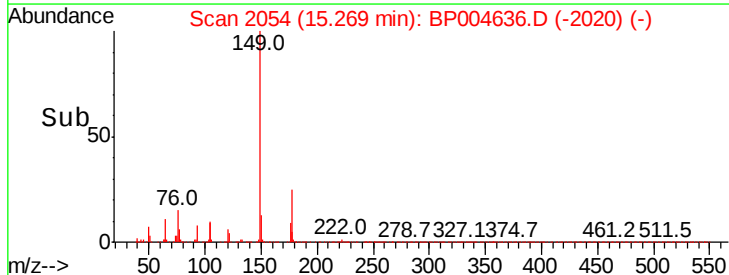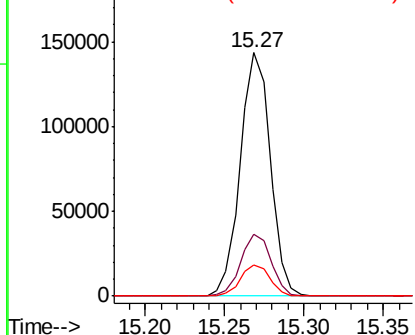



#59

Fluorene

Concen: 19.059 ng/ul

RT: 15.49 min Scan# 2092

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:166 Resp: 197582

Ion Ratio Lower Upper

166 100

165 95.0 76.0 114.0




167 13.3 10.6 16.0



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

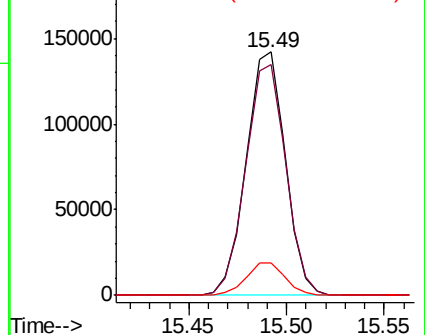

#60

4-Chlorophenyl-phenylether

Concen: 21.674 ng/ul

RT: 15.49 min Scan# 2091

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:204 Resp: 120174

Ion Ratio Lower Upper

204 100

206 33.4 26.7 40.1



141 51.2 41.0 61.4




Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E




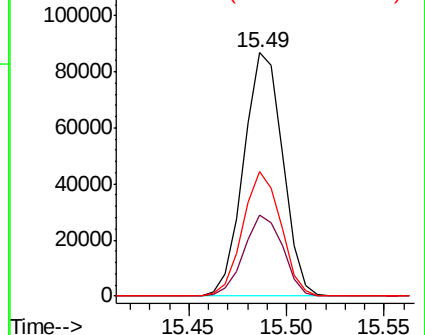




#61
4-Nitroaniline
Concen: 17.673 ng/ul
RT: 15.50 min Scan# 2094
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:138 Resp: 34984
Ion Ratio Lower Upper
138 100
92 61.4 49.1 73.7
108 132.7 106.2 159.2

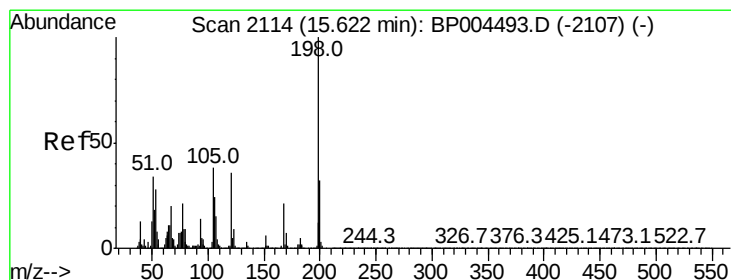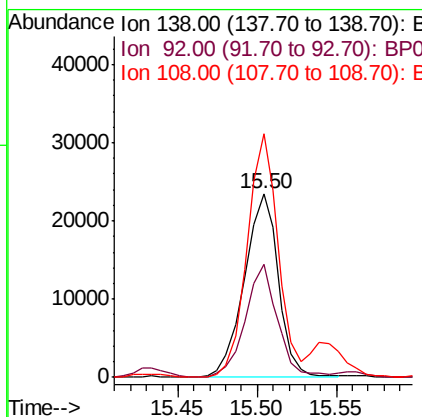

#64
4,6-Dinitro-2-methylphenol
Concen: 17.056 ng/ul
RT: 15.56 min Scan# 2103
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:198 Resp: 38407
Ion Ratio Lower Upper
198 100
182 2.5 2.0 3.0
77 29.1 23.3 34.9



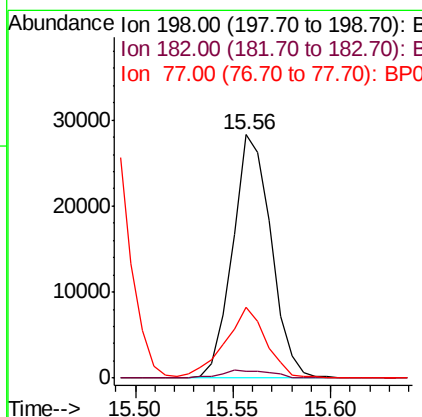
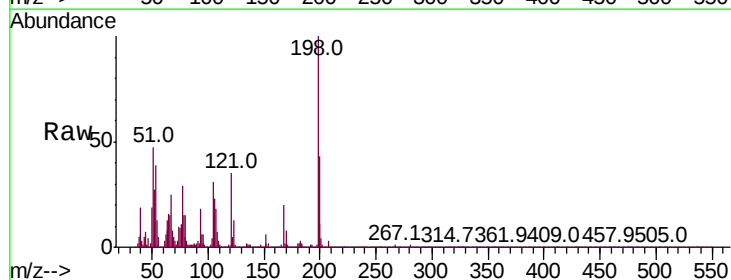




#65
N-Nitrosodiphenylamine
Concen: 17.337 ng/ul
RT: 15.70 min Scan# 2127
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:169 Resp: 172226
Ion Ratio Lower Upper
169 100
168 65.4 52.3 78.5
167 35.1 28.1 42.1

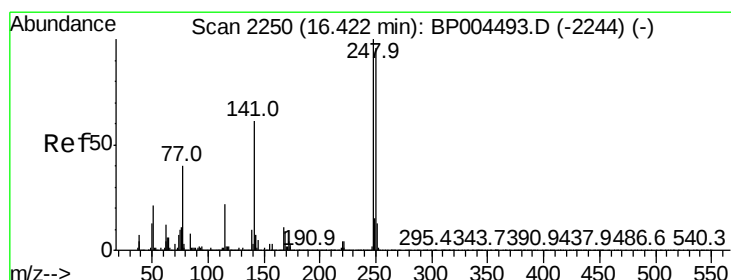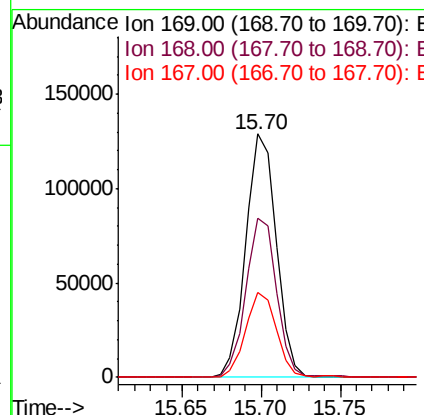

#66
4-Bromophenyl-phenylether
Concen: 19.655 ng/ul
RT: 16.39 min Scan# 2244
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:248 Resp: 78680
Ion Ratio Lower Upper
248 100
250 97.9 78.3 117.5
141 63.3 50.6 76.0


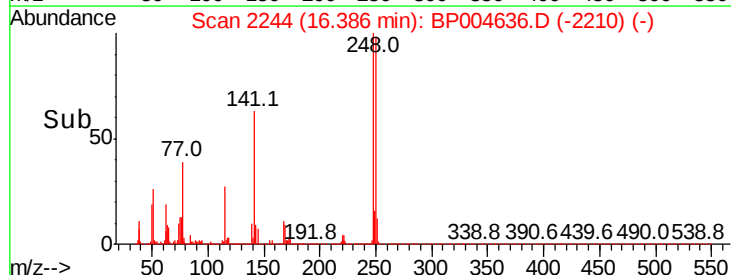
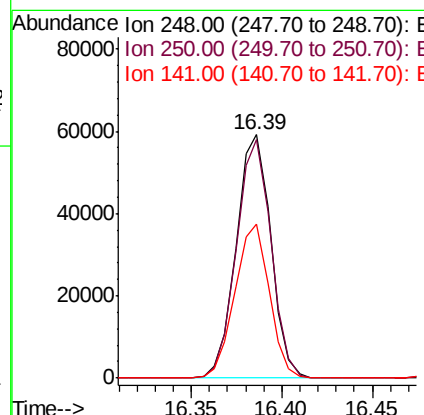





#67
Hexachlorobenzene
Concen: 19.161 ng/ul
RT: 16.49 min Scan# 2262
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion	Ratio	Lower	Upper
284	100		
142	27.5	22.0	33.0
249	31.6	25.3	37.9

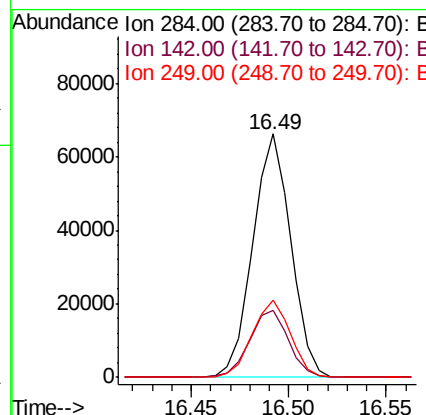

#68
Atrazine
Concen: 20.692 ng/ul
RT: 16.66 min Scan# 2290
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
200	100		
173	21.6	17.3	25.9
215	49.0	39.2	58.8


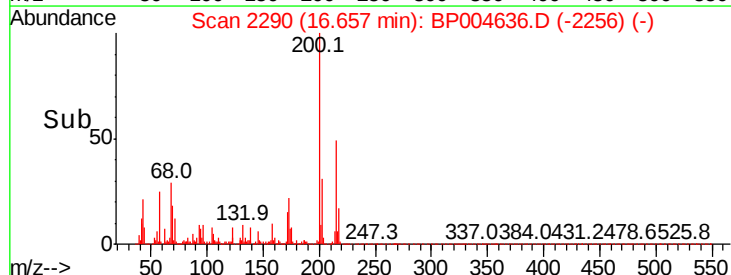
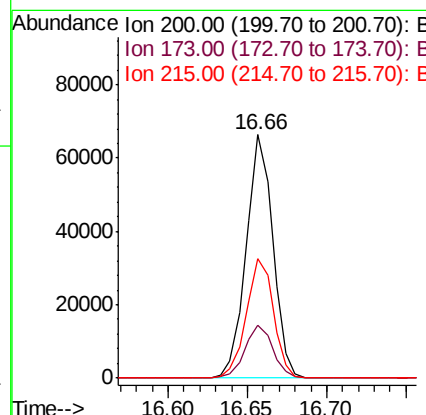





#69
 Pentachlorophenol
 Concen: 21.759 ng/ul
 RT: 16.84 min Scan# 2321
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079


Tot Ion:266 Resp: 53144
 Ion Ratio Lower Upper
 266 100
 264 61.8 49.4 74.2
 268 68.4 54.7 82.1

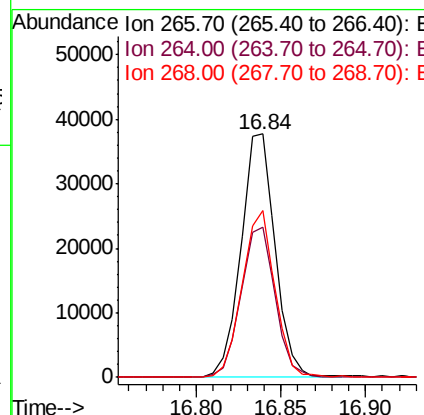

#70
 Phenanthrene
 Concen: 17.416 ng/ul
 RT: 17.23 min Scan# 2388
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32

Tgt Ion:178 Resp: 334422
 Ion Ratio Lower Upper
 178 100
 179 16.2 13.0 19.4
 176 19.0 15.2 22.8

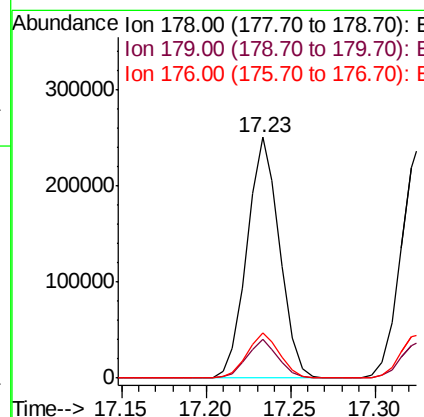



#72

Anthracene

Concen: 17.720 ng/ul

RT: 17.33 min Scan# 2404

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :





BNA_P

ClientSampleId :

SSTD02079

Tot Ion:178 Resp: 340769

Ion	Ratio	Lower	Upper
178	100		
179	15.3	12.2	18.4
176	18.4	14.7	22.1



#73

1,2,3,4-Tetrachlorobenzene

Concen: 18.696 ng/uL

RT: 13.23 min Scan# 1707




Delta R.T. 0.00 min


Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Tgt Ion:216 Resp: 100087

Ion	Ratio	Lower	Upper
216	100		
214	76.5	61.2	91.8
218	47.5	38.0	57.0









#74
 Pentachlorobenzene
 Concen: 19.686 ng/uL
 RT: 14.76 min Scan# 1967
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079


Tot Ion	Ratio	Lower	Upper
250	100		
248	59.0	47.2	70.8
252	62.3	49.8	74.8

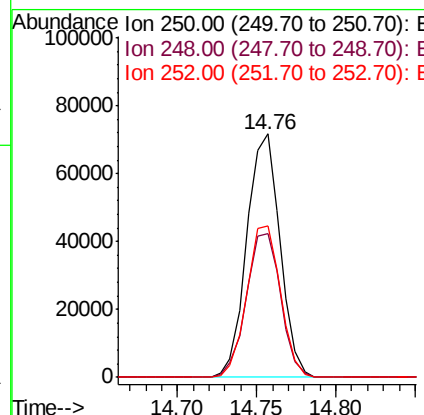

#75
 Carbazole
 Concen: 17.980 ng/uL
 RT: 17.60 min Scan# 2450
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
167	100		
166	20.9	16.7	25.1
139	11.8	9.4	14.2


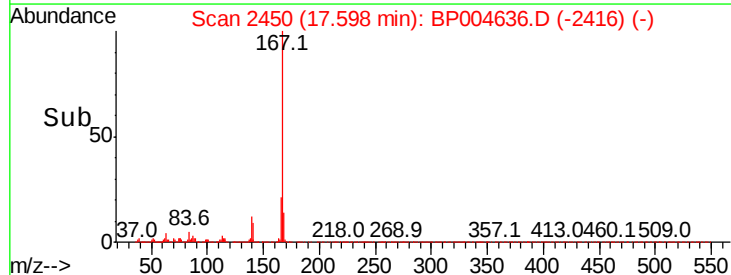
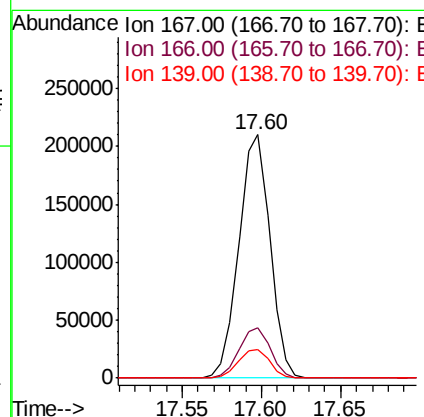





#76
Di-n-butylphthalate
Concen: 15.650 ng/ul
RT: 18.16 min Scan# 2546
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion:149 Resp: 312562
Ion Ratio Lower Upper
149 100
150 9.2 7.4 11.0
104 6.9 5.5 8.3

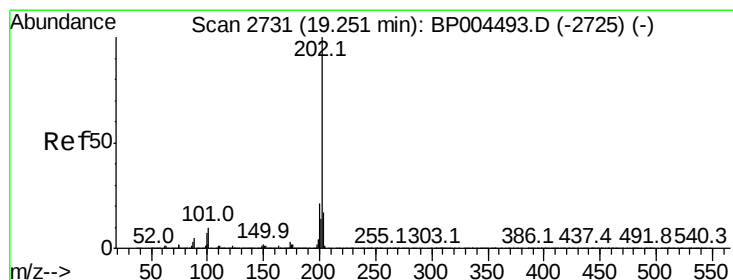

#77
Fluoranthene
Concen: 19.626 ng/ul
RT: 19.20 min Scan# 2723
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:202 Resp: 427503
Ion Ratio Lower Upper
202 100
101 4.8 3.8 5.8
100 4.2 3.4 5.0




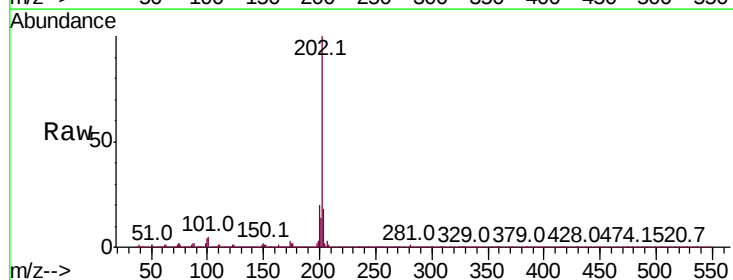




#80
Pvrene
Concen: 18.090 ng/ul
RT: 19.56 min Scan# 2783
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tot Ion	Ratio	Lower	Upper
202	100		
101	6.6	5.3	7.9
100	5.6	4.5	6.7

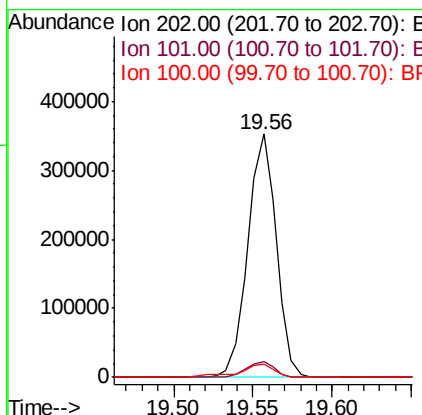

#81
Butylbenzylphthalate
Concen: 14.338 ng/ul
RT: 20.44 min Scan# 2933
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
149	100		
91	73.1	58.5	87.7
206	28.4	22.7	34.1

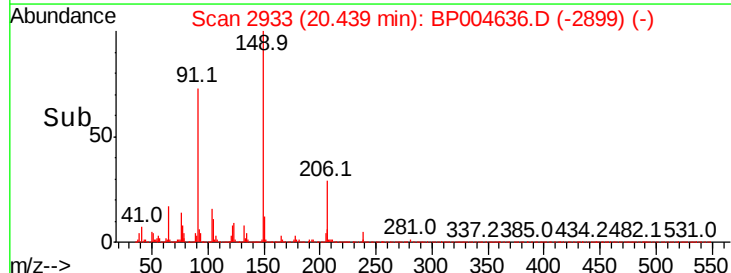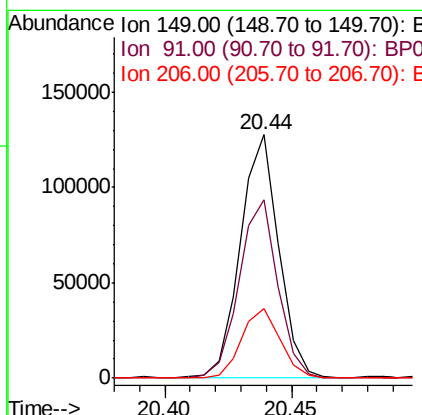



#82

3,3'-Dichlorobenzidine

Concen: 20.555 ng/ul

RT: 21.20 min Scan# 3062

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:252 Resp: 152126

Ion Ratio Lower Upper

252 100

254 64.3 51.4 77.2




126 6.3 5.0 7.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

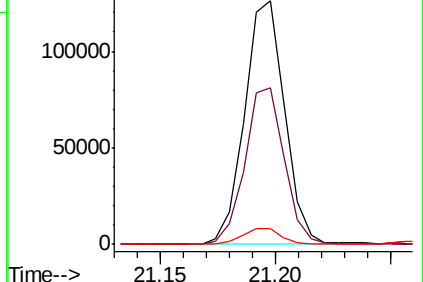

#83

Benzo(a)anthracene

Concen: 17.570 ng/ul

RT: 21.26 min Scan# 3073

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:228 Resp: 422334

Ion Ratio Lower Upper

228 100

229 19.7 15.8 23.6



226 26.1 20.9 31.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E




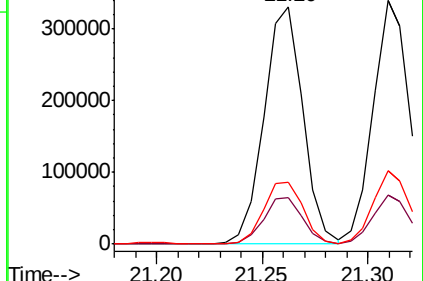




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 14.176 ng/ul
 RT: 21.20 min Scan# 3062
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD02079


Tot Ion:149 Resp: 194427
 Ion Ratio Lower Upper
 149 100
 167 31.2 25.0 37.4
 279 6.6 5.3 7.9

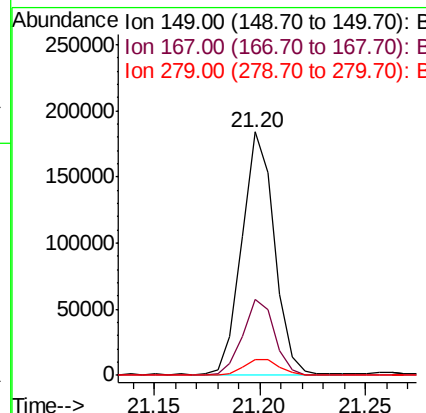

#85
 Chrysene
 Concen: 17.536 ng/ul
 RT: 21.31 min Scan# 3081
 Delta R.T. 0.00 min
 Lab File: BP004636.D
 Acq: 26 Jan 2021 17:32

Tgt Ion:228 Resp: 406965
 Ion Ratio Lower Upper
 228 100
 226 30.3 24.2 36.4
 229 20.3 16.2 24.4



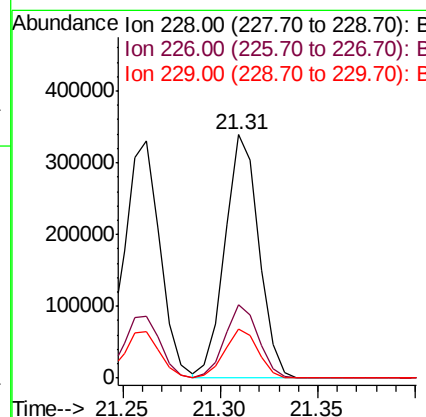





#87
Di-n-octyl phthalate
Concen: 15.676 ng/ul
RT: 22.10 min Scan# 3215
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32




Instrument :
BNA_P
ClientSampleId :
SSTD02079


Tgt Ion:149 Resp: 311686

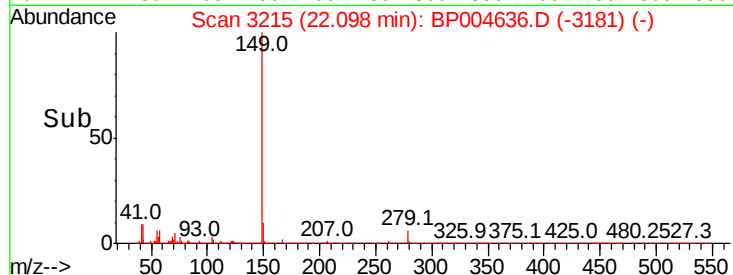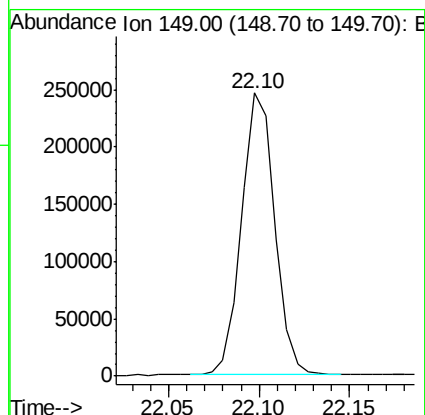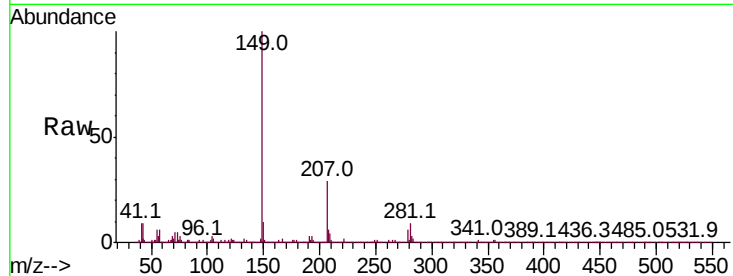

#88
Benzo(b)fluoranthene
Concen: 19.335 ng/ul
RT: 22.89 min Scan# 3350
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion:252 Resp: 425294
Ion Ratio Lower Upper
252 100
253 23.0 18.4 27.6
125 3.7 3.0 4.4

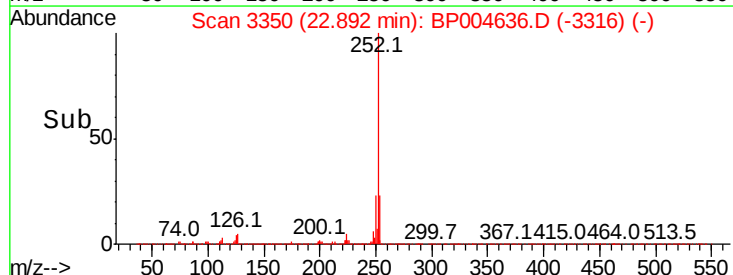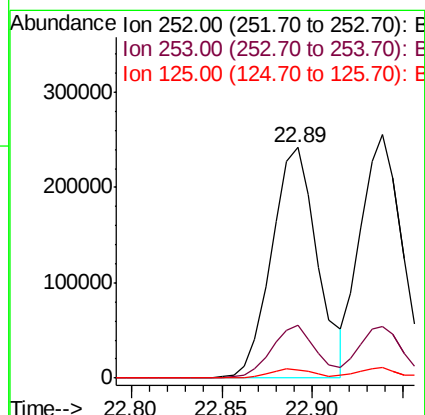



#89

Benzo(k)fluoranthene

Concen: 19.008 ng/ul

RT: 22.94 min Scan# 3358

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079


Tot Ion:252 Resp: 405665

Ion Ratio Lower Upper

252 100

253 21.0 16.8 25.2




125 4.6 3.7 5.5



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

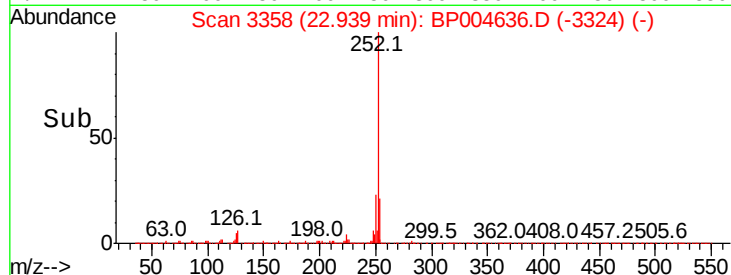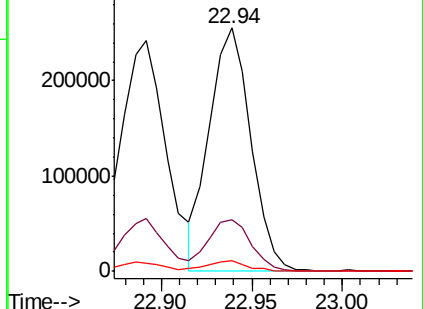

#91

Benzo(a)pyrene

Concen: 17.695 ng/ul

RT: 23.49 min Scan# 3452

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32


Tgt Ion:252 Resp: 359013

Ion Ratio Lower Upper

252 100

253 22.2 17.8 26.6



125 4.6 3.7 5.5




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

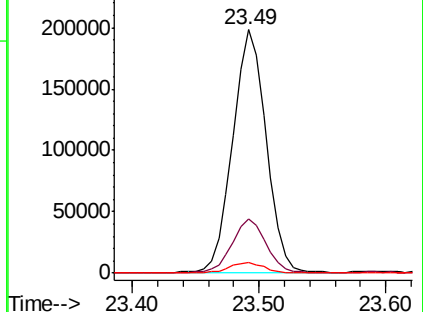







#92

Indeno(1,2,3-cd)pyrene
Concen: 17.948 ng/ul
RT: 25.98 min Scan# 3875
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Instrument :
BNA_P
ClientSampleId :
SSTD02079




Tot Ion	Ratio	Lower	Upper
276	100		
138	9.7	7.8	11.6
277	23.8	19.0	28.6

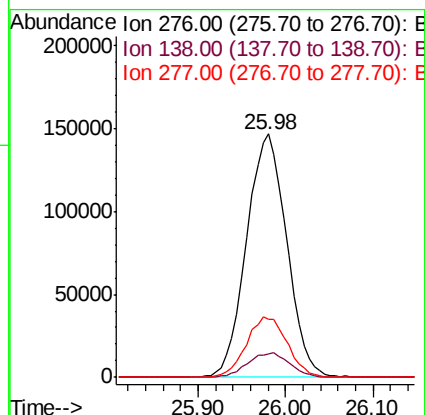


#93

Dibenzo(a,h)anthracene
Concen: 18.207 ng/ul
RT: 26.00 min Scan# 3878
Delta R.T. 0.00 min
Lab File: BP004636.D
Acq: 26 Jan 2021 17:32

Tgt Ion	Ratio	Lower	Upper
278	100		
139	6.8	5.4	8.2
279	26.0	20.8	31.2





#94

Benzo(a,h,i)perylene

Concen: 17.527 ng/ul

RT: 26.71 min Scan# 3999

Delta R.T. 0.00 min

Lab File: BP004636.D

Acq: 26 Jan 2021 17:32

Instrument :

BNA_P

ClientSampleId :

SSTD02079

Tot Ion: 276 Resp: 376955

Ion Ratio Lower Upper

276 100

138 8.7 7.0 10.4

277 24.6 19.7 29.5

