

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012721\
 Data File : BP004650.D
 Acq On : 27 Jan 2021 14:27
 Operator : CG/JU
 Sample : M1173-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0FY4

Quant Time: Jan 27 15:07:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP012721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 27 11:31:03 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	37956	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	135161	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	115870	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.19	188	289462	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	332958	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	312757	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.27	96	3824	5.21	ng/uL	0.00
5) Phenol-d5	6.95	99	18941	6.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	53210	33.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	51872	26.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	34903	16.56	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	30503	34.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	38596	34.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	79686	30.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	4828	2.21	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	331869	38.64	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	370106	36.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	10469	8.24	ng/ul	0.00
58) Fluorene-d10	15.43	176	305048	39.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	71498	40.88	ng/ul	0.00
71) Anthracene-d10	17.29	188	598130	46.45	ng/ul	0.00
79) Pyrene-d10	19.53	212	739729	45.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	763873	47.20	ng/ul	0.00


Target Compounds				Ovalue		
6) Phenol	6.98	94	5411	1.874	ng/ul#	86
45) Dimethylphthalate	13.89	163	8881	1.019	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP012721\
Data File : BP004650.D
Acq On : 27 Jan 2021 14:27
Operator : CG/JU
Sample : M1173-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0FY4

Quant Time: Jan 27 15:07:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP012721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 27 11:31:03 2021
Response via : Initial Calibration

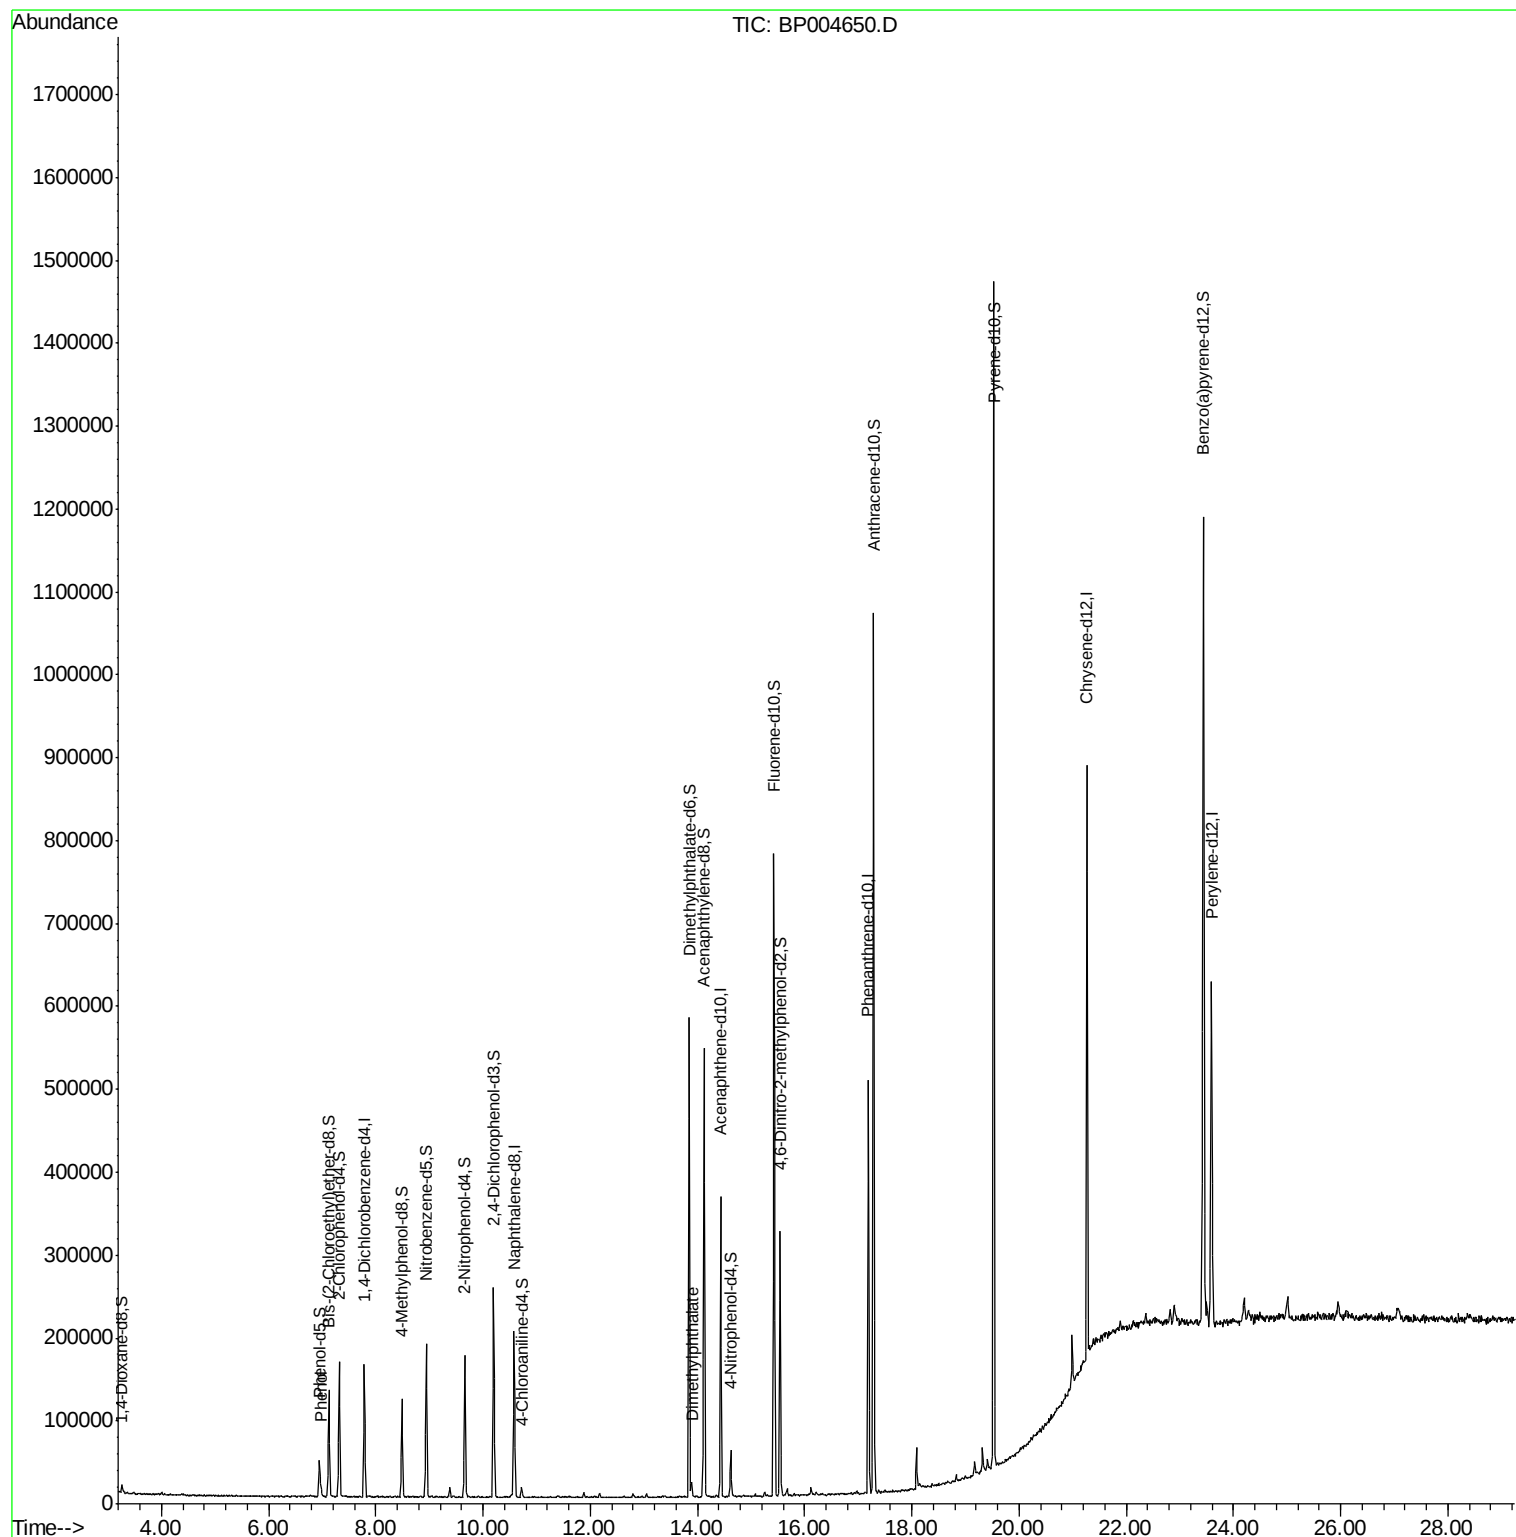

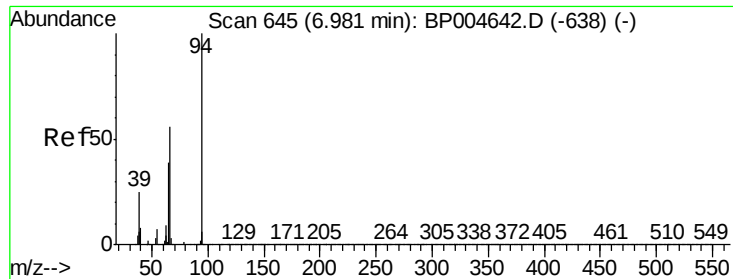

#6

Phenol

Concen: 1.874 ng/ul

RT: 6.98 min Scan# 644

Delta R.T. -0.01 min

Lab File: BP004650.D

Acq: 27 Jan 2021 14:27

Instrument :

BNA_P

ClientSampled :

C0FY4


Tot Ion: 94 Resp: 5411

Ion Ratio Lower Upper

94 100

65 27.7 30.1 45.1#




66 48.8 46.4 69.6

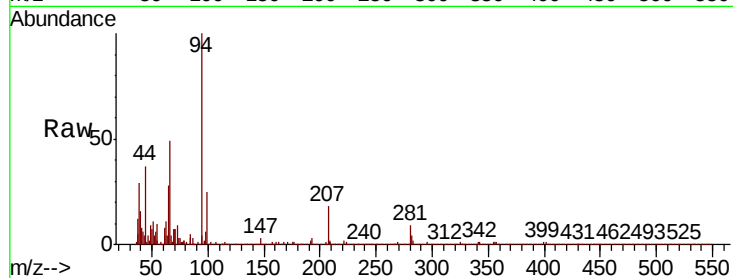

Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

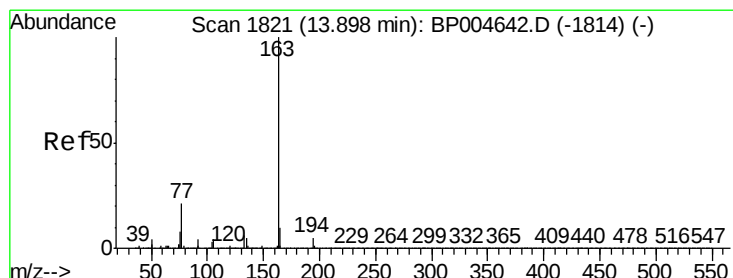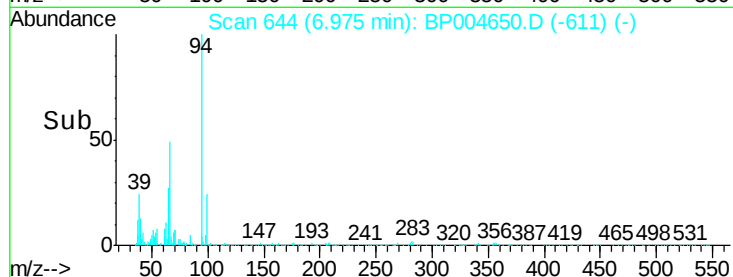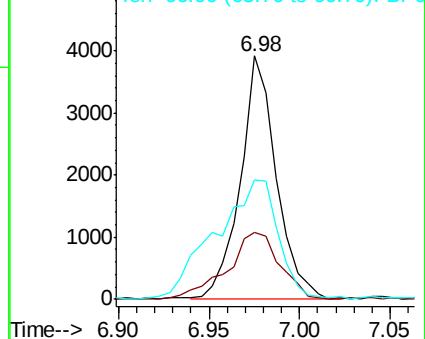

#45

Dimethylphthalate

Concen: 1.019 ng/ul

RT: 13.89 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BP004650.D

Acq: 27 Jan 2021 14:27


Tgt Ion: 163 Resp: 8881

Ion Ratio Lower Upper

163 100

194 4.6 4.2 6.2

164 9.8 8.0 12.0

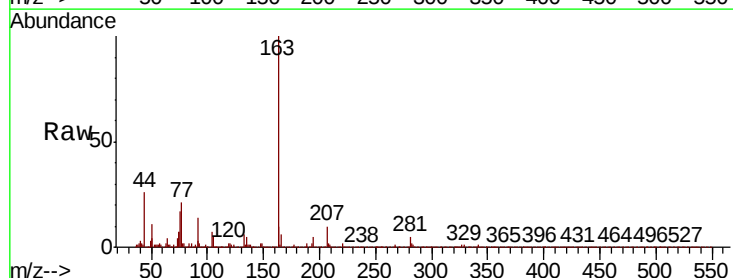

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

