
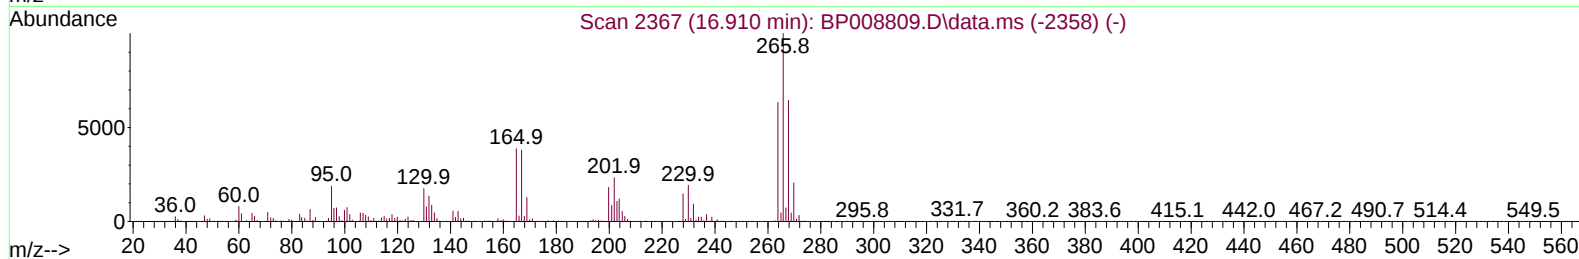
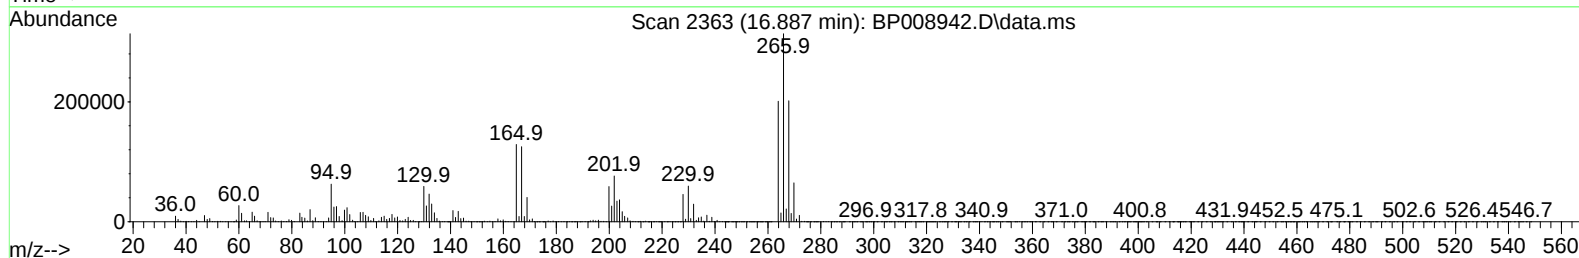


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008942.D
Acq On : 27 Jan 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:03:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 26 01:52:51 2022
Response via : Initial Calibration

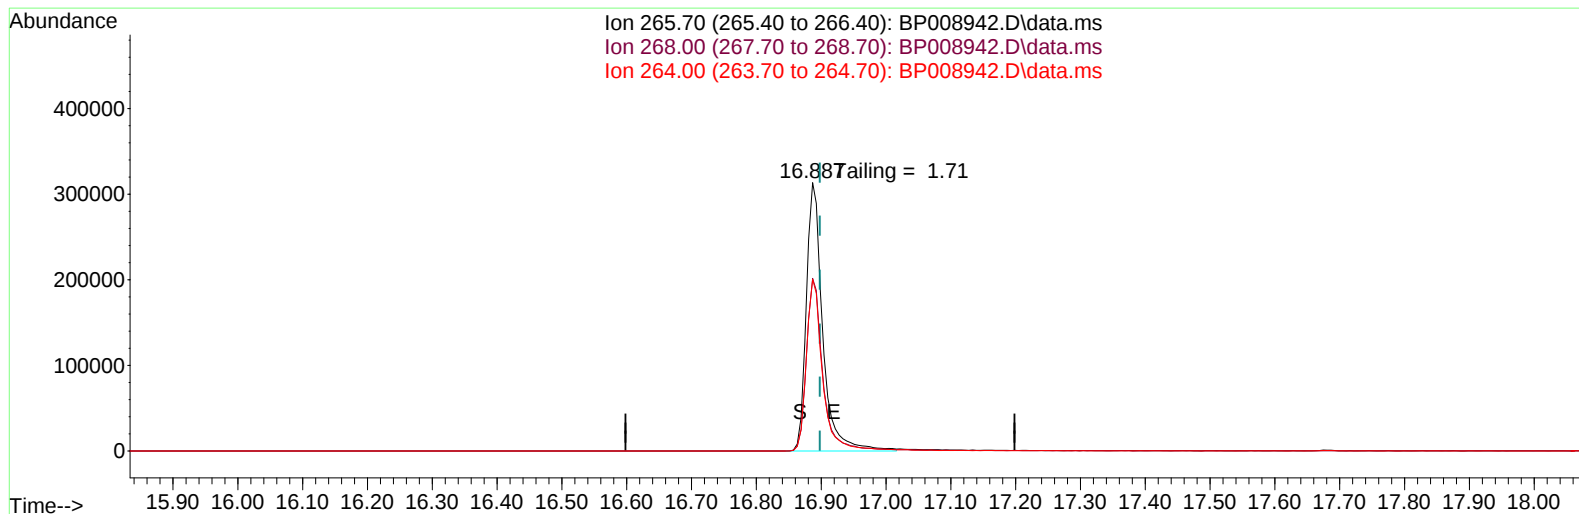

TIC: BP008942.D\data.ms

(70) Pentachlorophenol (C)




16.887min (-0.012) 183745.98 ng

response 557394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.36
264.00	62.90	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008942.D
 Acq On : 27 Jan 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:03:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

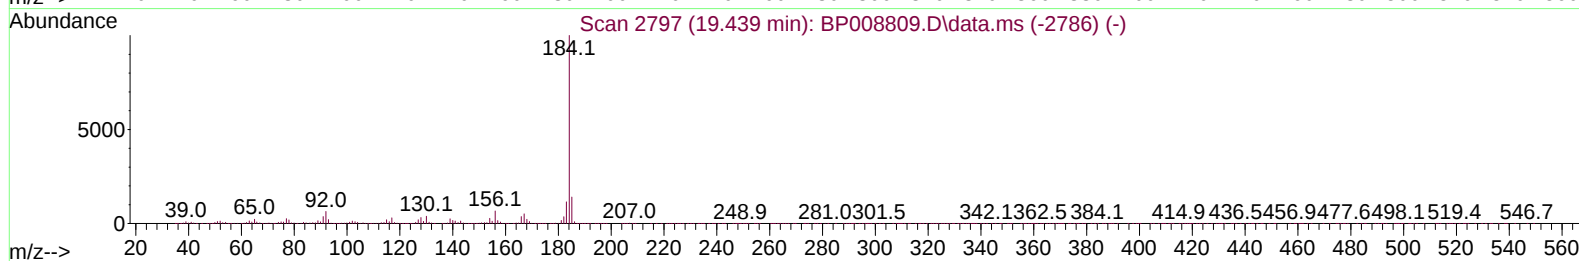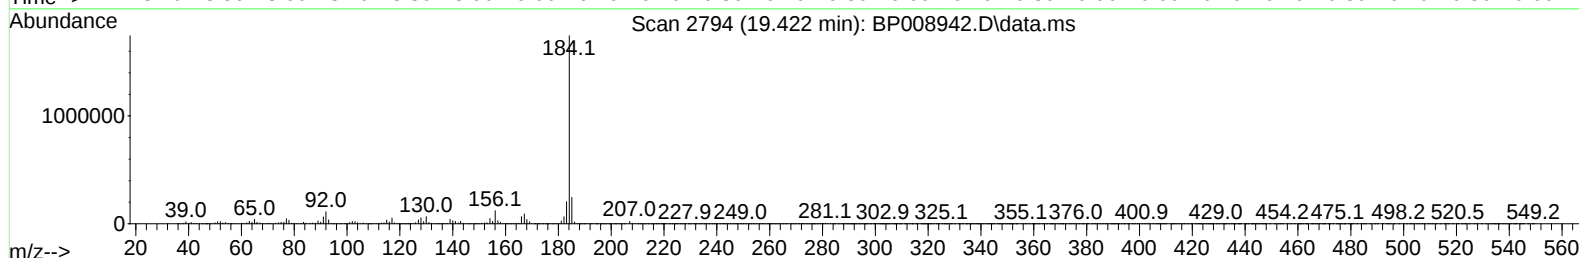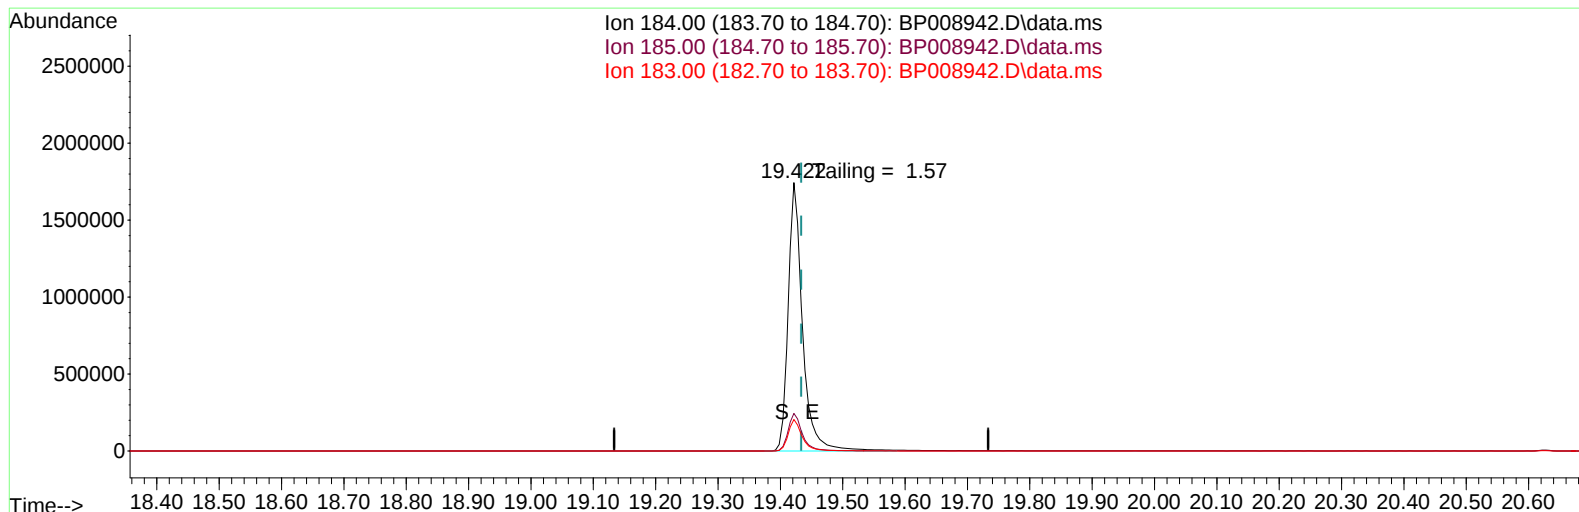

TIC: BP008942.D\data.ms

(77) Benzidine**19.422min (-0.012) 37887.15 ng****response 2824170**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.01
183.00	11.90	11.76
0.00	0.00	0.00