

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008944.D
 Acq On : 27 Jan 2022 13:12
 Operator : CG/JU
 Sample : PB142279BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142279BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	15	rVB	212554	273432	1.74%	0.379%
2	5.428	408	415	436	rBV	4968070	7557731	48.20%	10.475%
3	7.022	678	686	710	rBV	4330600	7446834	47.50%	10.322%
4	7.840	818	825	836	rBV	993225	1609066	10.26%	2.230%
5	9.005	1013	1023	1046	rBV	2737870	4848214	30.92%	6.720%
6	10.640	1292	1301	1316	rBV	1203766	2178280	13.89%	3.019%
7	13.104	1712	1720	1740	rBV	7804735	11912872	75.98%	16.512%
8	14.481	1945	1954	1972	rBV	1811144	2866940	18.29%	3.974%
9	15.975	2201	2208	2238	rBV	5208259	8528915	54.40%	11.821%
10	17.239	2414	2423	2436	rBV	2078720	3249423	20.72%	4.504%
11	19.798	2852	2858	2870	rBV	12856768	15678785	100.00%	21.731%
12	21.327	3113	3118	3130	rBV	2096848	2967876	18.93%	4.114%
13	21.445	3135	3138	3142	rBV	147322	201901	1.29%	0.280%
14	23.745	3523	3529	3542	rVB2	1339279	2827762	18.04%	3.919%




Sum of corrected areas: 72148031

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008944.D
Acq On : 27 Jan 2022 13:12
Operator : CG/JU
Sample : PB142279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142279BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

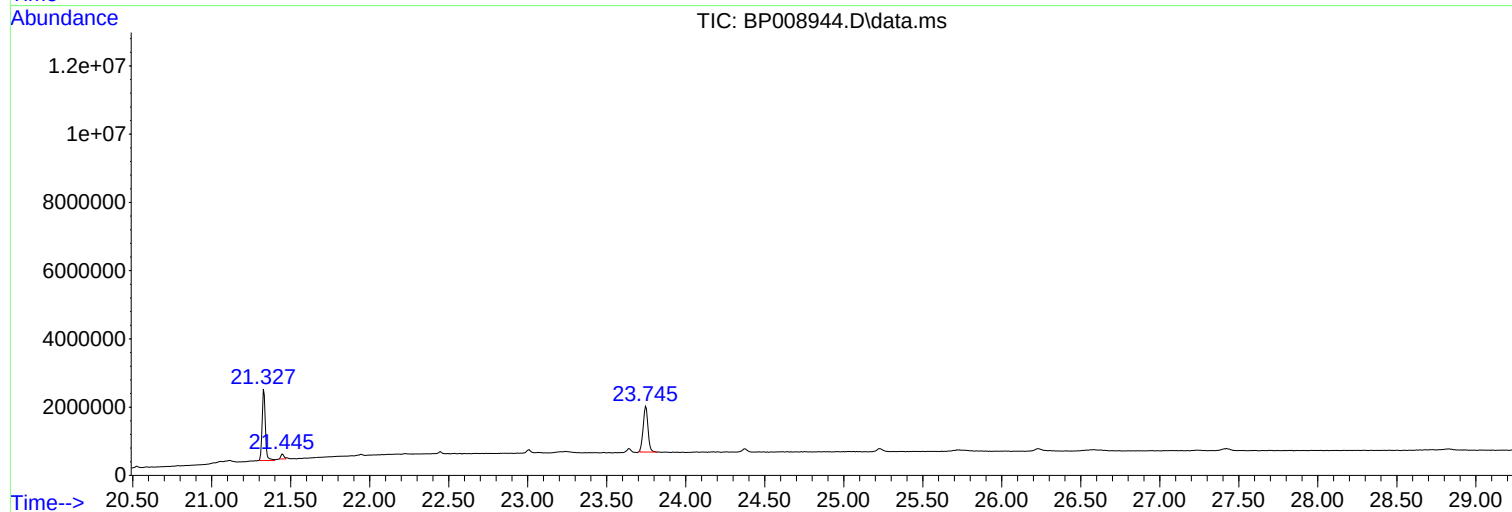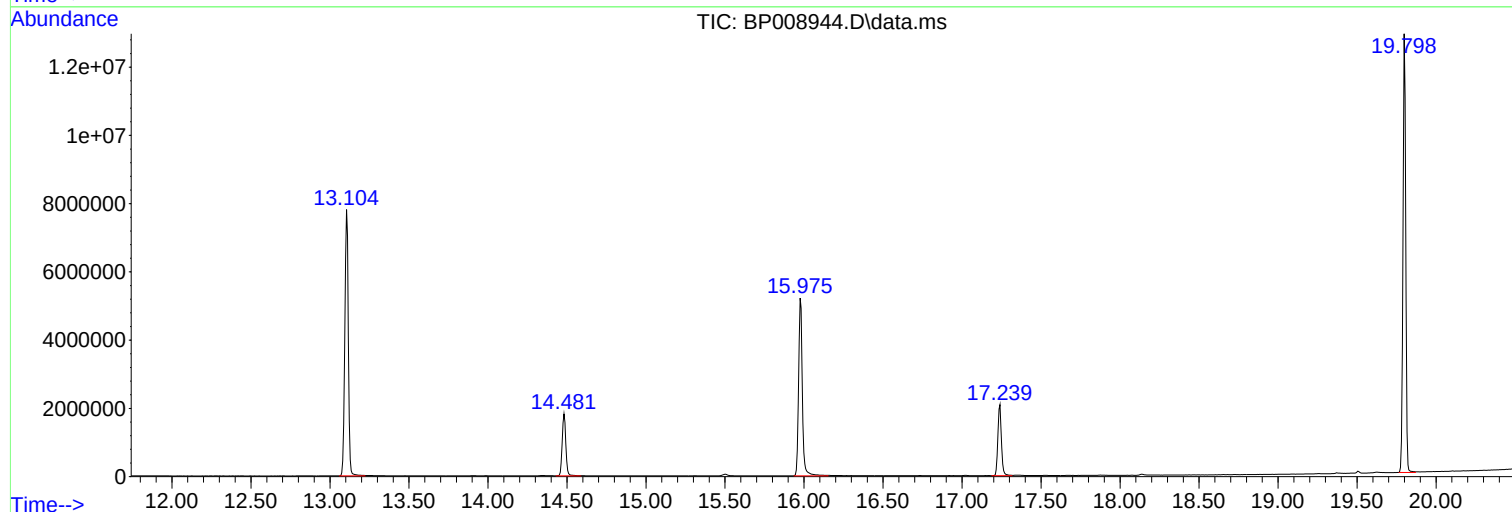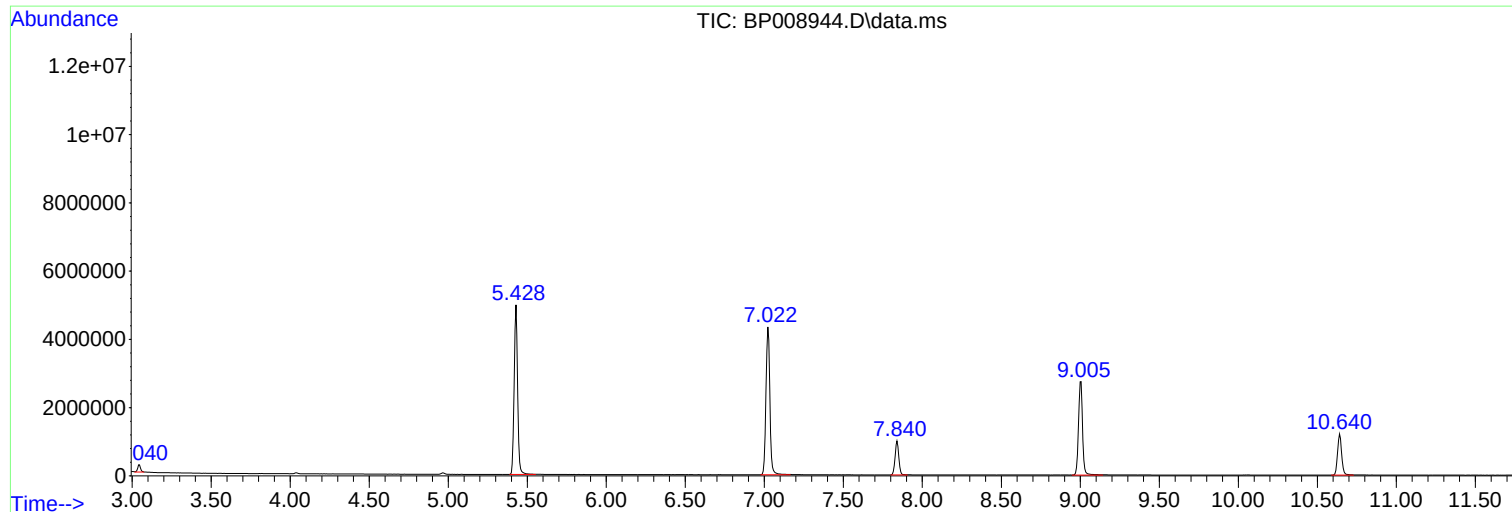

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008944.D
Acq On : 27 Jan 2022 13:12
Operator : CG/JU
Sample : PB142279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142279BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.040	3.40 ng	273432	1,4-Dichlorobenzene-d4	7.840

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	25
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23

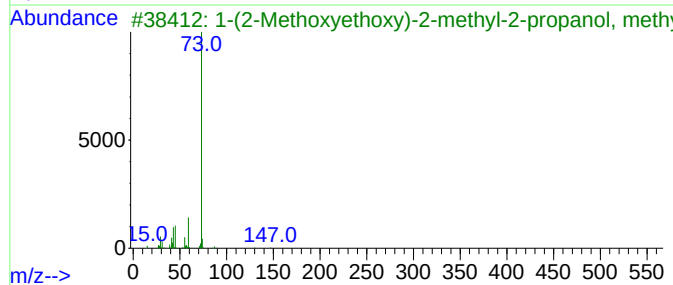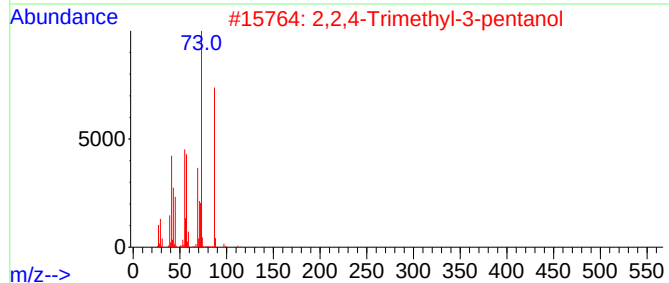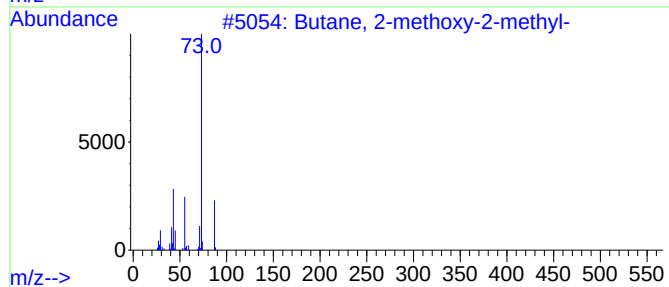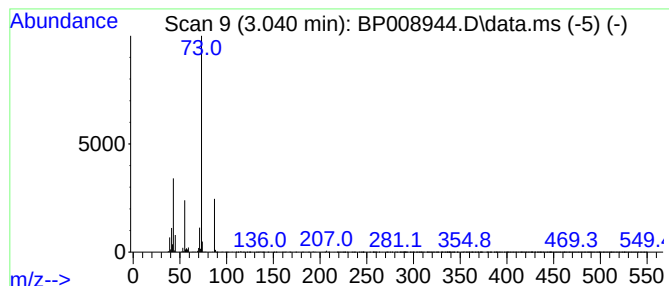

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008944.D
Acq On : 27 Jan 2022 13:12
Operator : CG/JU
Sample : PB142279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142279BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.040	3.4	ng	273432	1	7.840	1609070	20.0