

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008946.D
 Acq On : 27 Jan 2022 14:21
 Operator : CG/JU
 Sample : PB142303BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142303BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	21	rVB	218182	291576	1.99%	0.425%
2	5.422	407	414	435	rBV	4650504	7193577	49.11%	10.486%
3	7.016	677	685	704	rBV	4147925	7098094	48.46%	10.347%
4	7.834	817	824	839	rBV	946268	1550260	10.58%	2.260%
5	8.993	1012	1021	1046	rBV	2650756	4695418	32.06%	6.845%
6	10.634	1289	1300	1319	rBV	1173947	2122612	14.49%	3.094%
7	13.098	1711	1719	1734	rBV	7529735	11595367	79.16%	16.903%
8	14.475	1946	1953	1972	rBV	1749275	2779858	18.98%	4.052%
9	15.969	2199	2207	2231	rBV	4914526	8154431	55.67%	11.887%
10	17.228	2414	2421	2436	rBV	1929593	3103620	21.19%	4.524%
11	19.792	2851	2857	2871	rBV	11901005	14647403	100.00%	21.352%
12	21.321	3112	3117	3127	rBV	1992844	2713281	18.52%	3.955%
13	23.733	3521	3527	3540	rVB2	1236257	2653622	18.12%	3.868%




Sum of corrected areas: 68599119

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008946.D
Acq On : 27 Jan 2022 14:21
Operator : CG/JU
Sample : PB142303BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142303BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

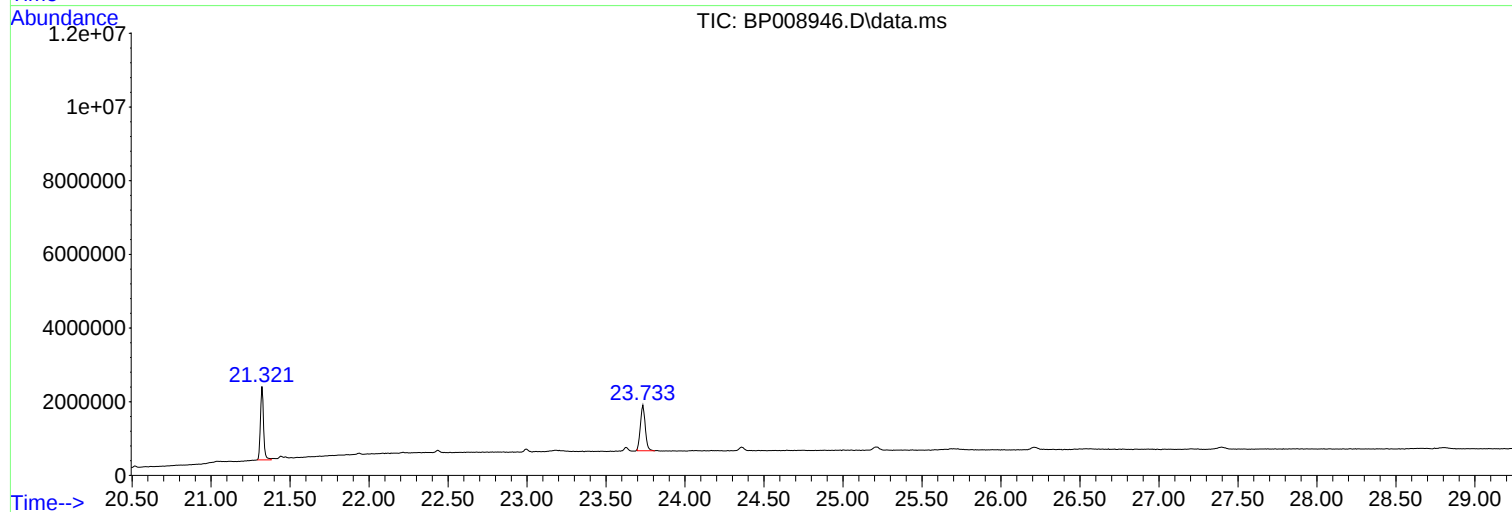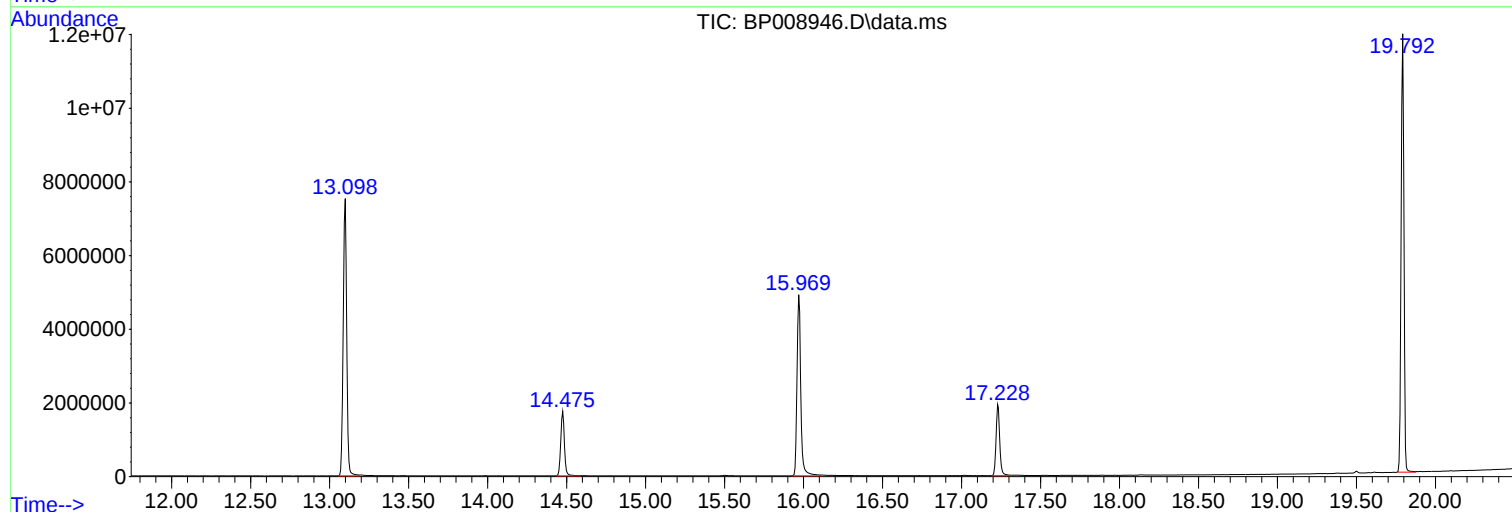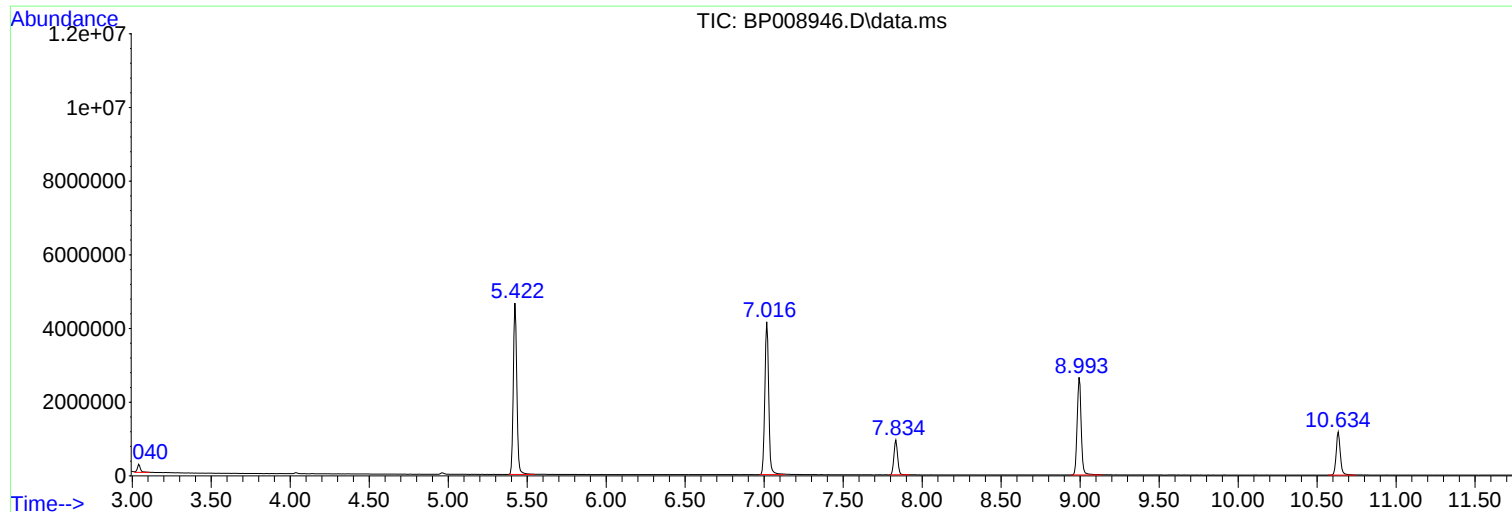

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008946.D
Acq On : 27 Jan 2022 14:21
Operator : CG/JU
Sample : PB142303BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142303BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.040	3.76 ng	291576	1,4-Dichlorobenzene-d4	7.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

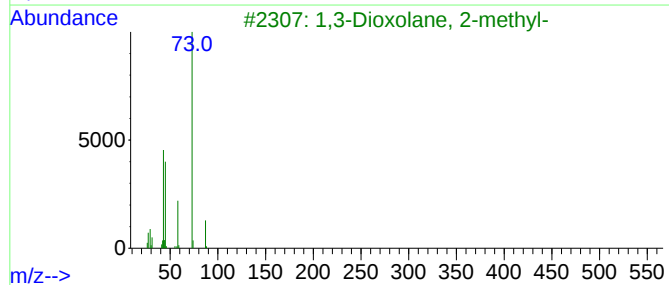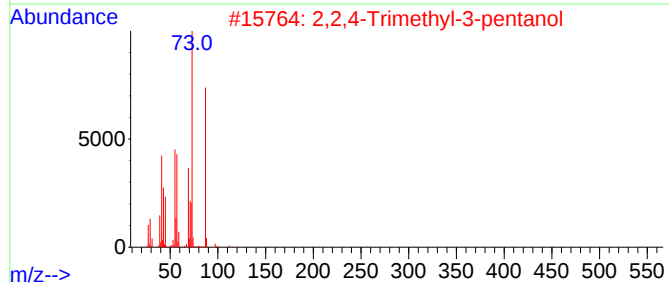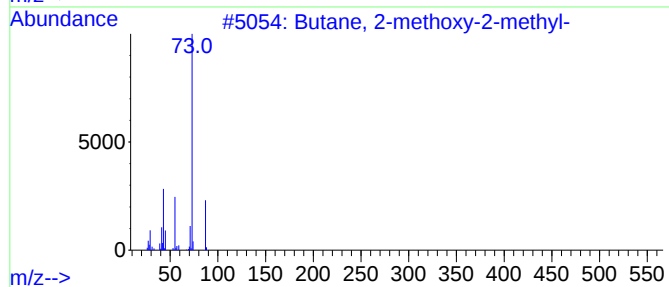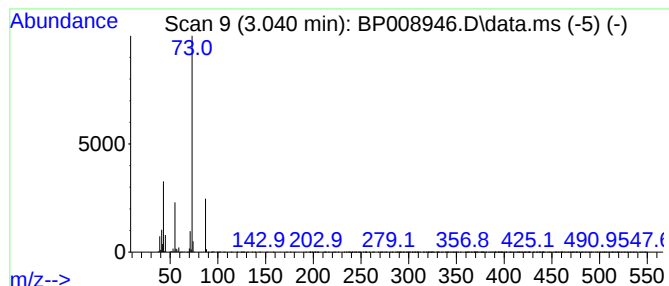

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
Data File : BP008946.D
Acq On : 27 Jan 2022 14:21
Operator : CG/JU
Sample : PB142303BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142303BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.040	3.8	ng	291576	1	7.834	1550260	20.0