
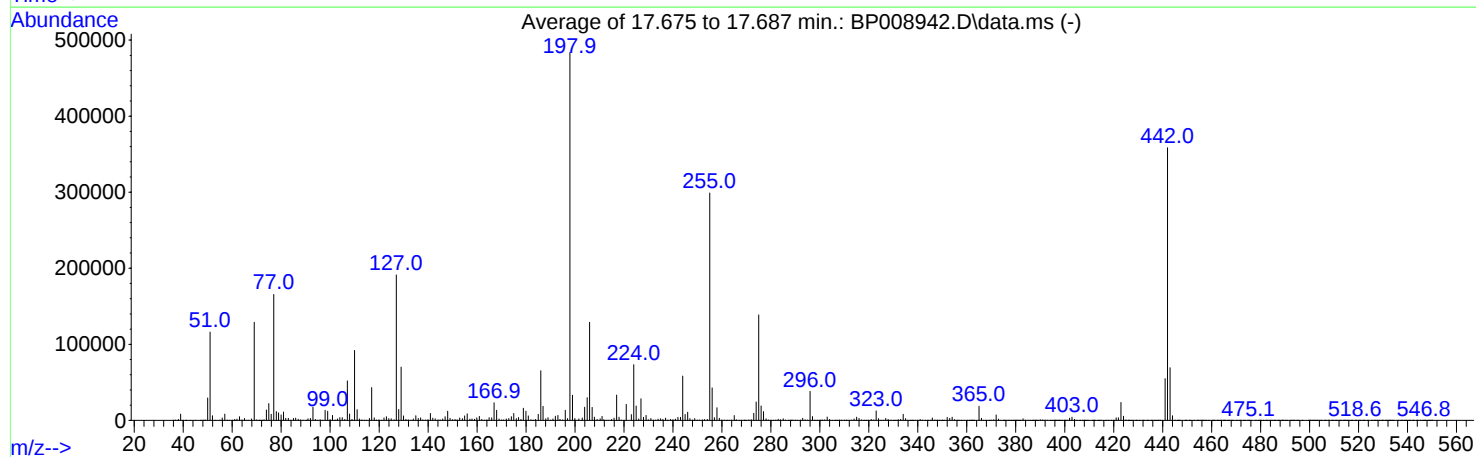


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008942.D
 Acq On : 27 Jan 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 26 01:52:51 2022

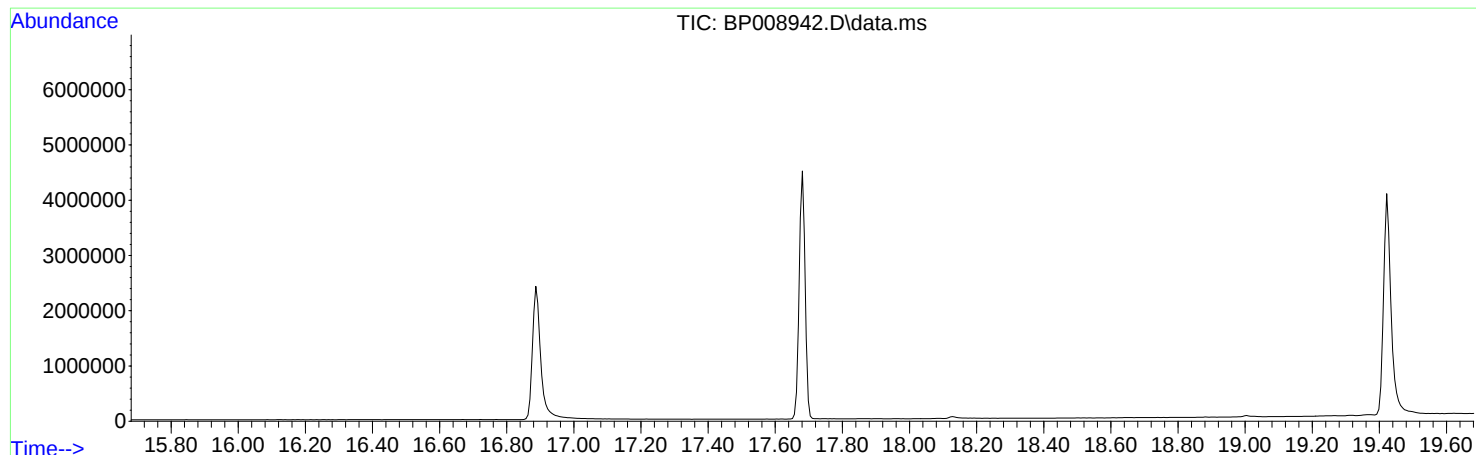




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	116161	PASS
68	69	0.00	2	1.5	1993	PASS
69	198	0.00	100	26.7	128997	PASS
70	69	0.00	2	0.5	659	PASS
127	198	10	80	39.5	191254	PASS
197	198	0.00	2	0.5	2314	PASS
198	198	100	100	100.0	483692	PASS
199	198	5	9	6.8	33023	PASS
275	198	10	60	28.7	138709	PASS
365	198	1	100	3.8	18433	PASS
441	198	0.01	100	11.4	54973	PASS
442	442	100	100	100.0	358507	PASS
443	442	15	24	19.3	69299	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008942.D
 Acq On : 27 Jan 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:03:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

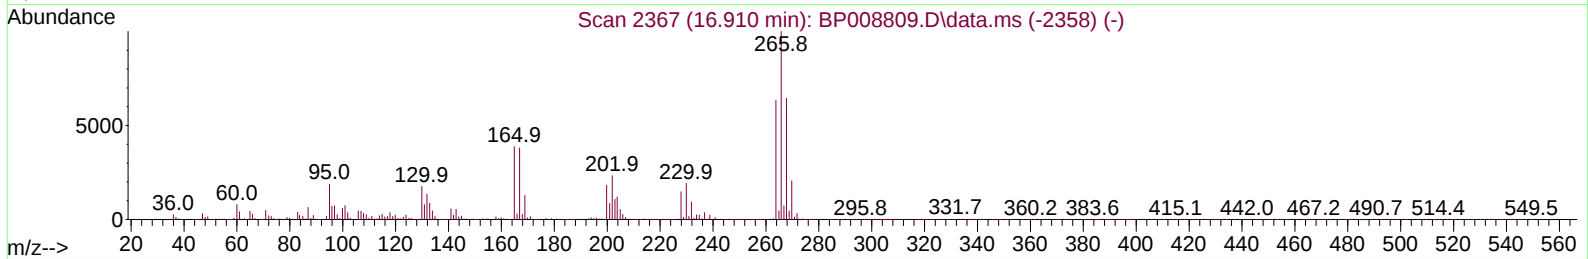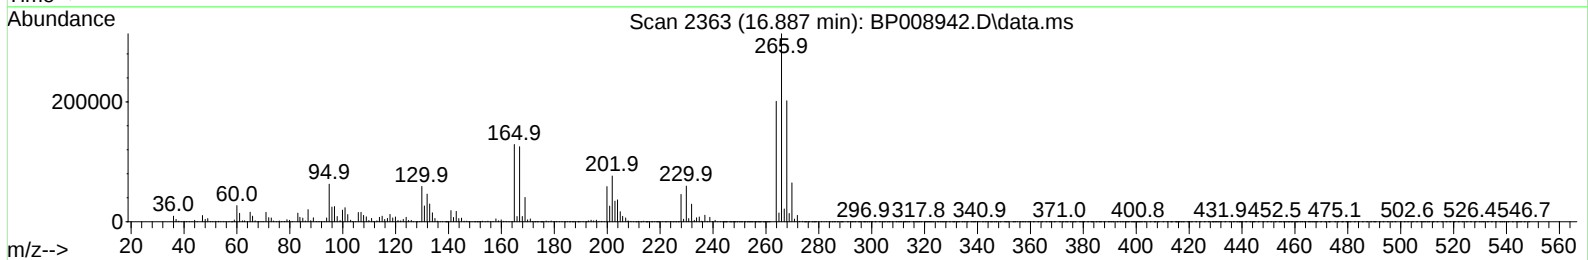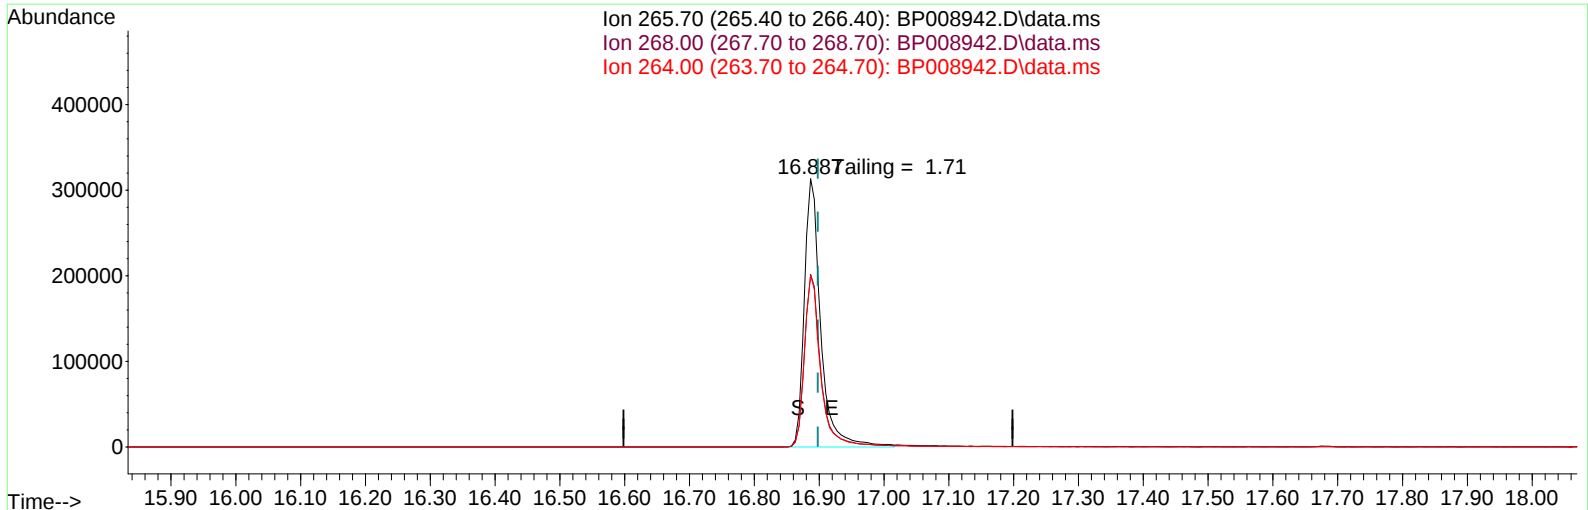

TIC: BP008942.D\data.ms

(70) Pentachlorophenol (C)

16.887min (-0.012) 183745.98 ng




response 557394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.36
264.00	62.90	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012722\
 Data File : BP008942.D
 Acq On : 27 Jan 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:03:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 01:52:51 2022
 Response via : Initial Calibration

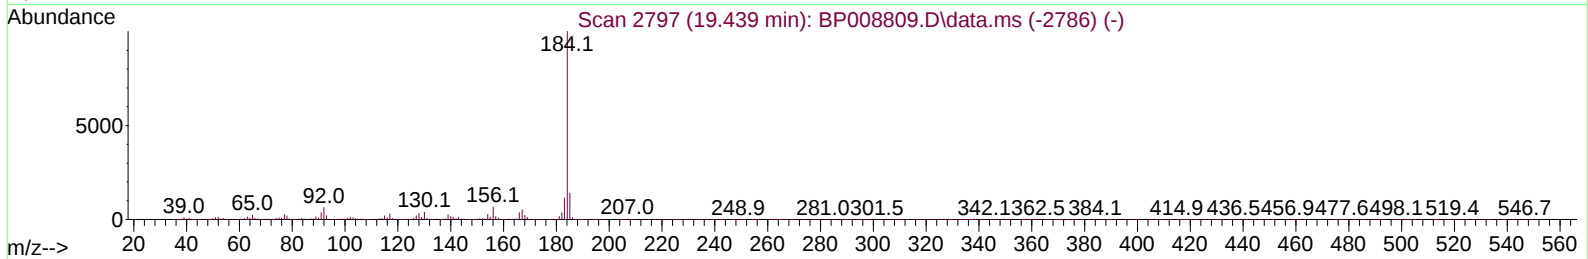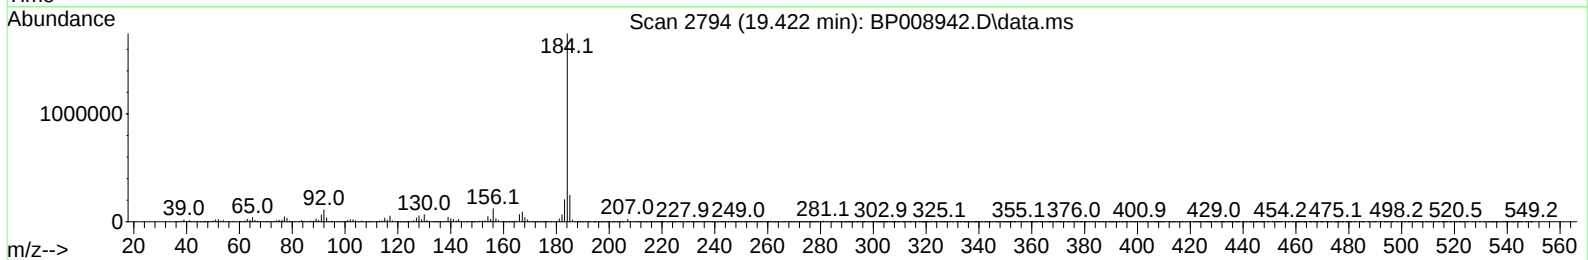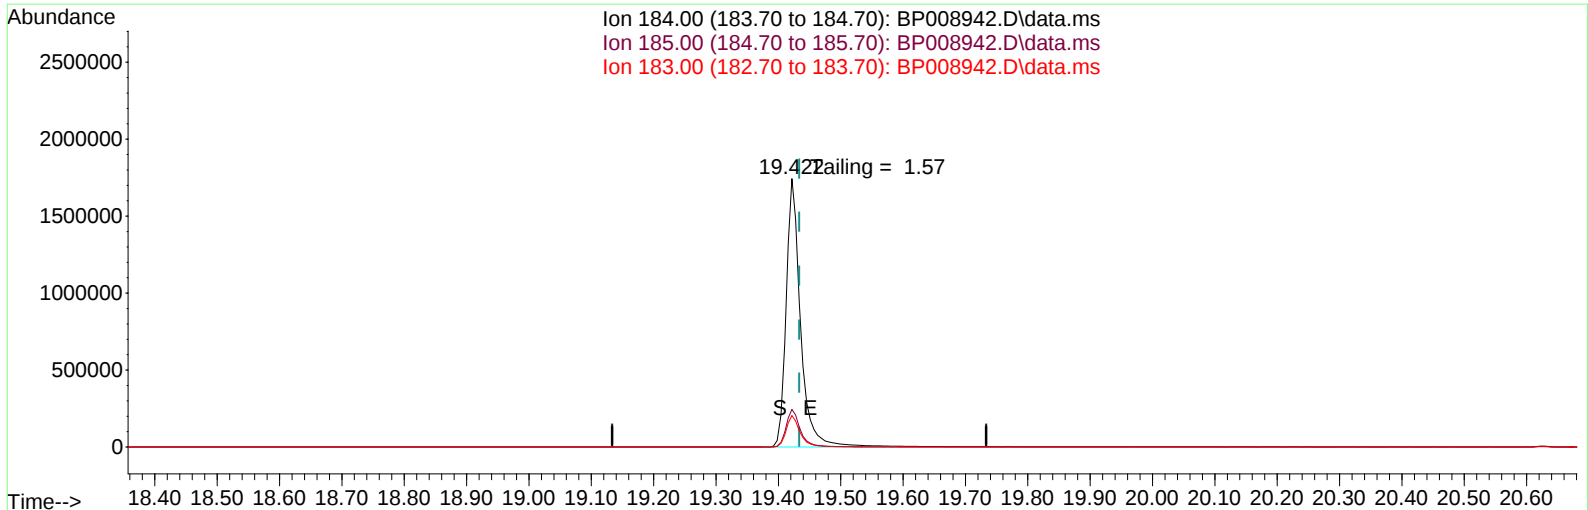

TIC: BP008942.D\data.ms

(77) Benzidine

19.422min (-0.012) 37887.15 ng

response 2824170

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.01
183.00	11.90	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2022	BNA_P	<u>BP008942.D</u>
Compound Name	Response	Retention Time
DDT	1633419	20.628
DDD	66705	20.198
DDE	6470	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
73175	1706594	4.29

Instrument :
BNA_P
ClientSampleId :
DFTPP