
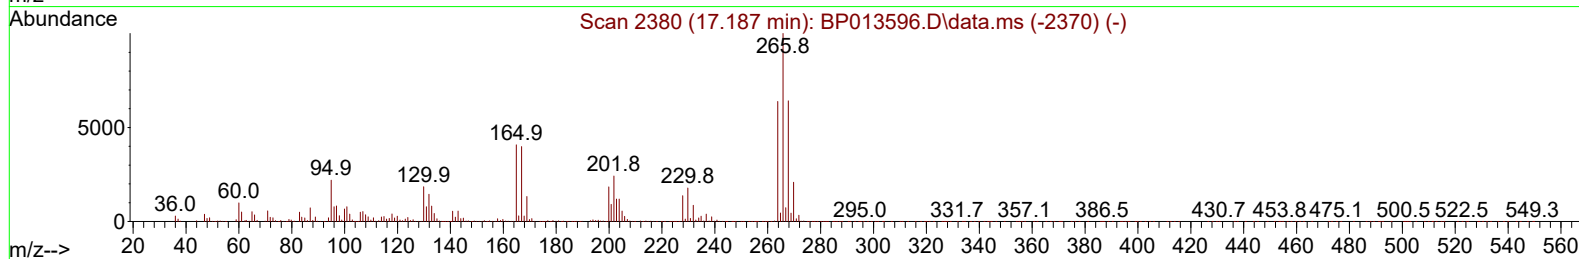
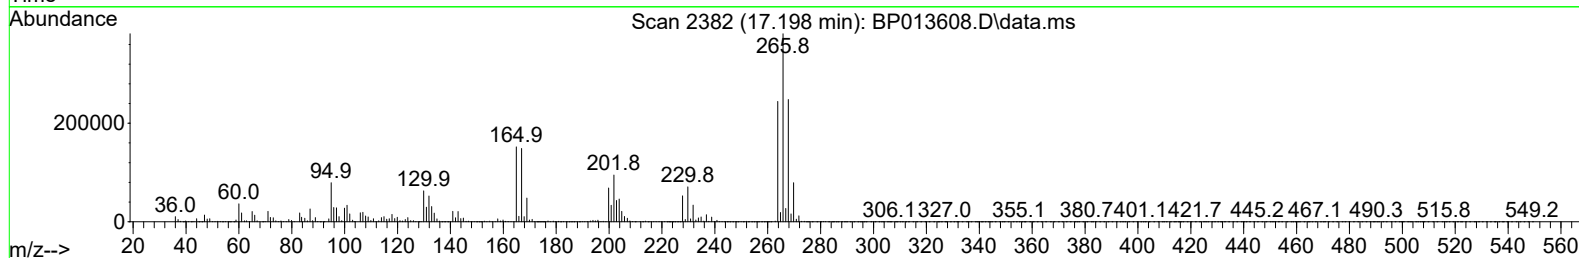


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP012723\  
Data File : BP013608.D  
Acq On : 27 Jan 2023 09:27  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:38:34 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP012623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 27 03:27:54 2023  
Response via : Initial Calibration

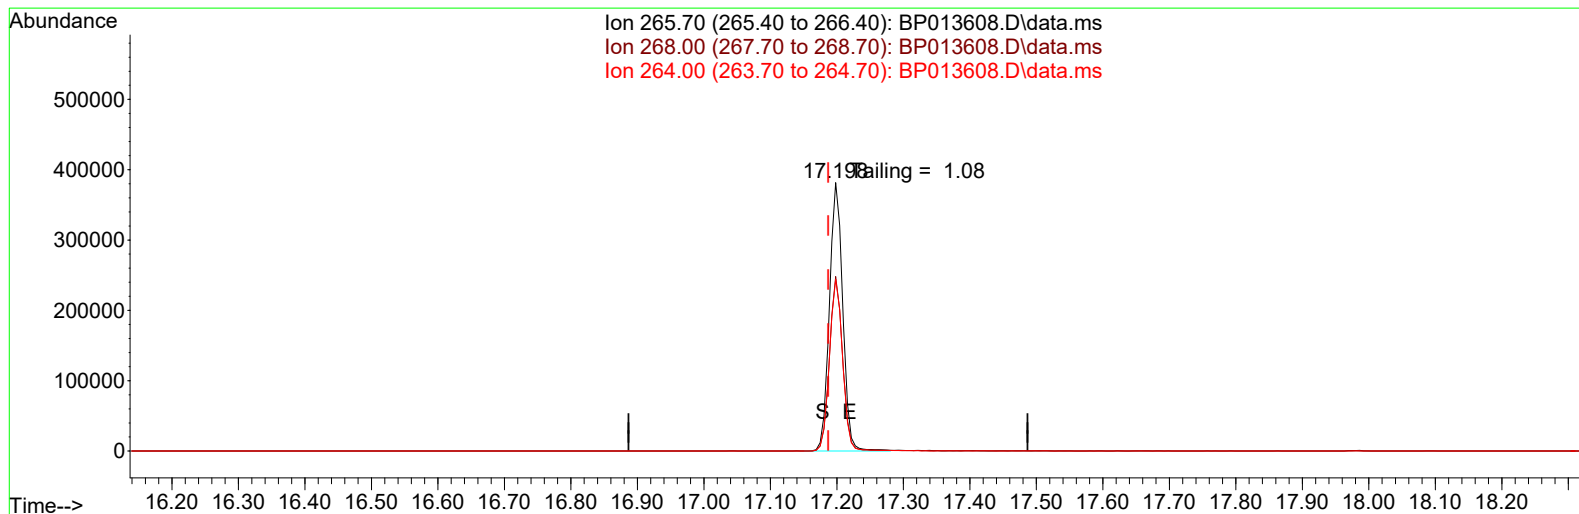

TIC: BP013608.D\data.ms

**(70) Pentachlorophenol (C)**




17.198min (+ 0.011) 293586.44 ng

response 531800

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.20  | 65.00  |
| 264.00 | 63.80  | 64.04  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP012723\  
Data File : BP013608.D  
Acq On : 27 Jan 2023 09:27  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:38:34 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP012623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 27 03:27:54 2023  
Response via : Initial Calibration

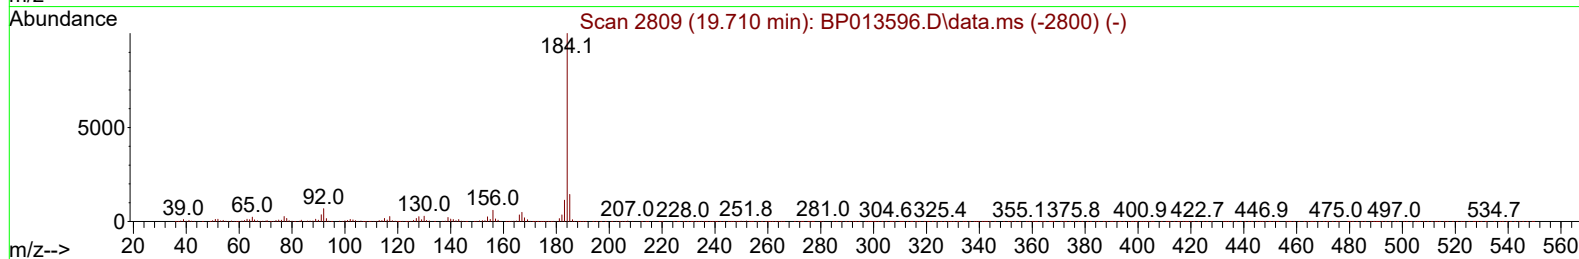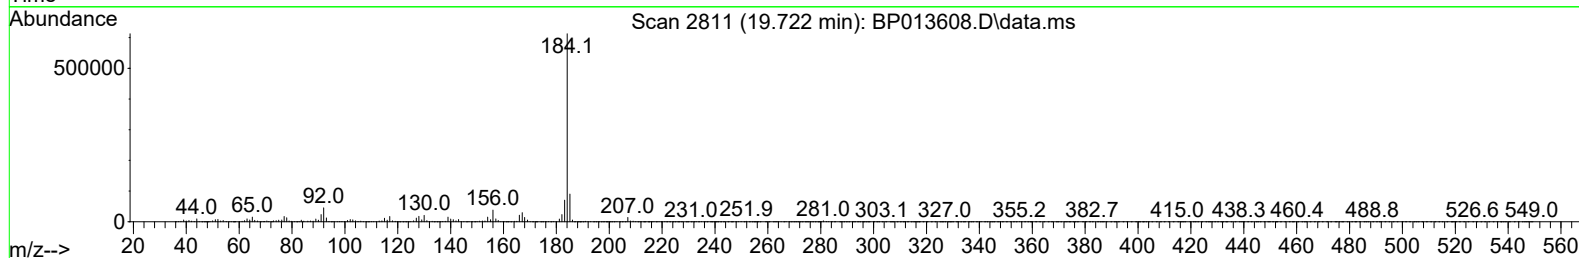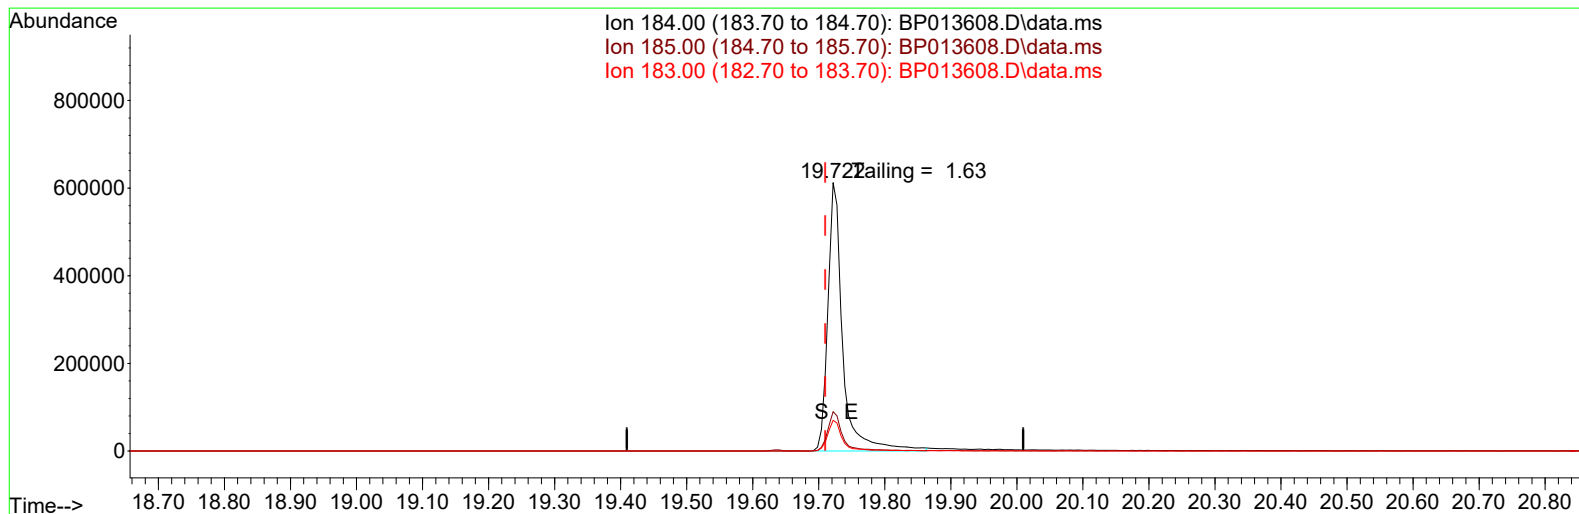

TIC: BP013608.D\data.ms

**(77) Benzidine****19.722min (+ 0.012) 5599.63 ng****response 949317**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.69  |
| 183.00 | 11.30  | 11.48  |
| 0.00   | 0.00   | 0.00   |