


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
 Data File : BP013608.D
 Acq On : 27 Jan 2023 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 27 03:27:54 2023

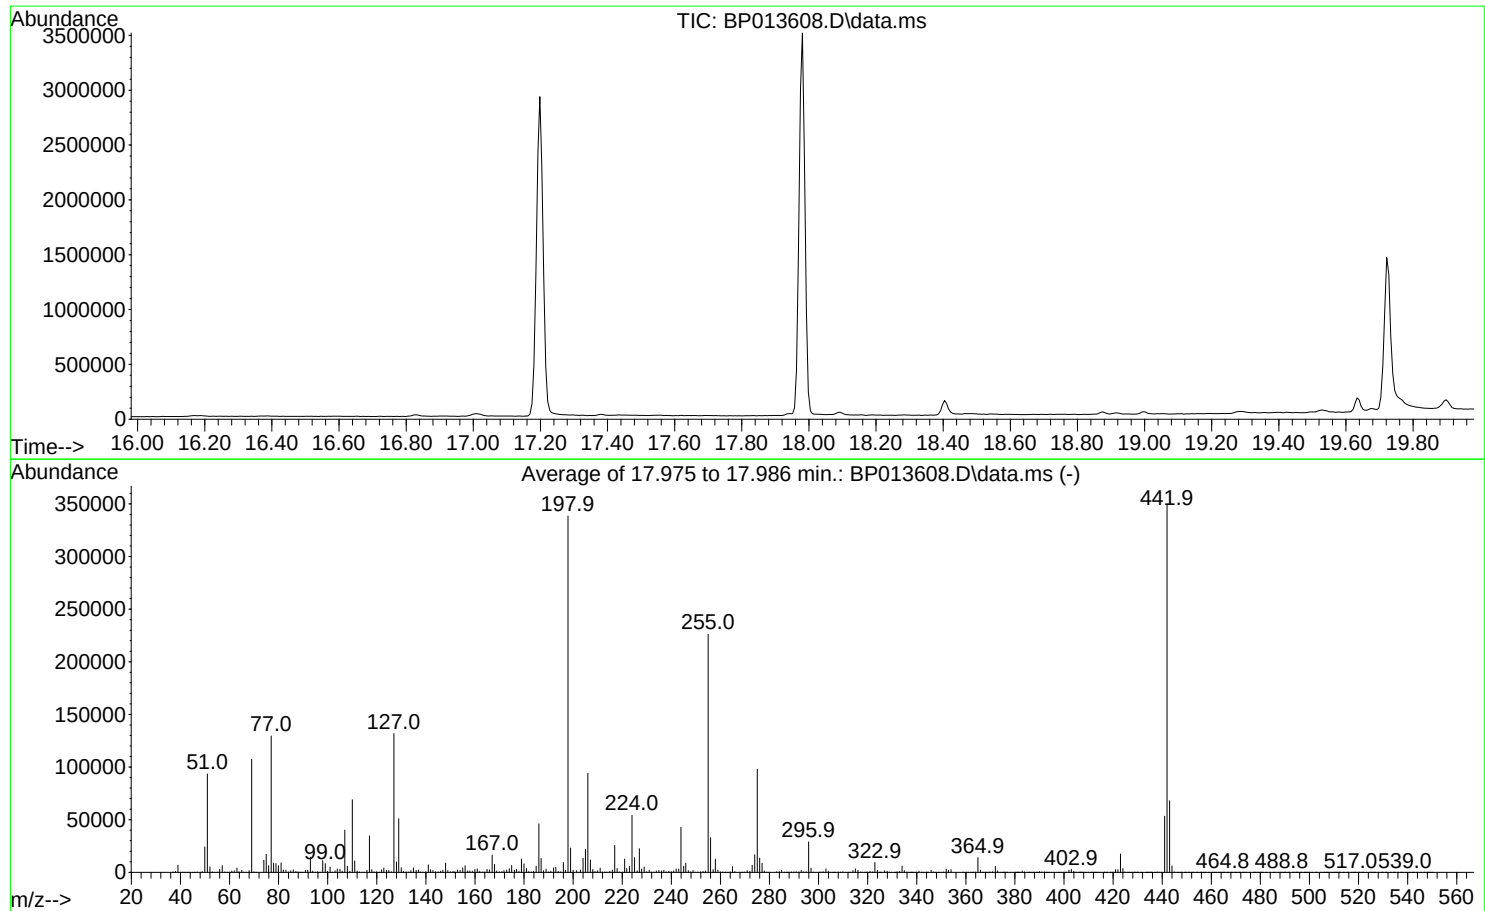




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	93380	PASS
68	69	0.00	2	1.5	1578	PASS
69	198	0.00	100	31.7	107389	PASS
70	69	0.00	2	0.5	586	PASS
127	198	10	80	38.9	131753	PASS
197	198	0.00	2	0.5	1705	PASS
198	198	100	100	100.0	338529	PASS
199	198	5	9	6.8	23013	PASS
275	198	10	60	28.9	97763	PASS
365	198	1	100	4.1	13903	PASS
441	198	0.01	100	15.7	53280	PASS
442	442	100	100	100.0	349510	PASS
443	442	15	24	19.5	68096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
 Data File : BP013608.D
 Acq On : 27 Jan 2023 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 05:38:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 03:27:54 2023
 Response via : Initial Calibration

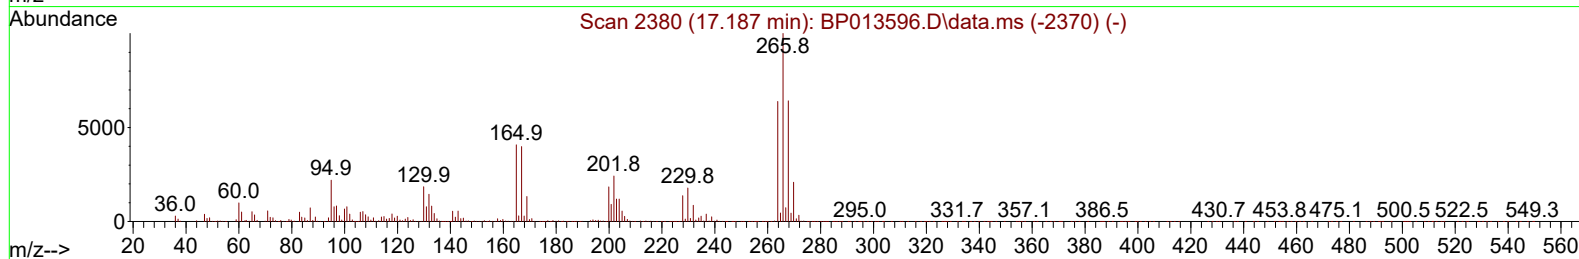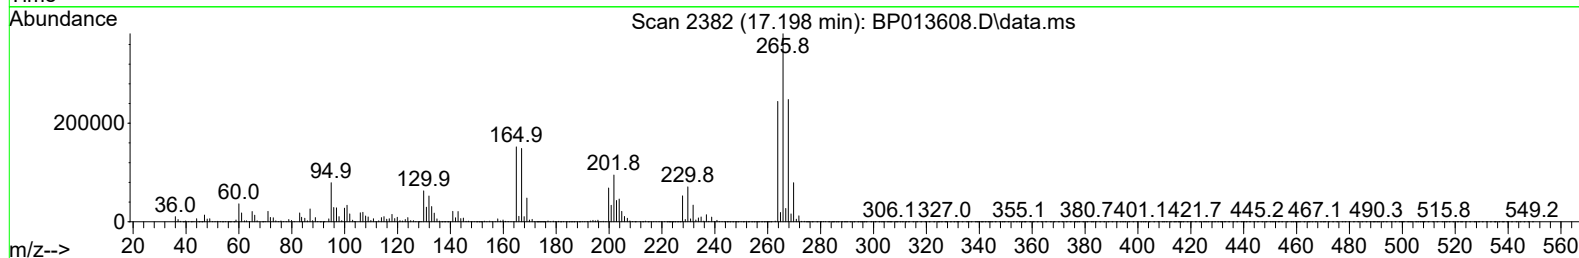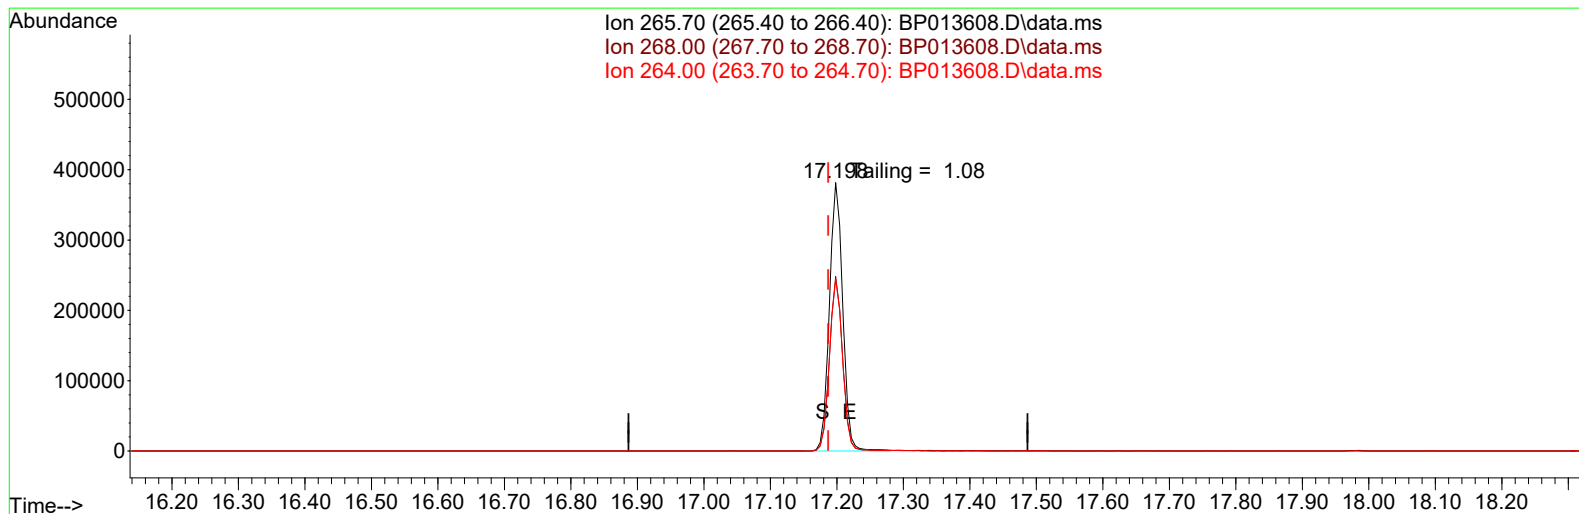

TIC: BP013608.D\data.ms

(70) Pentachlorophenol (C)

17.198min (+ 0.011) 293586.44 ng




response 531800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.00
264.00	63.80	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
Data File : BP013608.D
Acq On : 27 Jan 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 28 05:38:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 03:27:54 2023
Response via : Initial Calibration

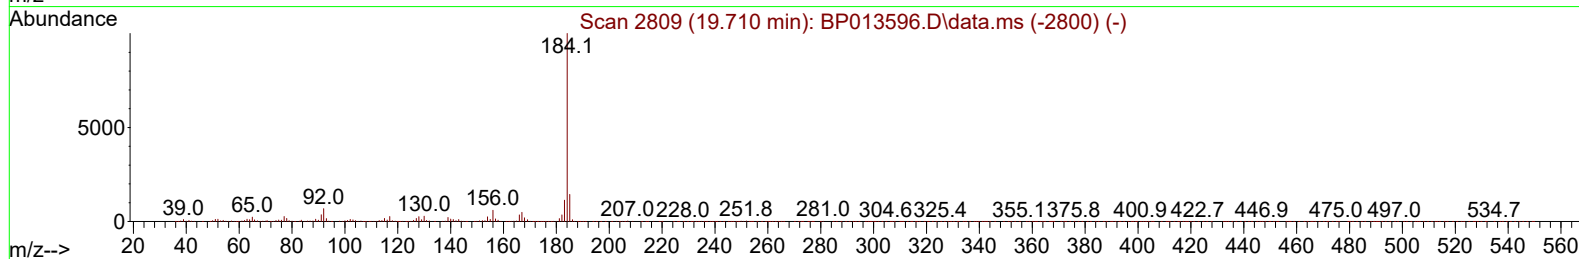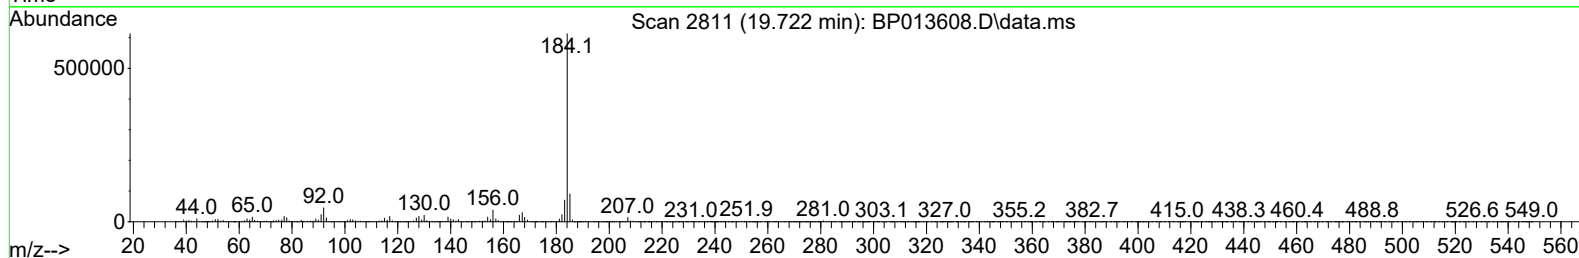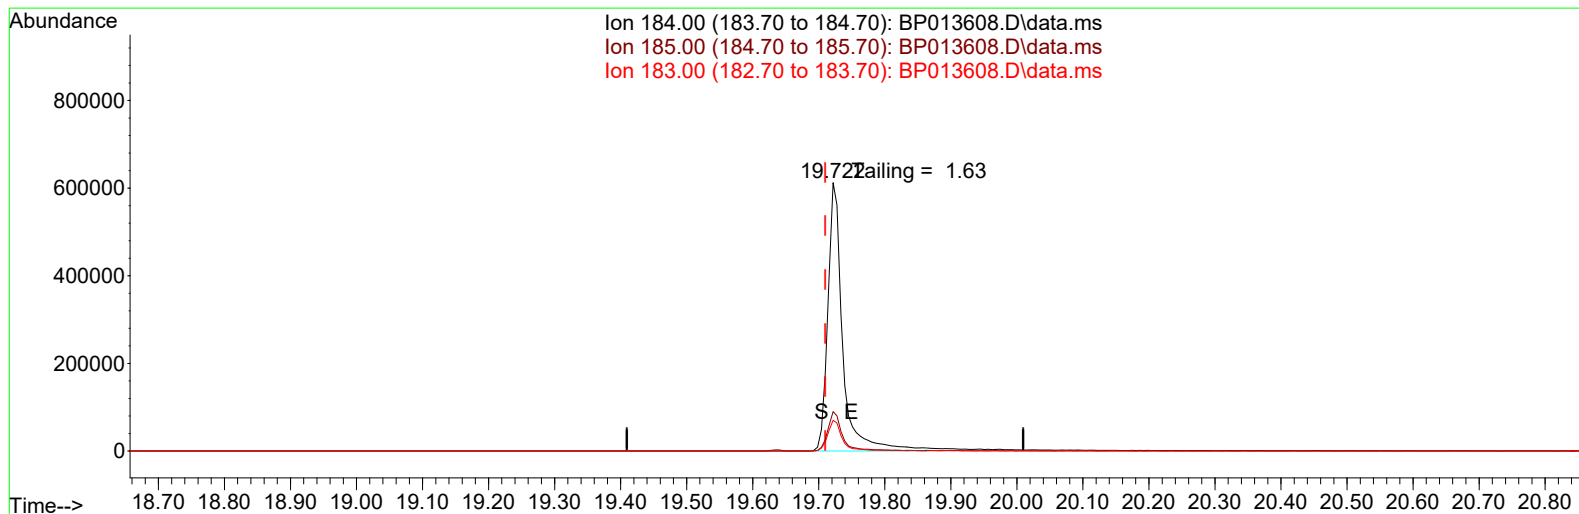

TIC: BP013608.D\data.ms

(77) Benzidine

19.722min (+ 0.012) 5599.63 ng

response 949317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.69
183.00	11.30	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_P	<u>BP013608.D</u>
Compound Name	Response	Retention Time
DDT	564523	20.922
DDD	11099	20.492
DDE	2382	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13481	578004	2.33

Instrument :
BNA_P
ClientSampleId :
DFTPP