


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
 Data File : BP013618.D
 Acq On : 27 Jan 2023 15:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 27 03:27:54 2023

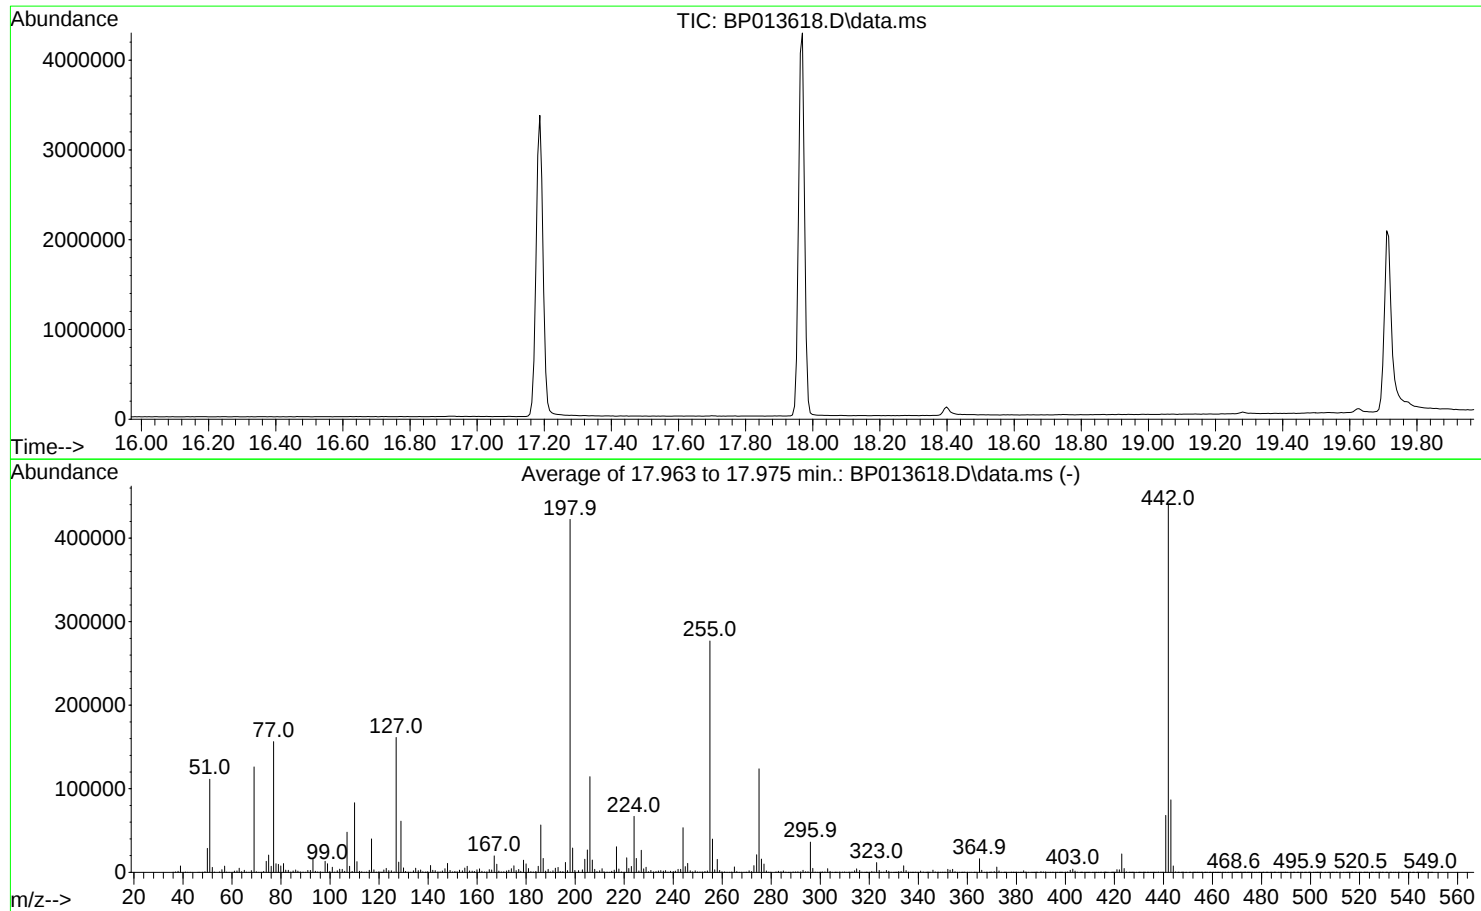




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	111413	PASS
68	69	0.00	2	1.6	2028	PASS
69	198	0.00	100	29.9	126071	PASS
70	69	0.00	2	0.6	741	PASS
127	198	10	80	38.2	161357	PASS
197	198	0.00	2	0.5	2035	PASS
198	198	100	100	100.0	422337	PASS
199	198	5	9	6.9	29032	PASS
275	198	10	60	29.3	123851	PASS
365	198	1	100	3.8	16229	PASS
441	198	0.01	100	16.1	68178	PASS
442	442	100	100	100.0	440334	PASS
443	442	15	24	19.7	86600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
 Data File : BP013618.D
 Acq On : 27 Jan 2023 15:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 05:41:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 03:27:54 2023
 Response via : Initial Calibration

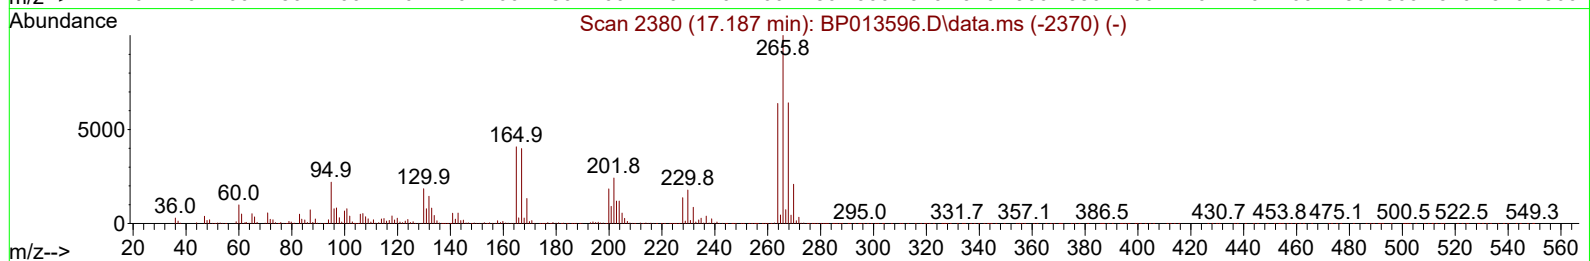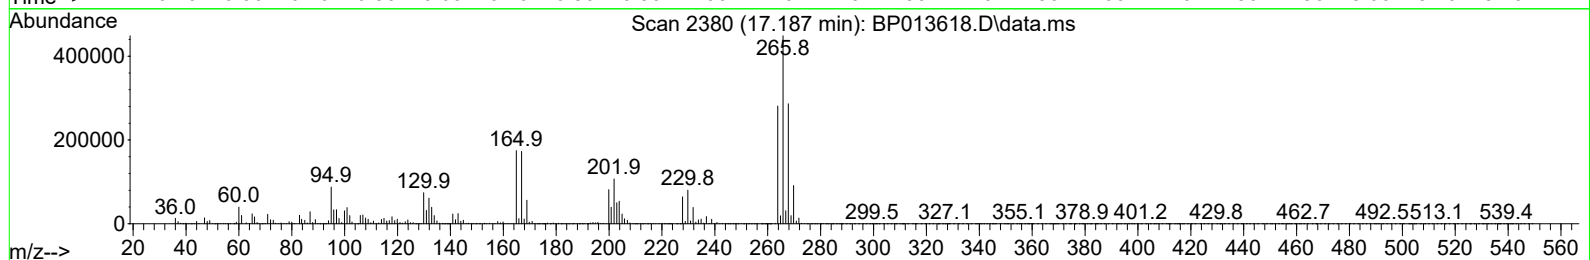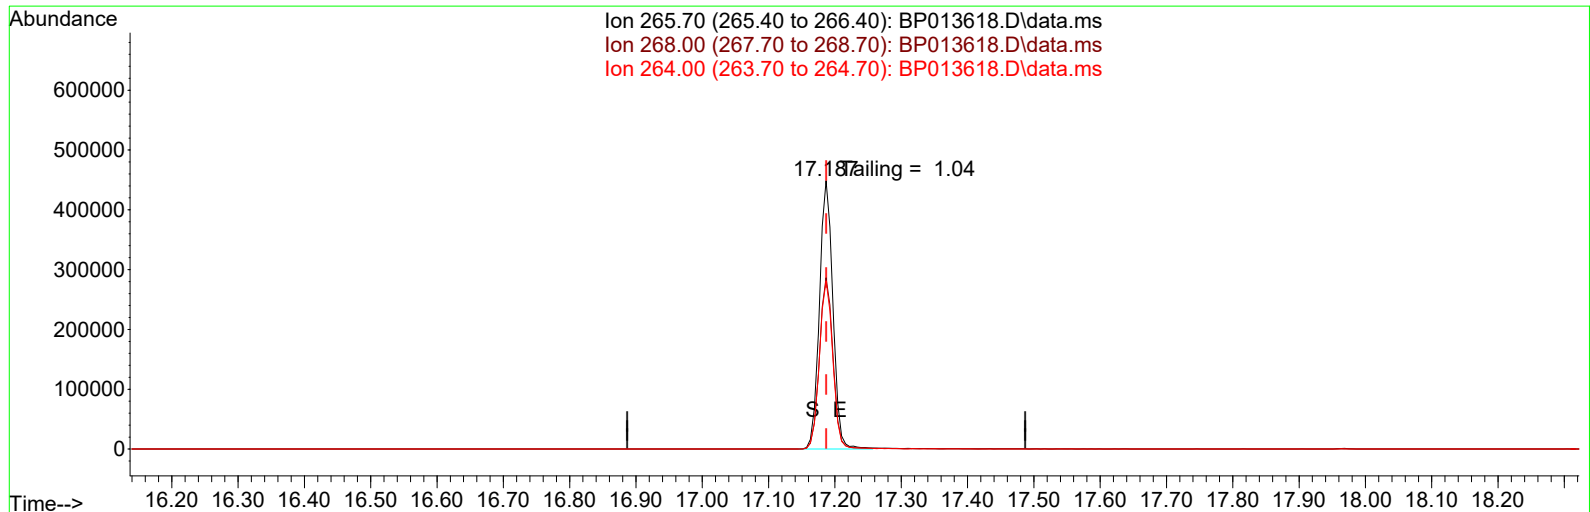

TIC: BP013618.D\data.ms

(70) Pentachlorophenol (C)

17.187min (-0.000) 347721.10 ng




response 640073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.82
264.00	63.80	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012723\
Data File : BP013618.D
Acq On : 27 Jan 2023 15:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 28 05:41:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 03:27:54 2023
Response via : Initial Calibration

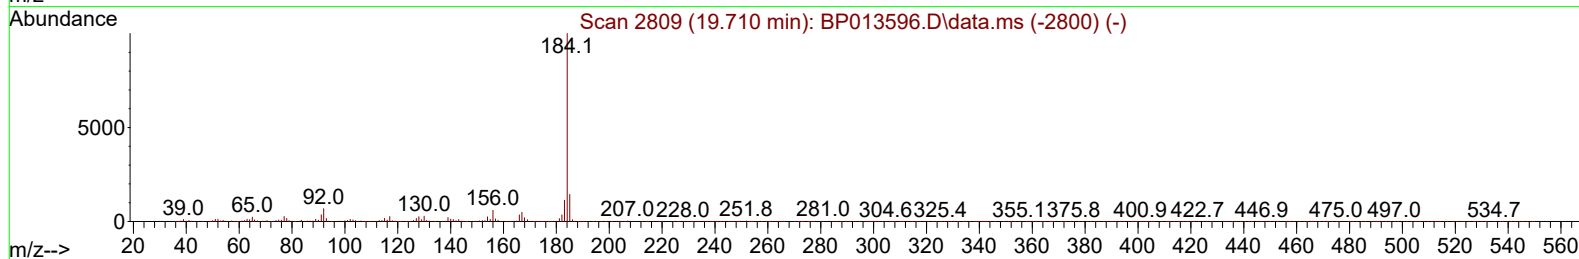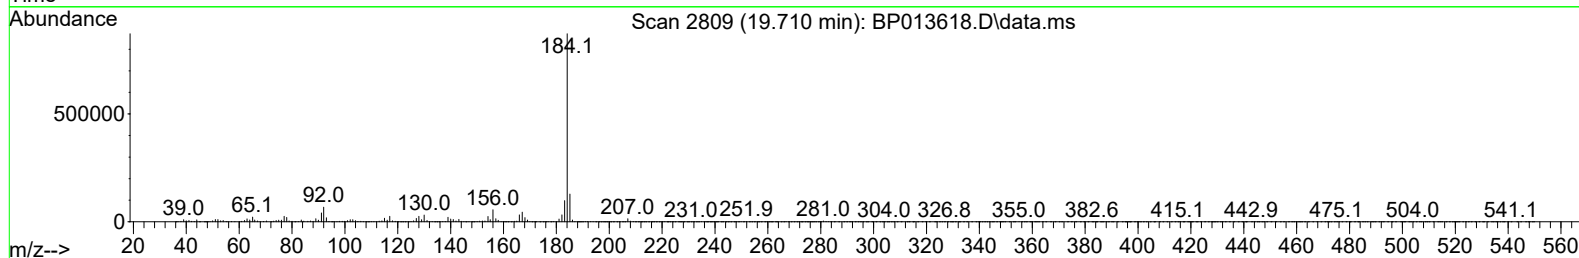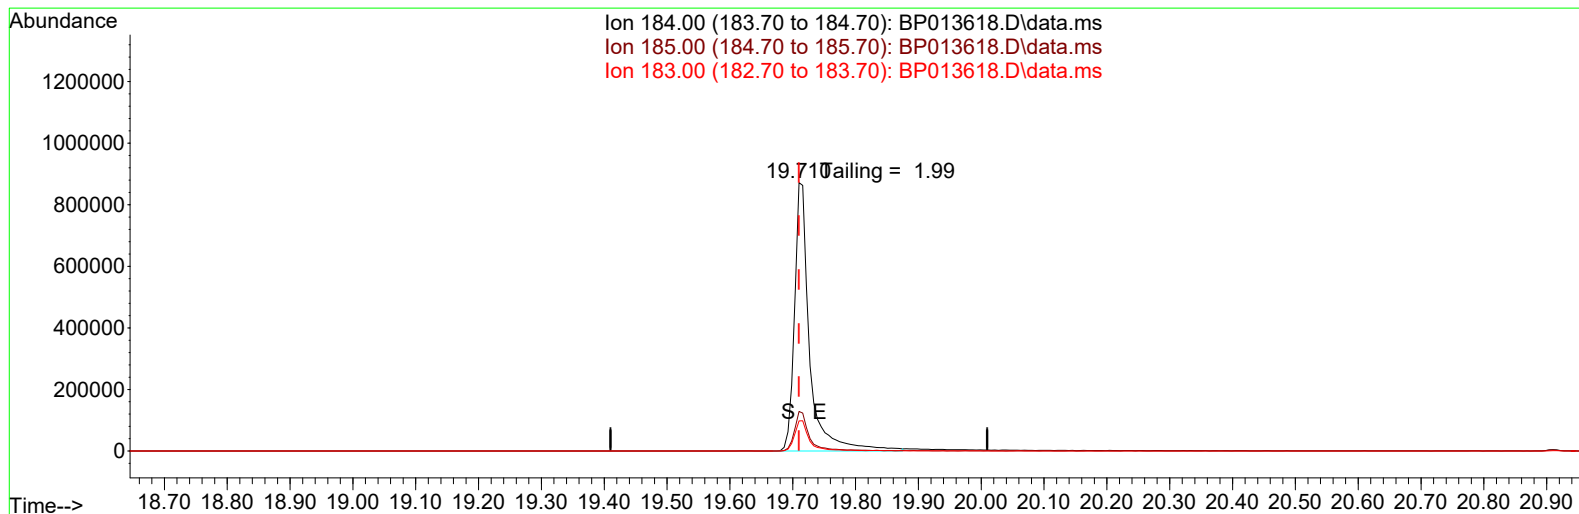

TIC: BP013618.D\data.ms

(77) Benzidine

19.710min (+ 0.000) 1399957.32 ng

response 1497121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.75
183.00	11.30	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_P	<u>BP013618.D</u>
Compound Name	Response	Retention Time
DDT	726813	20.91
DDD	11645	20.481
DDE	2021	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13666	740479	1.85

Instrument :
BNA_P
ClientSampleId :
DFTPP