
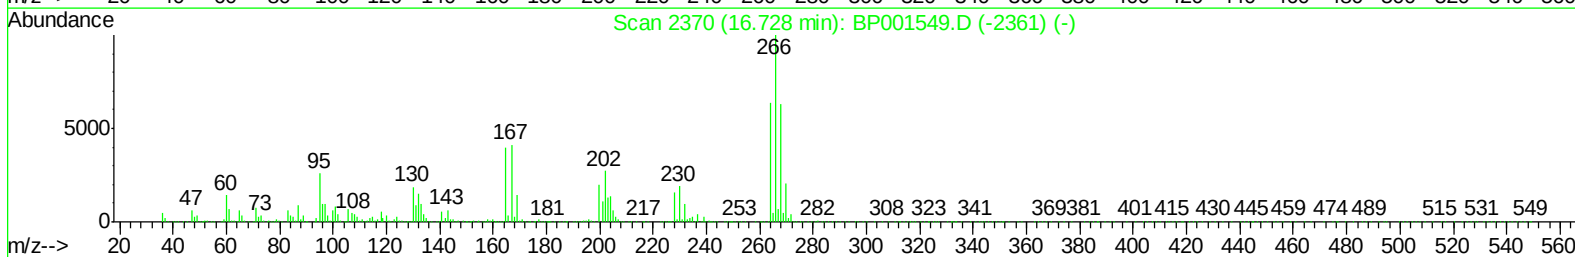
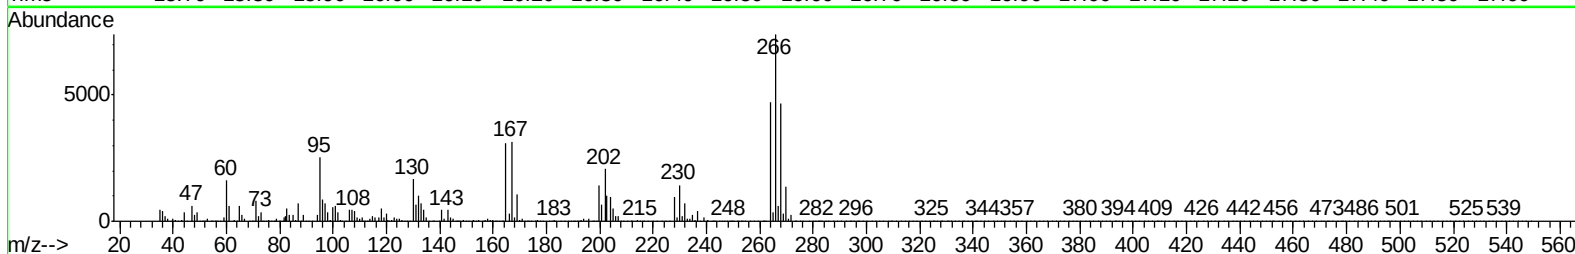


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP012820\
Data File : BP001699.D
Acq On : 28 Jan 2020 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 23:33:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 24 22:23:46 2020
Response via : Initial Calibration

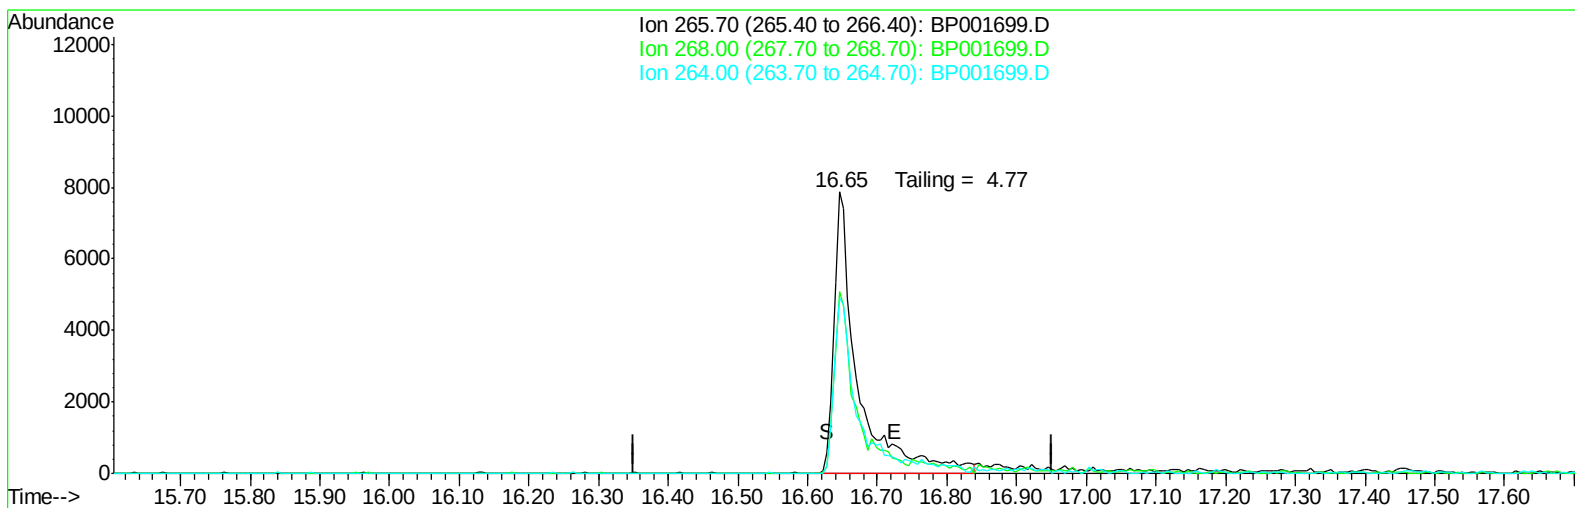

TIC: BP001699.D

(70) Pentachlorophenol (C)




16.651min (-16.651) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.10	0.00#
264.00	63.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP012820\
 Data File : BP001699.D
 Acq On : 28 Jan 2020 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 23:33:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 24 22:23:46 2020
 Response via : Initial Calibration

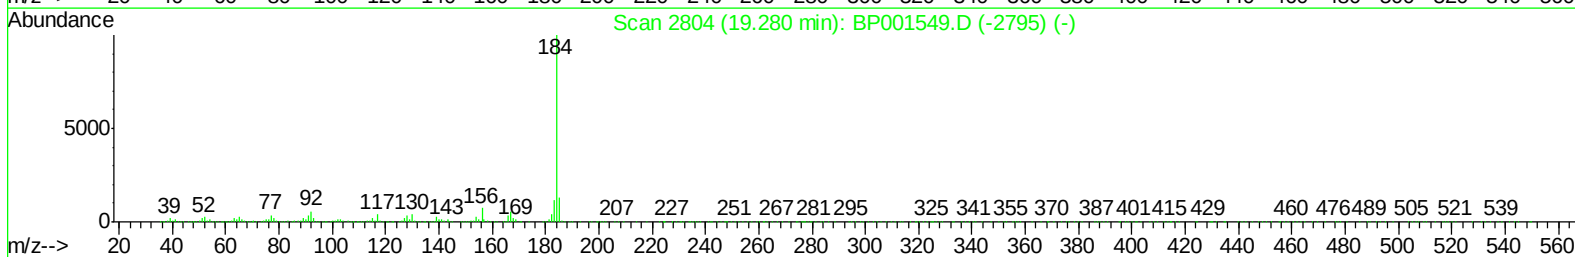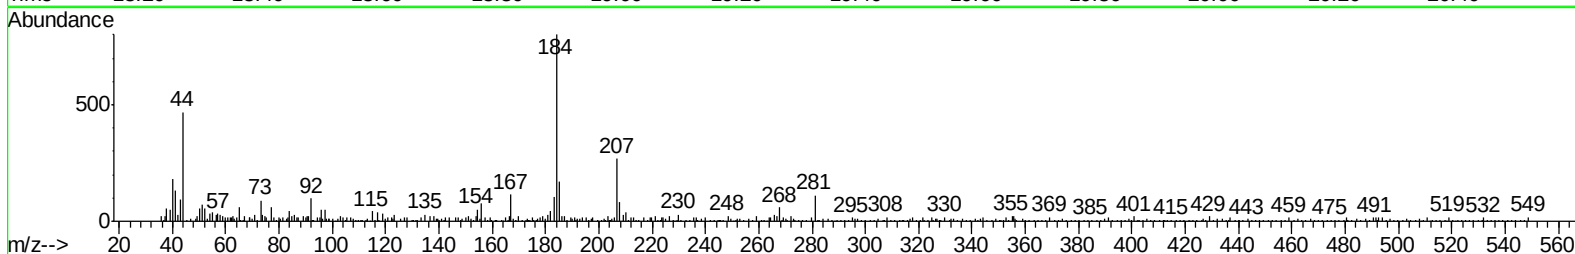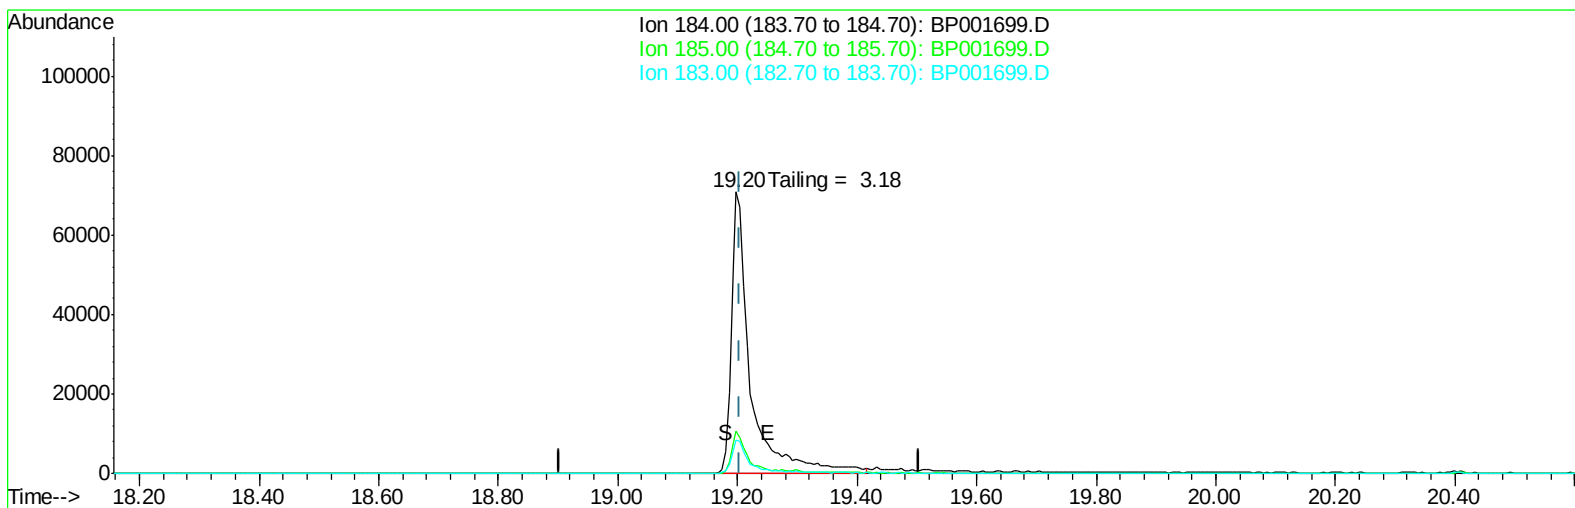

TIC: BP001699.D

(77) Benzidine

19.545min (+0.341) 2240.29ng

response 665

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	21.45#
183.00	11.70	12.84
0.00	0.00	0.00