


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012820\
 Data File : BP001699.D
 Acq On : 28 Jan 2020 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 24 22:23:46 2020

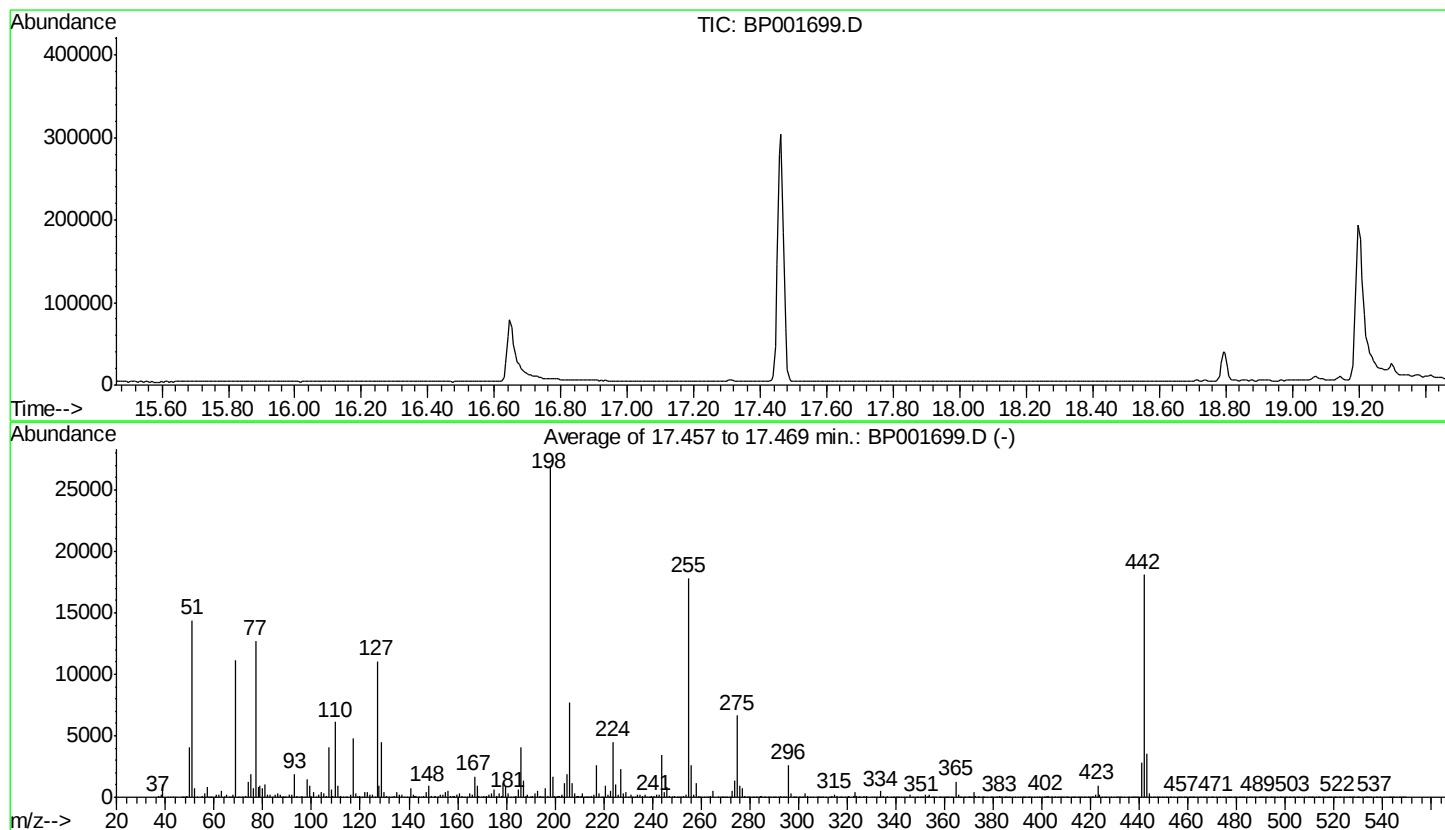

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	14383	PASS
68	69	0.00	2	1.6	184	PASS
69	198	0.00	100	41.4	11159	PASS
70	69	0.00	2	0.1	11	PASS
127	198	10	80	40.9	11036	PASS
197	198	0.00	2	0.4	105	PASS
198	198	100	100	100.0	26962	PASS
199	198	5	9	6.2	1685	PASS
275	198	10	60	24.7	6658	PASS
365	198	1	100	4.7	1277	PASS
441	198	0.01	100	10.6	2865	PASS
442	198	50	100	67.1	18094	PASS
443	442	15	24	19.3	3495	PASS