

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012821\
 Data File : BP004657.D
 Acq On : 28 Jan 2021 10:24
 Operator : CG/JU
 Sample : PB134337BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK337

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP012221.M
 Title : SVOA CALIBRATION

Signal : TIC: BP004657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	11	14	22	rVB2	10777	15811	1.08%	0.117%
2	3.364	28	30	33	rBV4	1782	2333	0.16%	0.017%
3	3.393	33	35	38	rVB3	1805	2035	0.14%	0.015%
4	3.681	81	84	101	rBV	133353	222782	15.27%	1.642%
5	3.834	108	110	114	rVB5	1504	1478	0.10%	0.011%
6	4.005	135	139	144	rVB7	2714	5127	0.35%	0.038%
7	5.810	443	446	449	rBV5	1065	1530	0.10%	0.011%
8	6.181	505	509	511	rBV4	1878	2608	0.18%	0.019%
9	6.334	533	535	536	rBV2	1482	1472	0.10%	0.011%
10	6.475	555	559	563	rBV5	1810	2570	0.18%	0.019%
11	6.852	620	623	627	rBV5	1146	1885	0.13%	0.014%
12	6.952	633	640	649	rBV	216626	333936	22.89%	2.461%
13	7.122	663	669	680	rBV	137747	220450	15.11%	1.625%
14	7.322	695	703	710	rBV	216521	337789	23.15%	2.489%
15	7.787	773	782	792	rVB	167593	269218	18.45%	1.984%
16	8.493	894	902	911	rBV	251045	388435	26.63%	2.863%
17	8.946	971	979	989	rBV	198574	320243	21.95%	2.360%
18	9.246	1025	1030	1032	rVB5	1077	1579	0.11%	0.012%
19	9.663	1092	1101	1110	rBV	172819	286105	19.61%	2.109%
20	10.198	1183	1192	1201	rBV	273769	451543	30.95%	3.328%
21	10.587	1246	1258	1266	rVB	203067	339634	23.28%	2.503%
22	10.722	1271	1281	1289	rBV	238366	404268	27.71%	2.979%
23	11.134	1347	1351	1354	rBV5	871	1562	0.11%	0.012%
24	11.410	1395	1398	1402	rBV6	1196	1512	0.10%	0.011%
25	11.657	1436	1440	1444	rVB7	1154	1715	0.12%	0.013%
26	12.092	1510	1514	1517	rBV6	936	1528	0.10%	0.011%
27	12.175	1522	1528	1536	rVV7	5025	9099	0.62%	0.067%
28	12.692	1611	1616	1617	rBV4	1069	1539	0.11%	0.011%
29	13.016	1668	1671	1673	rBV4	1311	1728	0.12%	0.013%
30	13.057	1673	1678	1680	rVB5	1497	2186	0.15%	0.016%
31	13.169	1694	1697	1701	rBV5	1345	2295	0.16%	0.017%
32	13.739	1789	1794	1795	rBV5	1020	1742	0.12%	0.013%
33	13.845	1806	1812	1820	rBV	519608	717388	49.18%	5.287%
34	14.128	1853	1860	1869	rBV	535756	771955	52.92%	5.689%
35	14.434	1906	1912	1921	rVB	349896	517778	35.49%	3.816%
36	14.628	1938	1945	1956	rBV	229814	341143	23.38%	2.514%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012821\
 Data File : BP004657.D
 Acq On : 28 Jan 2021 10:24
 Operator : CG/JU
 Sample : PB134337BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK337

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP012221.M
 Title : SVOA CALIBRATION

37	14.869	1983	1986	1989	rVB4	1609	1860	0.13%	0.014%
38	15.433	2074	2082	2089	rBV	709345	990471	67.90%	7.300%
39	15.539	2094	2100	2107	rBV	231646	320760	21.99%	2.364%
40	15.675	2115	2123	2127	rBV2	9414	13712	0.94%	0.101%
41	16.216	2212	2215	2221	rBV7	3549	3831	0.26%	0.028%
42	16.480	2256	2260	2262	rBV5	1410	1745	0.12%	0.013%
43	16.763	2306	2308	2311	rBV4	1738	1937	0.13%	0.014%
44	16.869	2323	2326	2330	rVB5	2427	3524	0.24%	0.026%
45	16.980	2341	2345	2349	rVV7	2140	3676	0.25%	0.027%
46	17.192	2372	2381	2387	rBV	478226	687823	47.15%	5.069%
47	17.286	2391	2397	2405	rBV	816292	1168507	80.10%	8.612%
48	17.410	2415	2418	2420	rBV4	1743	1996	0.14%	0.015%
49	17.504	2428	2434	2436	rBV6	1656	2971	0.20%	0.022%
50	17.998	2514	2518	2520	rBV4	1771	1785	0.12%	0.013%
51	19.169	2715	2717	2721	rVB2	9765	10031	0.69%	0.074%
52	19.416	2756	2759	2764	rBV3	10439	14114	0.97%	0.104%
53	19.527	2772	2778	2784	rBV	1151659	1458818	100.00%	10.751%
54	21.268	3070	3074	3080	rBV	675581	832883	57.09%	6.138%
55	23.439	3437	3443	3451	rVB	714148	1317795	90.33%	9.712%
56	23.586	3462	3468	3477	rVB2	398043	744490	51.03%	5.487%




Sum of corrected areas: 13568730

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012821\
Data File : BP004657.D
Acq On : 28 Jan 2021 10:24
Operator : CG/JU
Sample : PB134337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP012221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

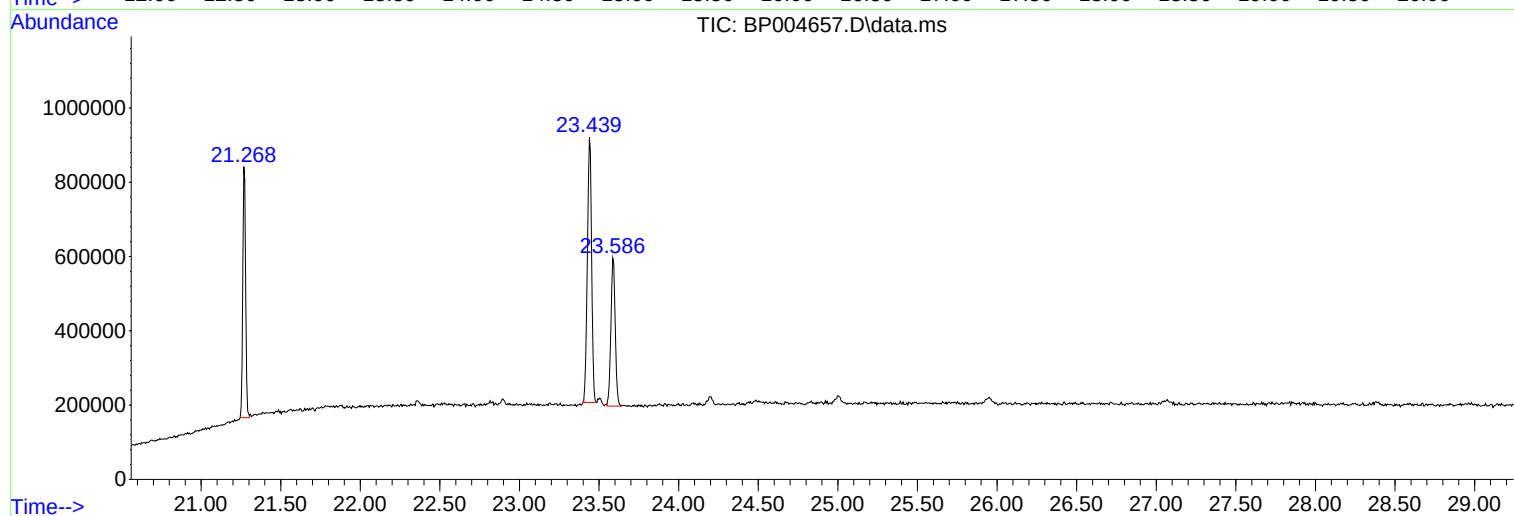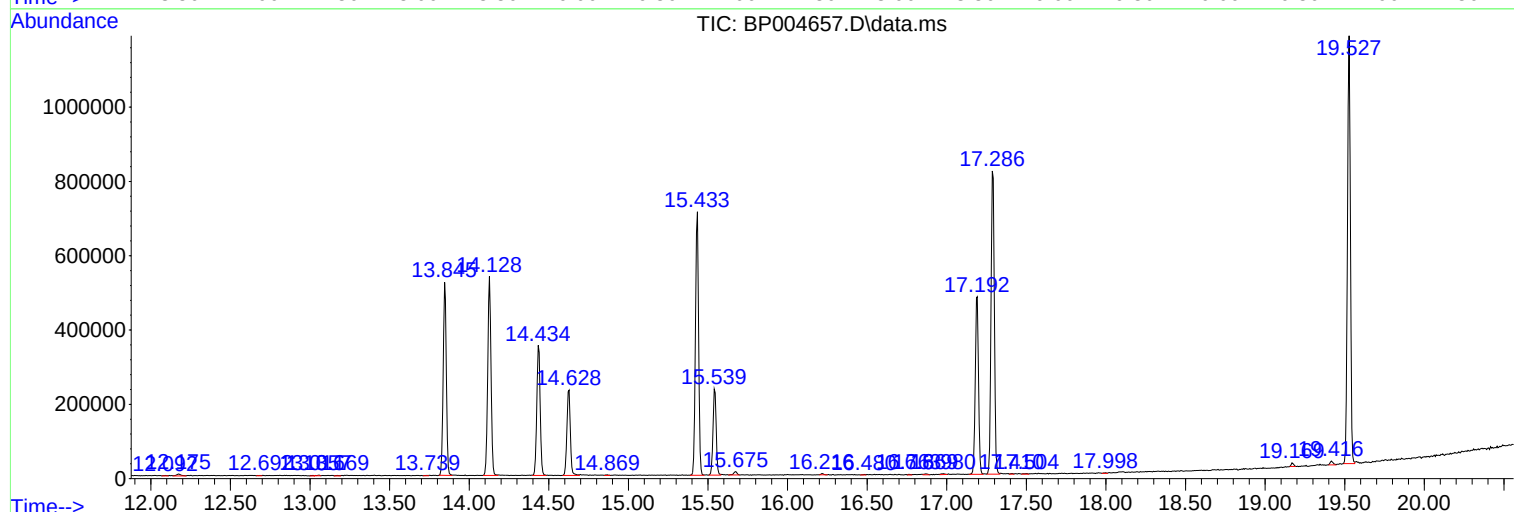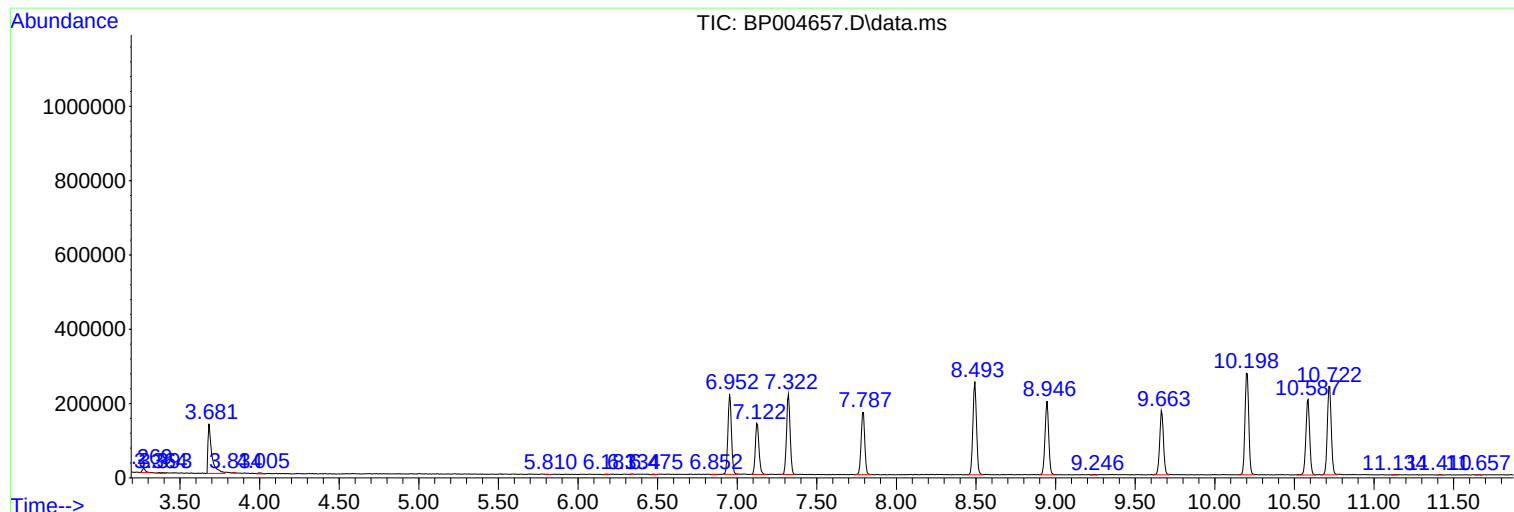

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012821\
Data File : BP004657.D
Acq On : 28 Jan 2021 10:24
Operator : CG/JU
Sample : PB134337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP012221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012821\
Data File : BP004657.D
Acq On : 28 Jan 2021 10:24
Operator : CG/JU
Sample : PB134337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK337

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP012221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
