
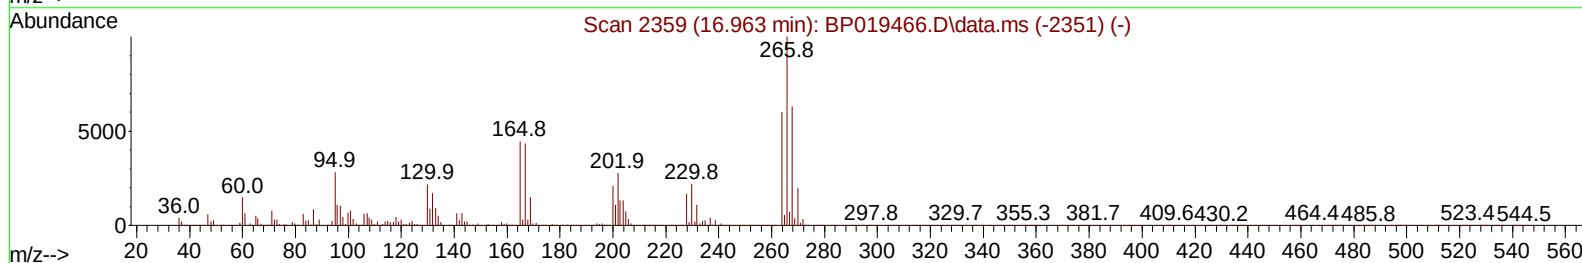
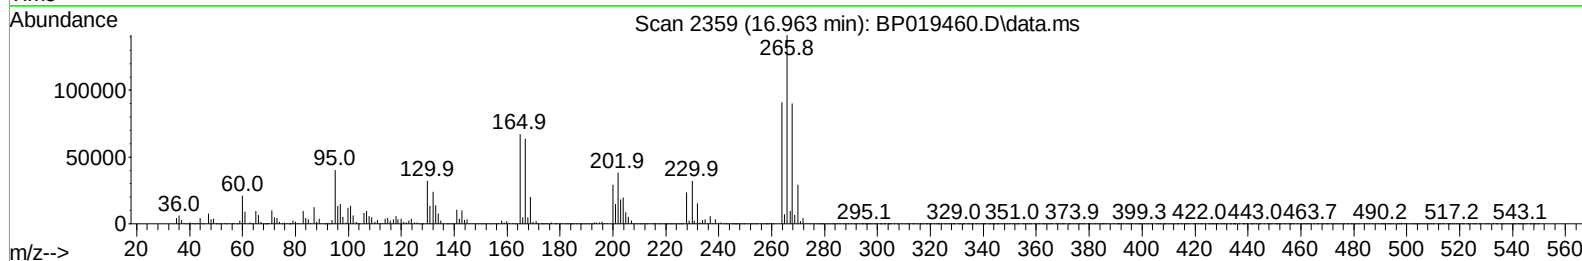


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019460.D
Acq On : 29 Jan 2024 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:10:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 00:59:08 2024
Response via : Initial Calibration

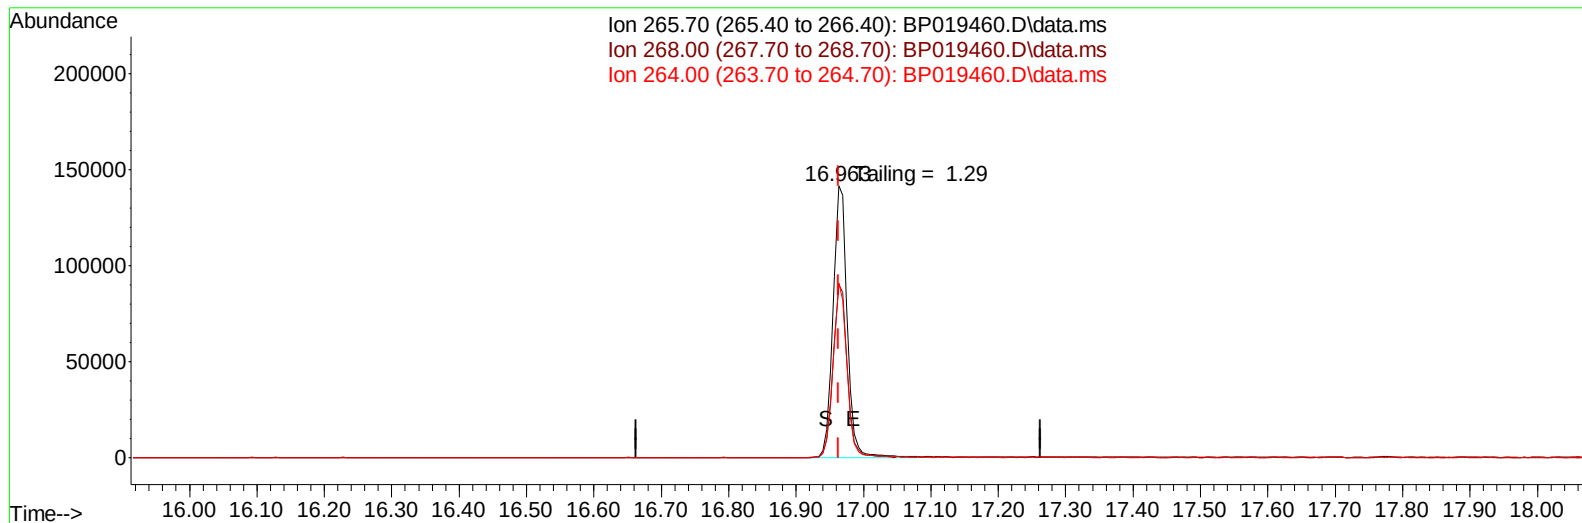




TIC: BP019460.D\data.ms

(70) Pentachlorophenol (C)**16.963min (-0.000) 181692.63 ng****response 205411**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.87
264.00	60.00	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019460.D
Acq On : 29 Jan 2024 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:10:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 00:59:08 2024
Response via : Initial Calibration

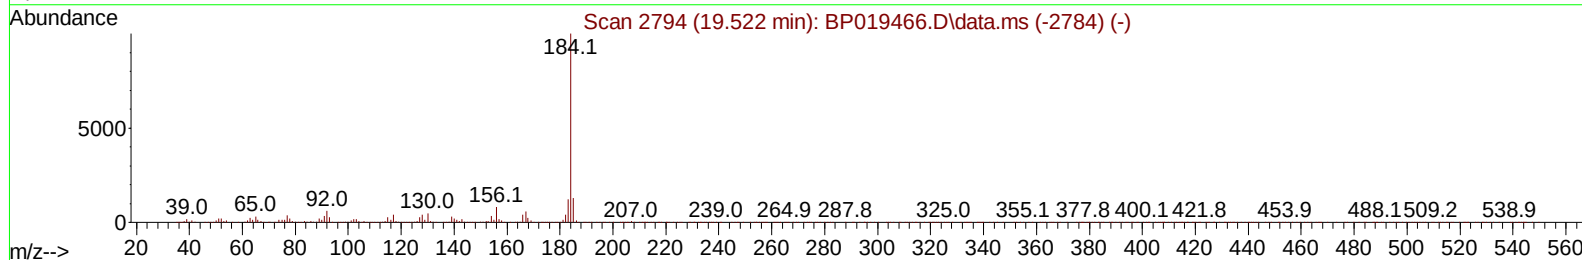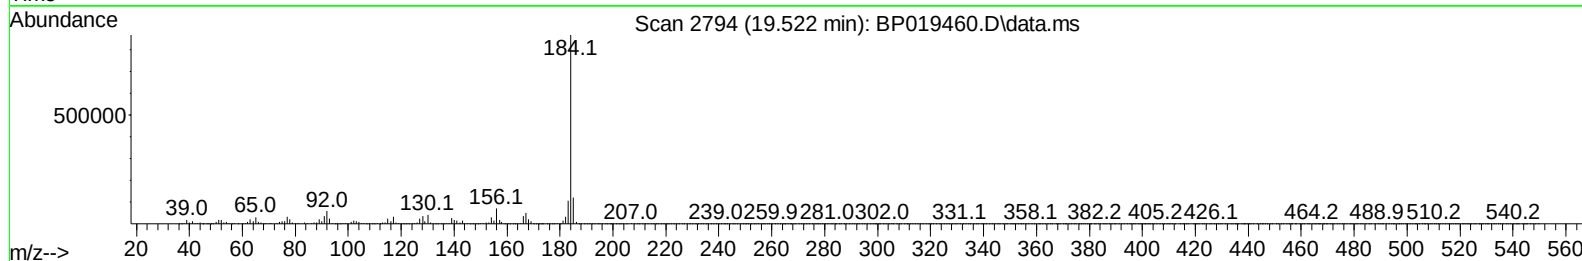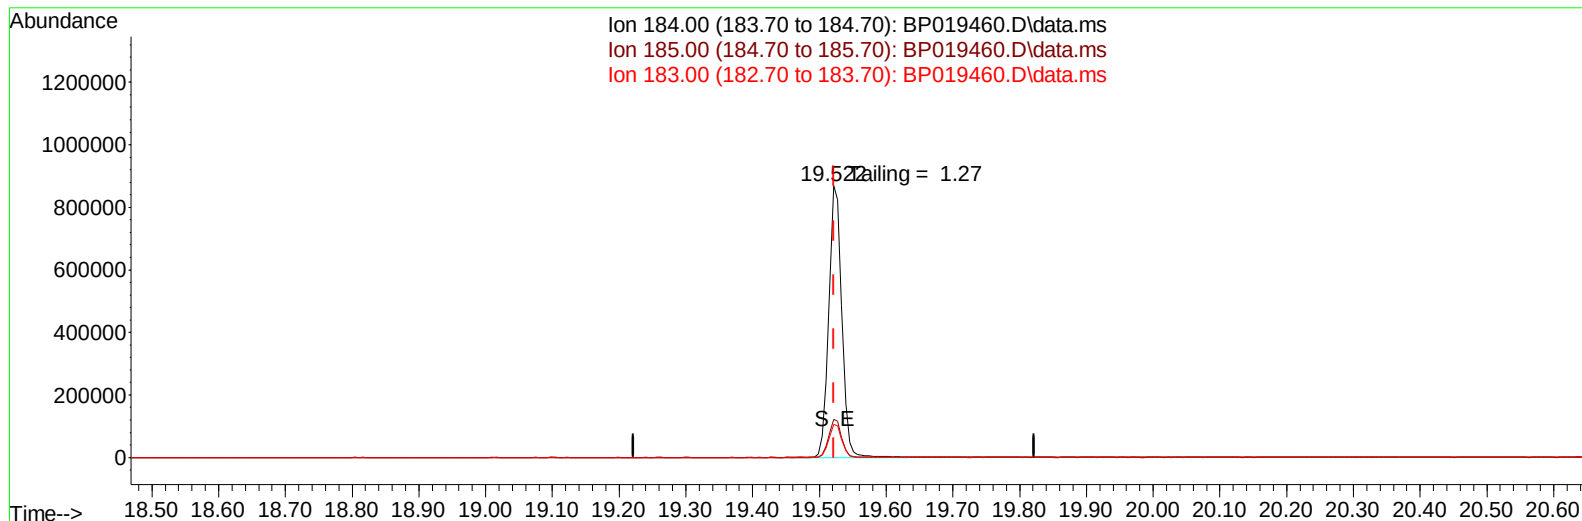

TIC: BP019460.D\data.ms

(77) Benzidine**19.522min (-0.000) 2269.04 ng****response 1186060**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.03
183.00	12.20	12.08
0.00	0.00	0.00