

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
 Data File : BP019472.D
 Acq On : 29 Jan 2024 18:45
 Operator : MA/JU
 Sample : PB158620BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB158620BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	404	411	420	rBV	1695249	2480862	44.56%	10.211%
2	7.099	673	682	694	rBV	1654208	2688267	48.29%	11.065%
3	7.928	816	823	833	rVB	290039	471844	8.48%	1.942%
4	9.098	1013	1022	1033	rBV	1029070	1724760	30.98%	7.099%
5	10.728	1289	1299	1309	rBV	366107	641992	11.53%	2.642%
6	13.192	1710	1718	1727	rVB	2678829	3926403	70.53%	16.161%
7	14.557	1943	1950	1959	rBV	581854	900109	16.17%	3.705%
8	16.051	2195	2204	2217	rBV	2095126	3108284	55.83%	12.794%
9	17.316	2413	2419	2427	rBV	768593	1121906	20.15%	4.618%
10	19.886	2850	2856	2862	rBV	4442535	5567358	100.00%	22.915%
11	21.410	3110	3115	3121	rVB	673674	905886	16.27%	3.729%
12	23.845	3522	3529	3539	rVB	361601	757841	13.61%	3.119%




Sum of corrected areas: 24295512

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019472.D
Acq On : 29 Jan 2024 18:45
Operator : MA/JU
Sample : PB158620BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158620BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

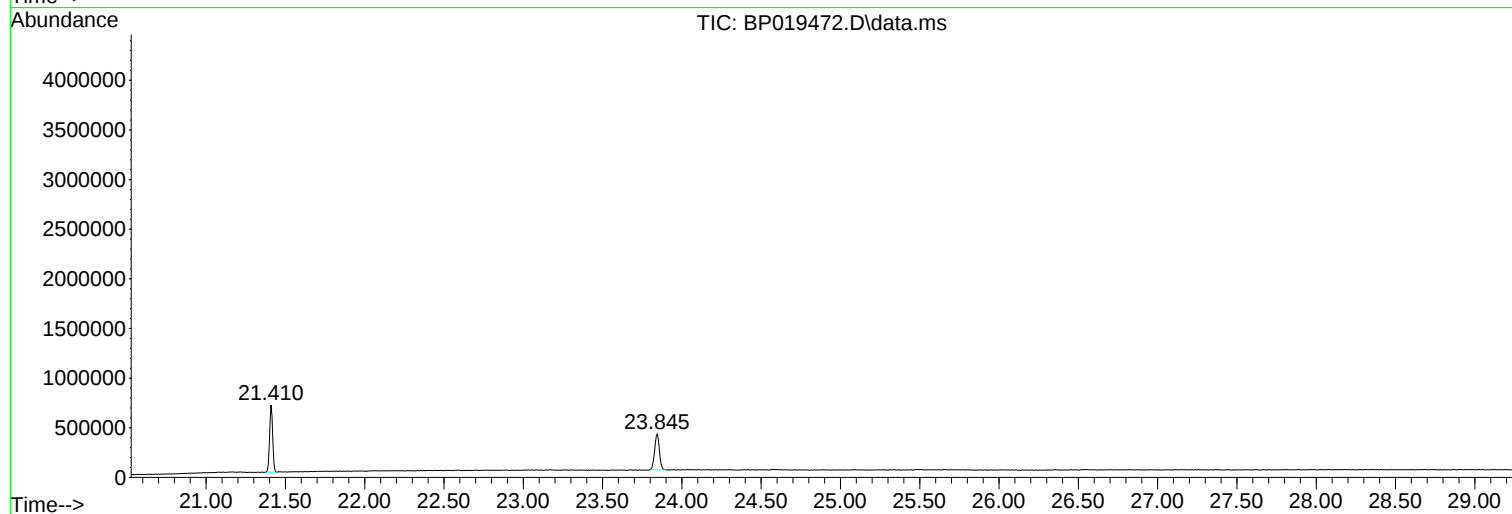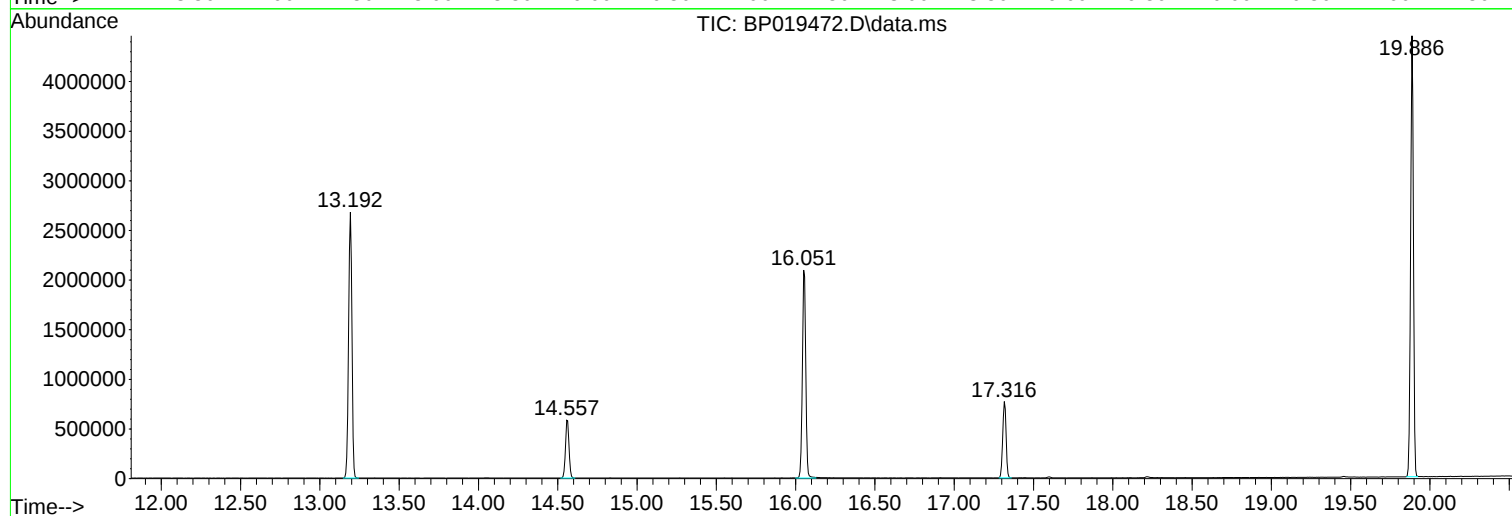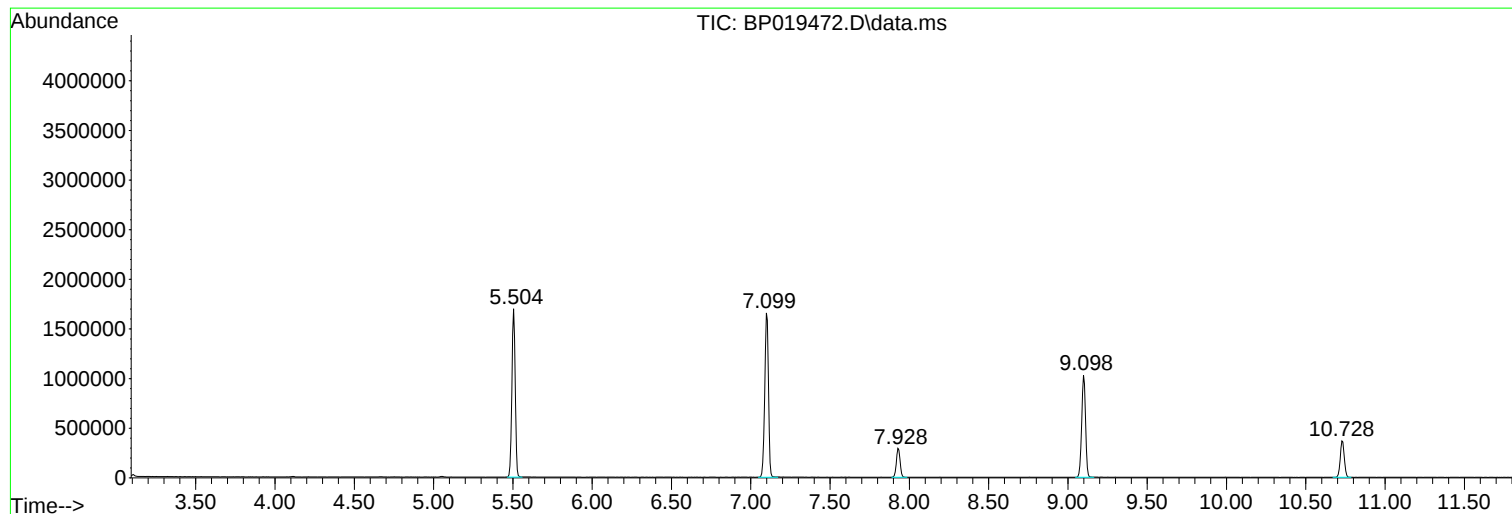

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019472.D
Acq On : 29 Jan 2024 18:45
Operator : MA/JU
Sample : PB158620BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158620BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019472.D
Acq On : 29 Jan 2024 18:45
Operator : MA/JU
Sample : PB158620BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158620BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------