
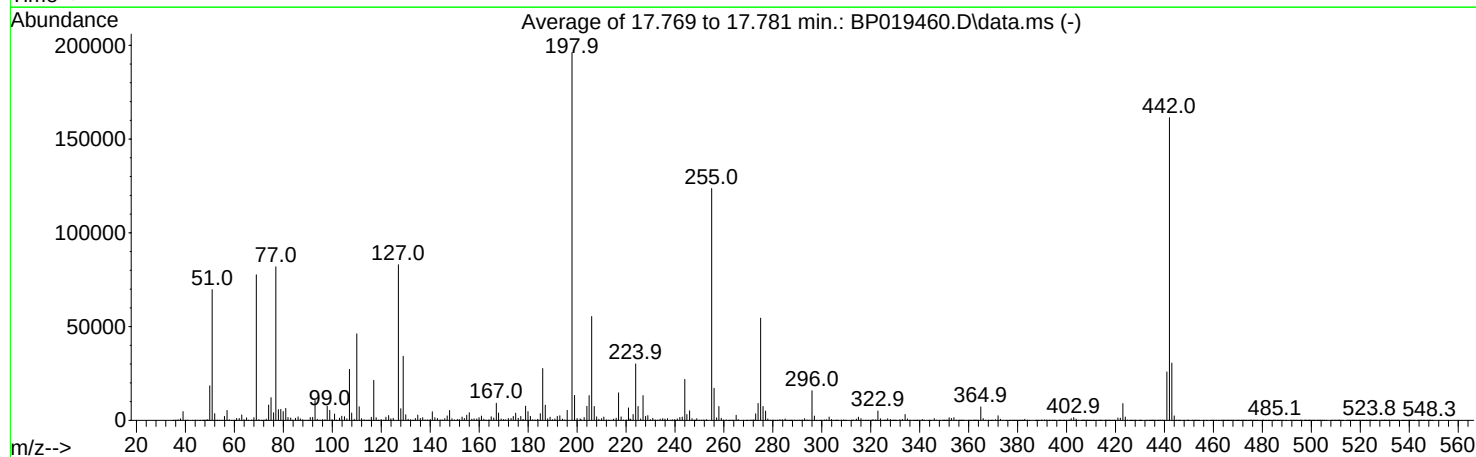


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019460.D
Acq On : 29 Jan 2024 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 30 00:59:08 2024

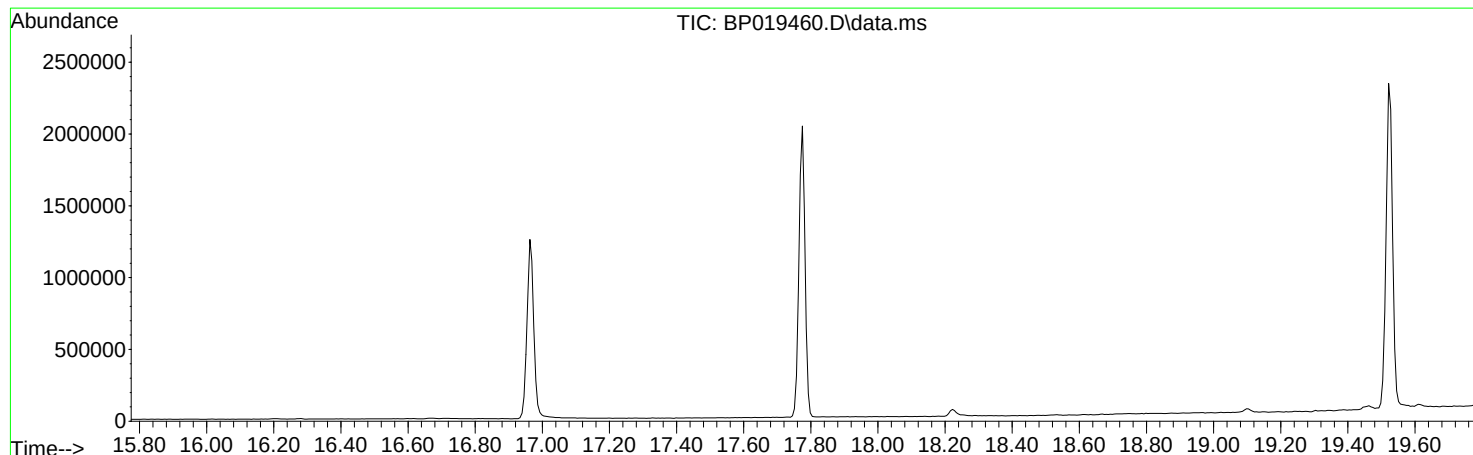




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	35.5	69684	PASS
68	69	0.00	2	1.8	1419	PASS
69	198	0.00	100	39.6	77682	PASS
70	69	0.00	2	0.5	415	PASS
127	198	10	80	42.3	83028	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196160	PASS
199	198	5	9	6.8	13326	PASS
275	198	10	60	27.8	54526	PASS
365	198	1	100	3.7	7166	PASS
441	198	0.01	100	13.2	25843	PASS
442	442	100	100	100.0	161454	PASS
443	442	15	24	18.9	30568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019460.D
Acq On : 29 Jan 2024 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 30 04:10:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 00:59:08 2024
Response via : Initial Calibration

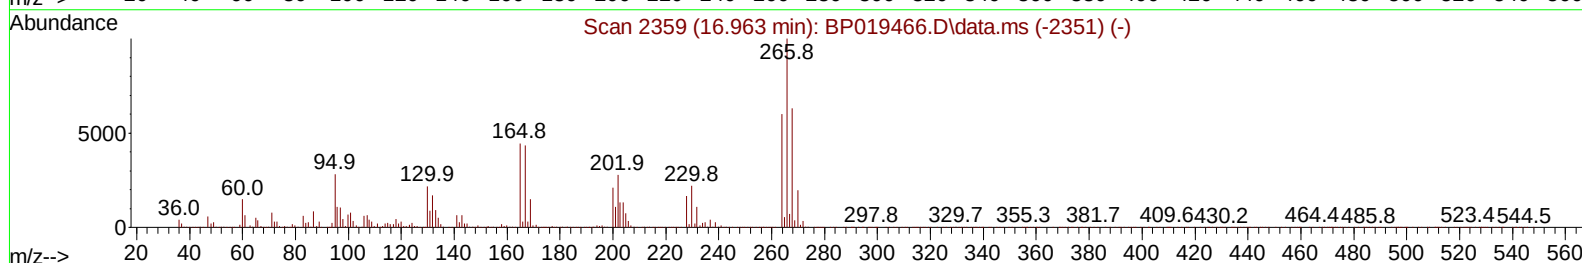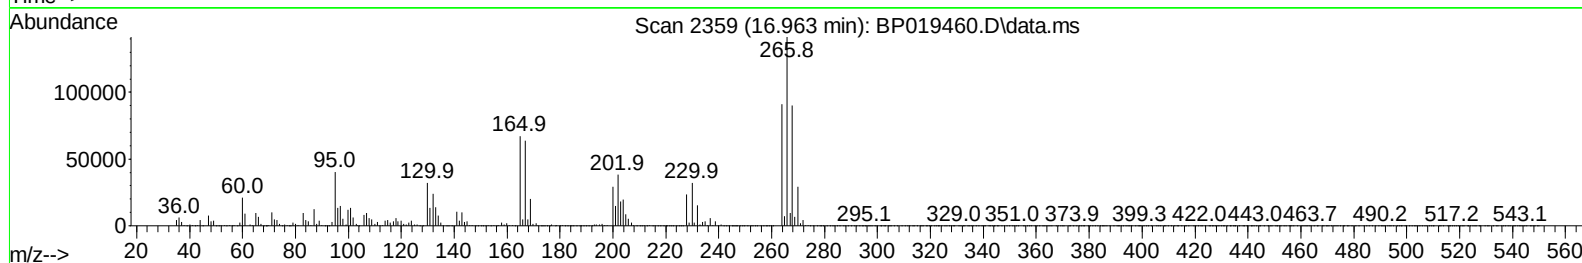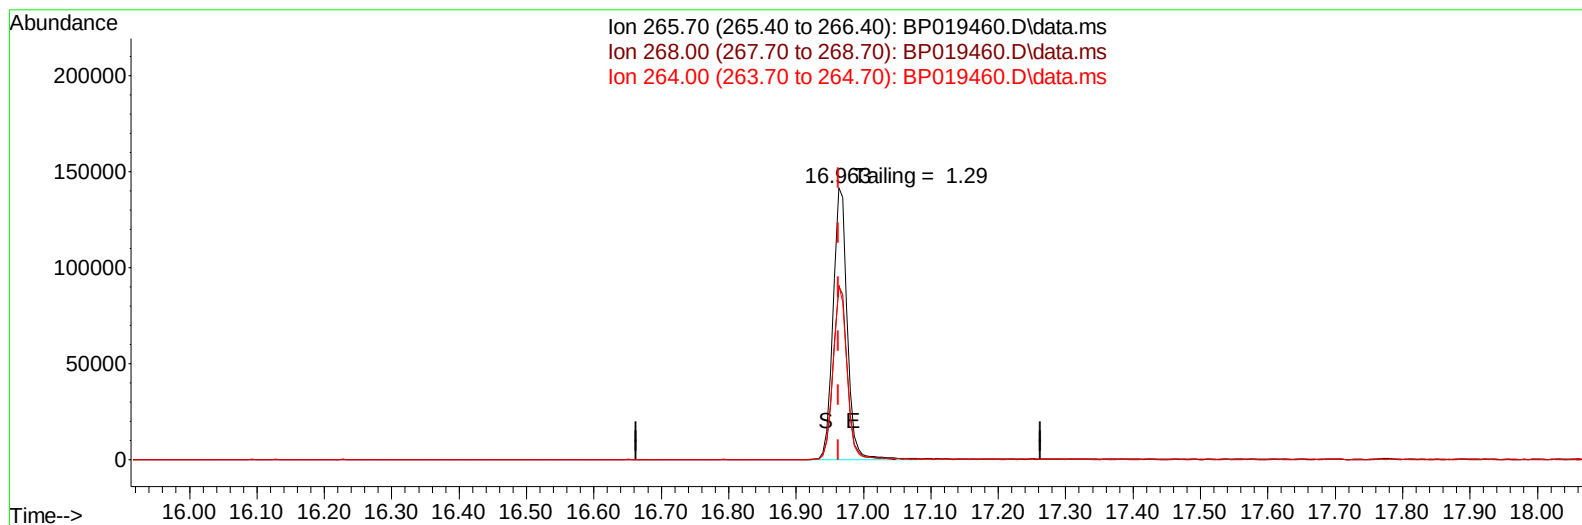

TIC: BP019460.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.000) 181692.63 ng




response 205411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.87
264.00	60.00	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012924\
Data File : BP019460.D
Acq On : 29 Jan 2024 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 30 04:10:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 00:59:08 2024
Response via : Initial Calibration

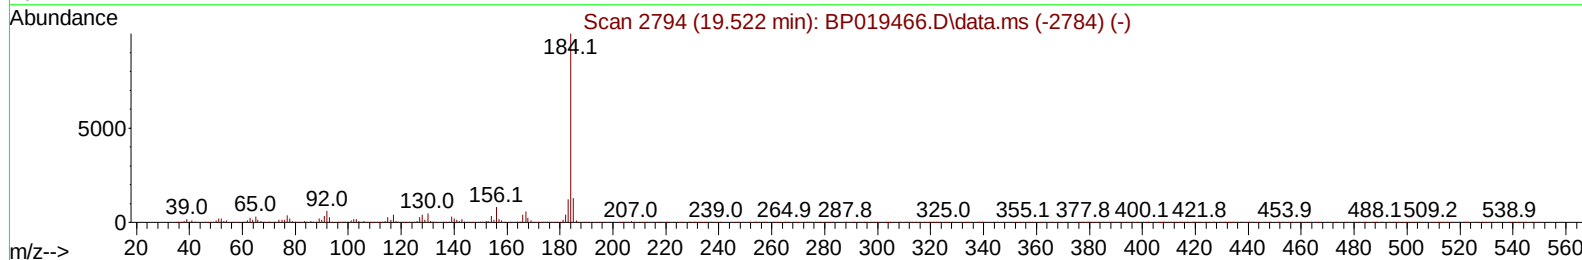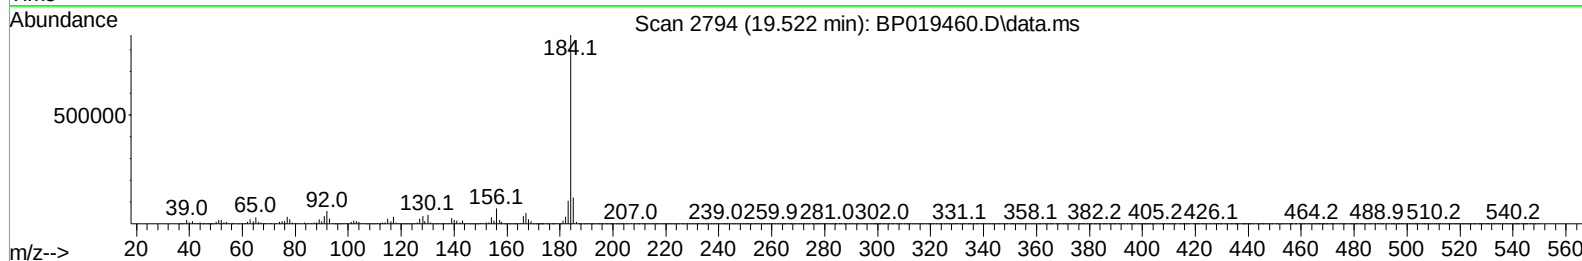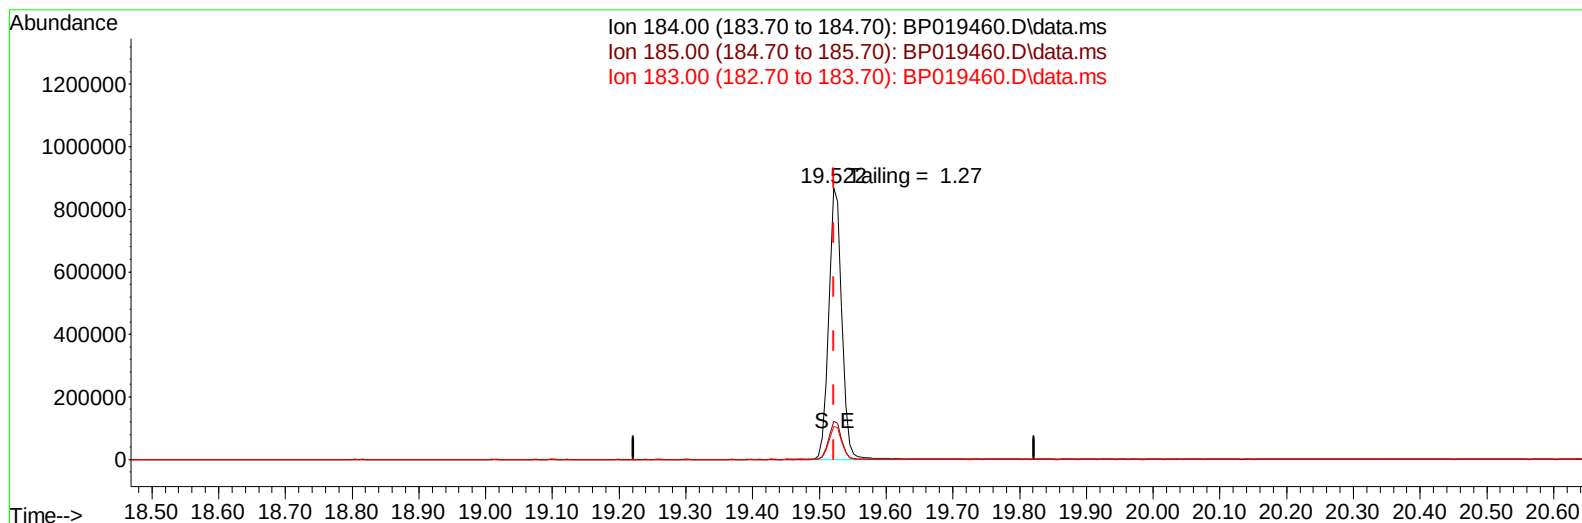

TIC: BP019460.D\data.ms

(77) Benzidine

19.522min (-0.000) 2269.04 ng

response 1186060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.03
183.00	12.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/29/2024	BNA_P	<u>BP019460.D</u>
Compound Name	Response	Retention Time
DDT	560571	20.727
DDD	10839	20.345
DDE	0	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10839	571410	1.90

Instrument :
BNA_P
ClientSampleId :
DFTPP