
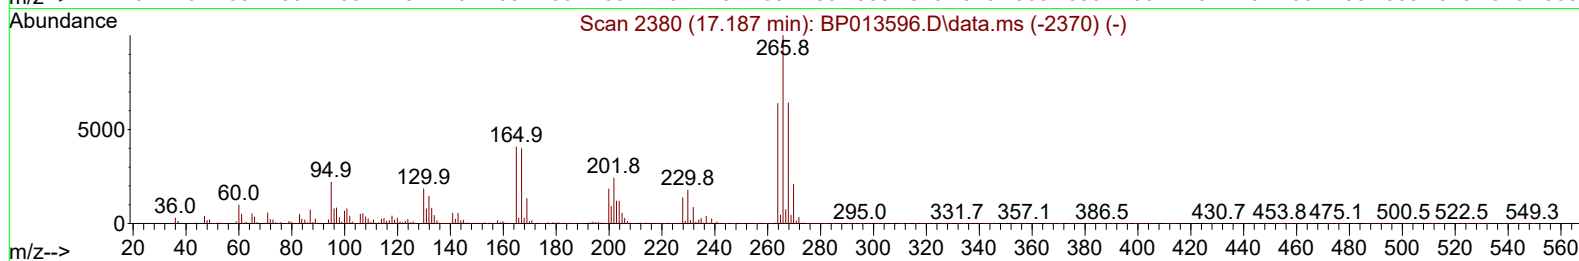
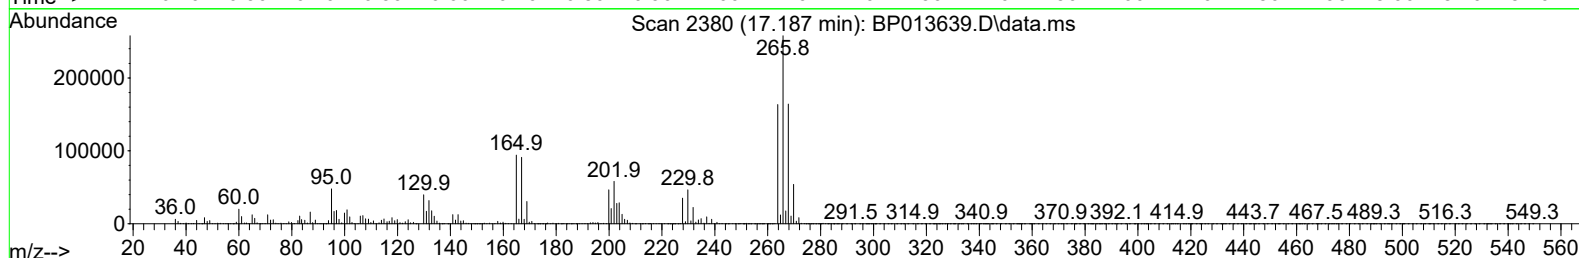


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
 Data File : BP013639.D
 Acq On : 30 Jan 2023 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:06:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 04:38:43 2023
 Response via : Initial Calibration

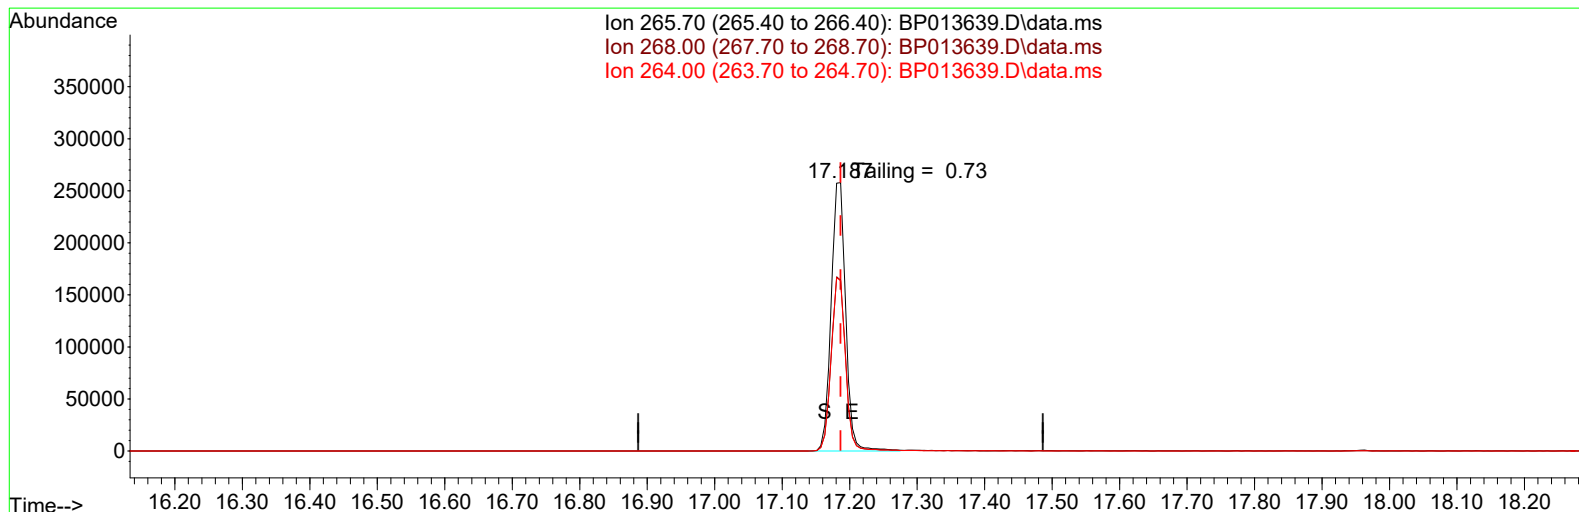

TIC: BP013639.D\data.ms

(70) Pentachlorophenol (C)




17.187min (-0.000) 165123.34 ng

response 384792

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.64
264.00	63.80	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
 Data File : BP013639.D
 Acq On : 30 Jan 2023 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:06:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 04:38:43 2023
 Response via : Initial Calibration

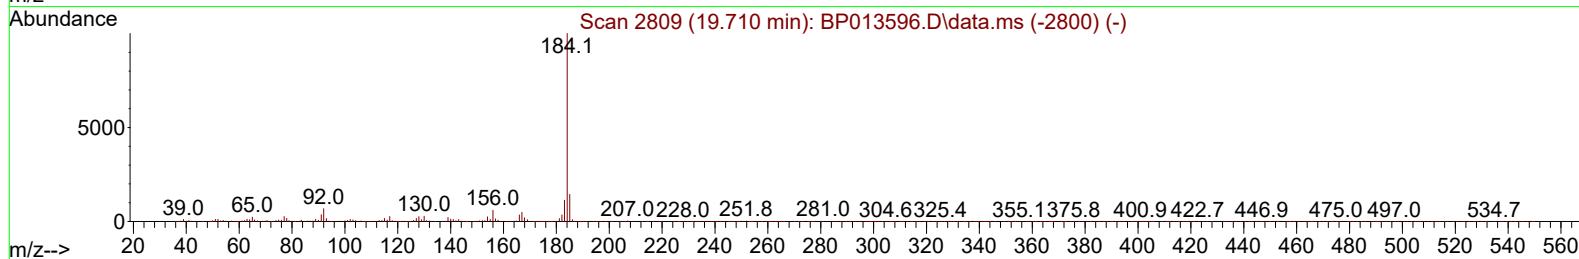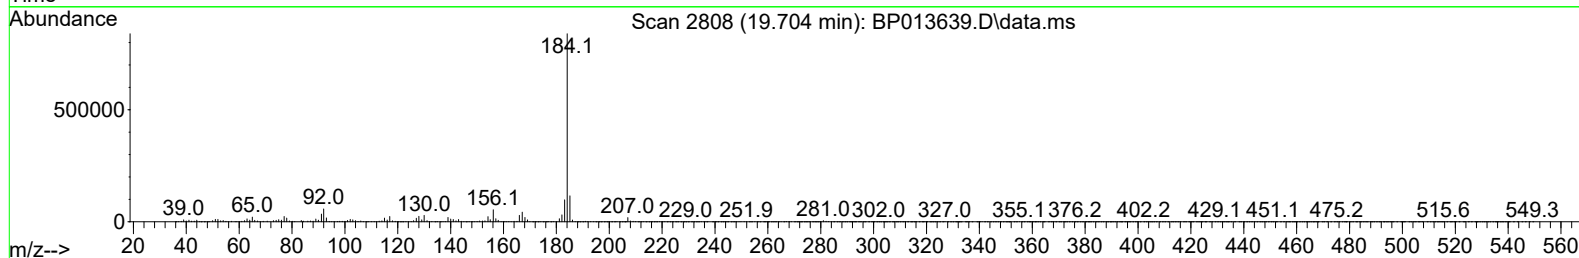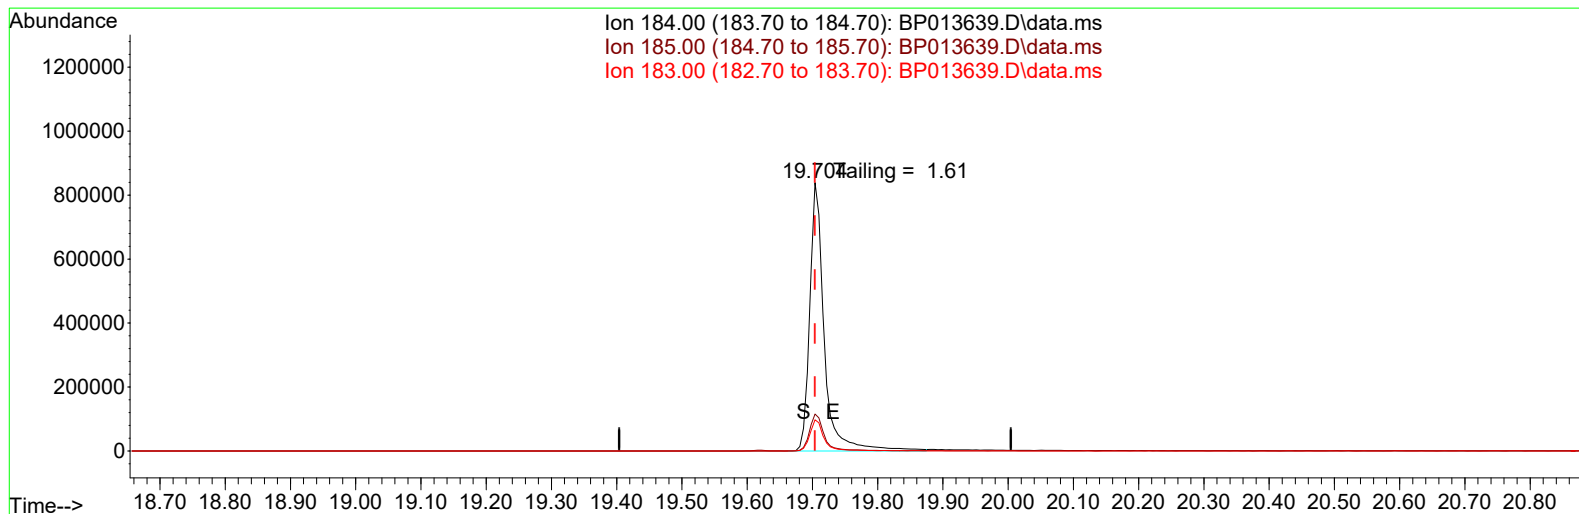

TIC: BP013639.D\data.ms

(77) Benzidine**19.704min (-0.000) 71421.36 ng****response 1293939**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.77
183.00	11.30	11.66
0.00	0.00	0.00