
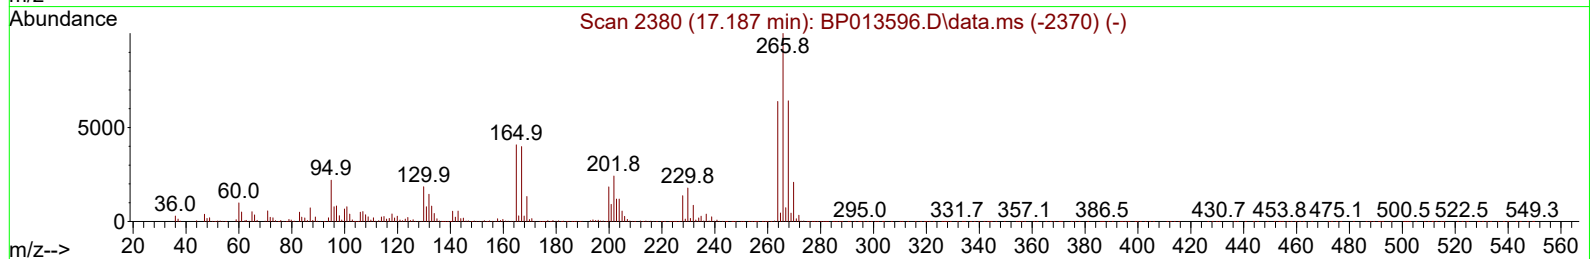
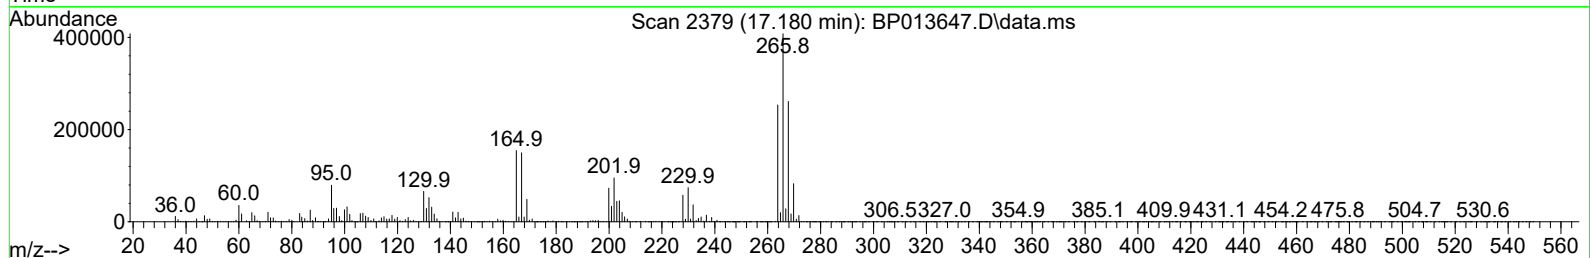


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013647.D
Acq On : 30 Jan 2023 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:07:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 04:38:43 2023
Response via : Initial Calibration

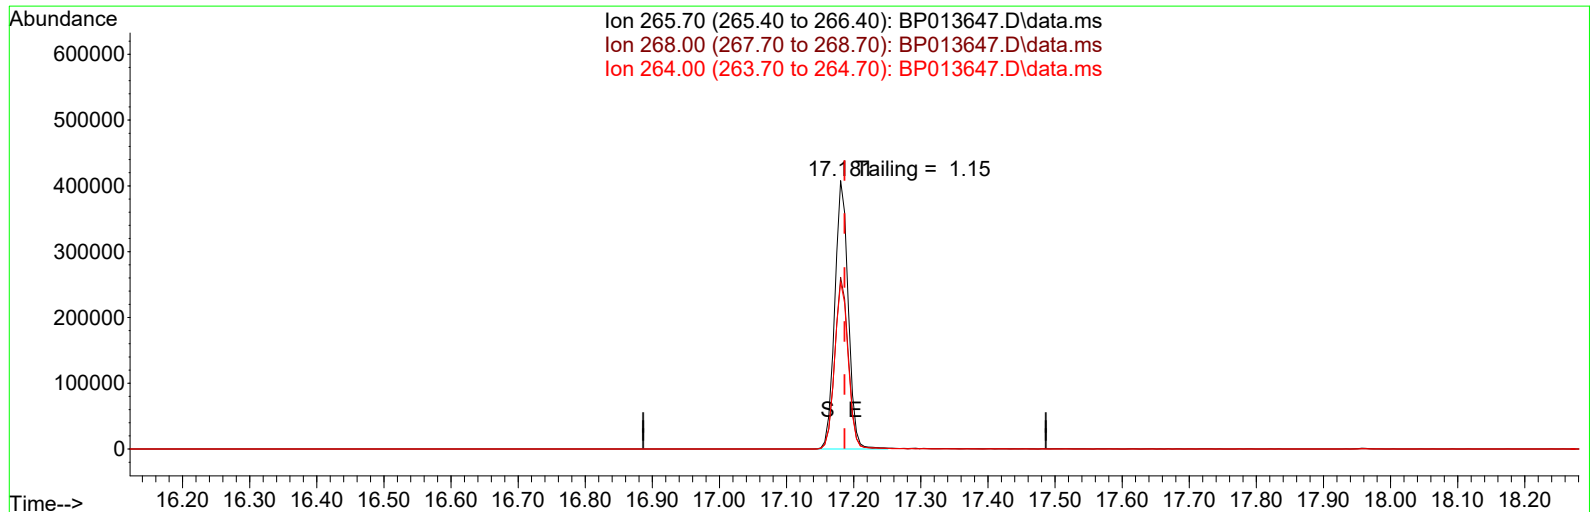

TIC: BP013647.D\data.ms

(70) Pentachlorophenol (C)




17.180min (-0.006) 119887.25 ng

response 574014

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.97
264.00	63.80	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013647.D
Acq On : 30 Jan 2023 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:07:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 04:38:43 2023
Response via : Initial Calibration

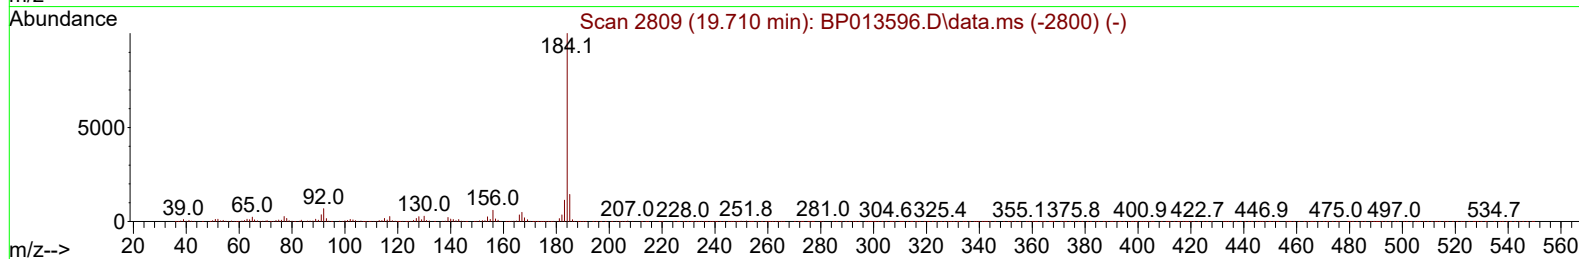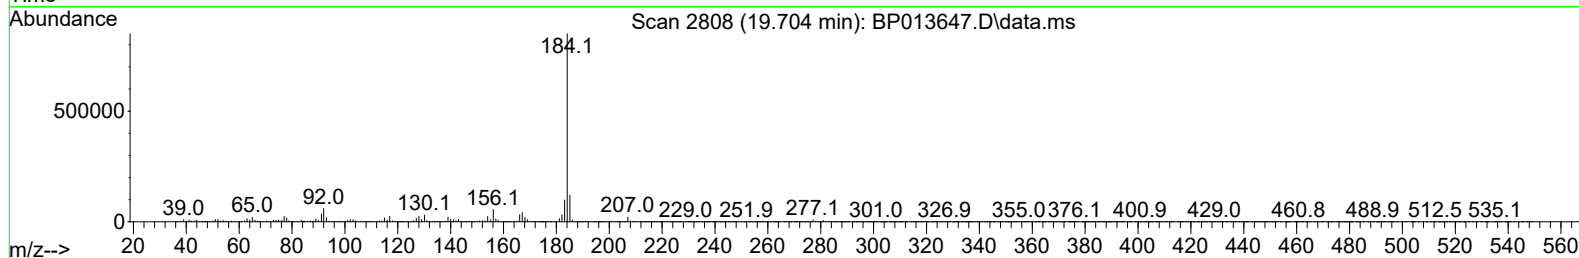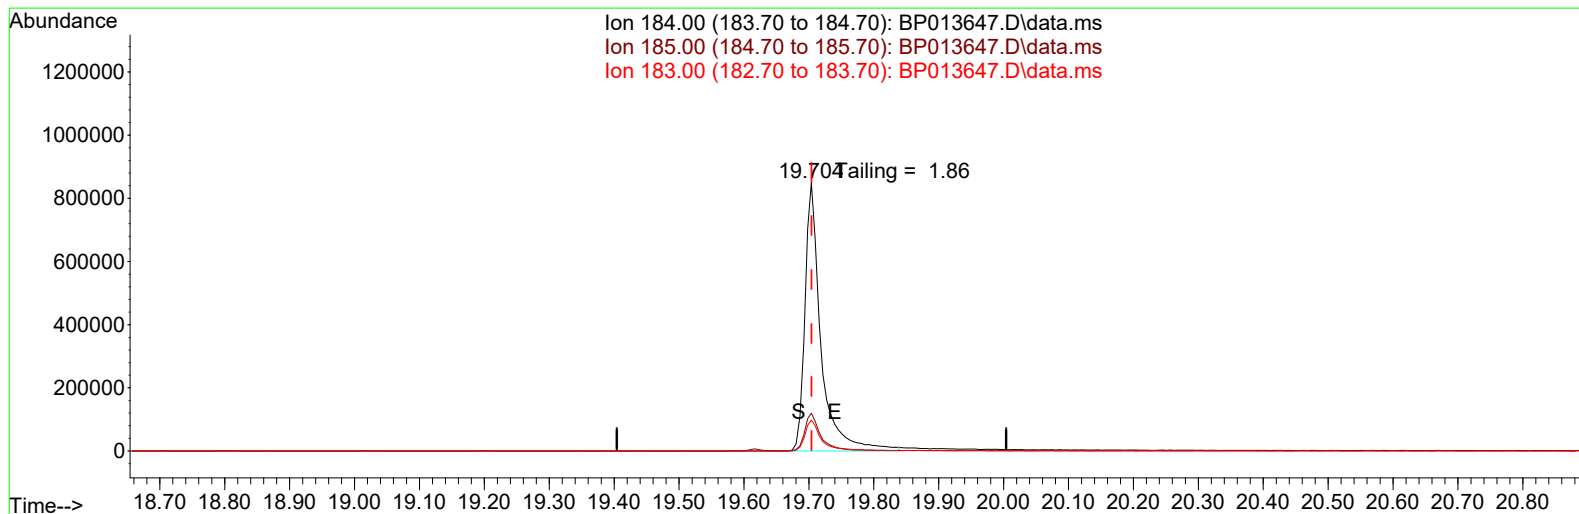

TIC: BP013647.D\data.ms

(77) Benzidine

19.704min (-0.000) 57009.23 ng

response 1490677

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.30	11.55
0.00	0.00	0.00