


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013639.D
Acq On : 30 Jan 2023 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 31 04:38:43 2023

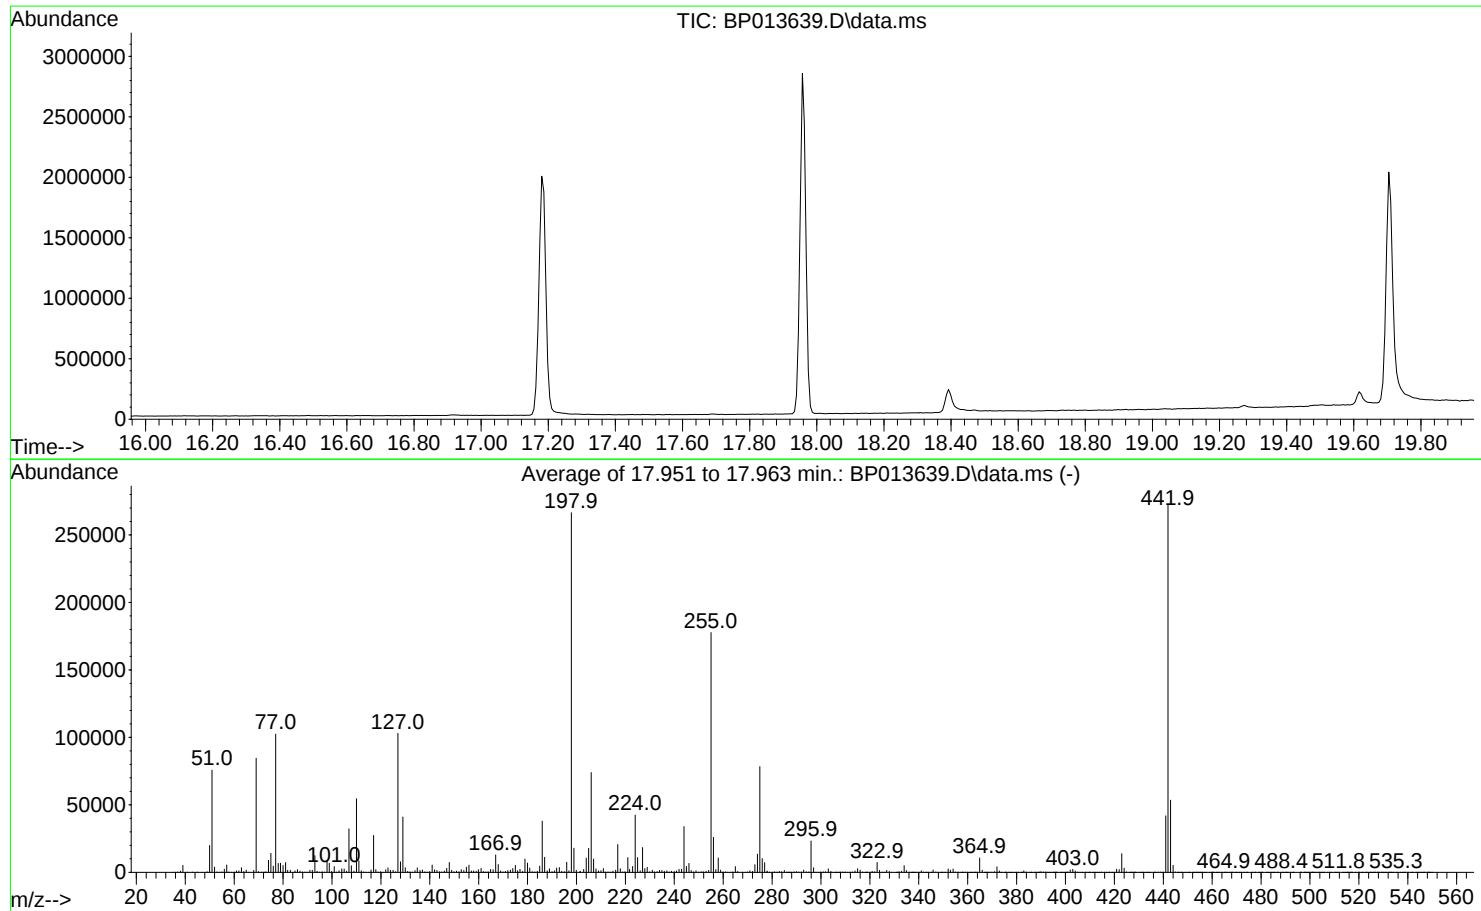




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	75748	PASS
68	69	0.00	2	1.6	1335	PASS
69	198	0.00	100	31.7	84482	PASS
70	69	0.00	2	0.6	482	PASS
127	198	10	80	38.6	102991	PASS
197	198	0.00	2	0.4	1158	PASS
198	198	100	100	100.0	266510	PASS
199	198	5	9	6.7	17880	PASS
275	198	10	60	29.4	78368	PASS
365	198	1	100	4.0	10622	PASS
441	198	0.01	100	15.7	41845	PASS
442	442	100	100	100.0	272634	PASS
443	442	15	24	19.6	53379	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013639.D
Acq On : 30 Jan 2023 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 31 06:06:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 04:38:43 2023
Response via : Initial Calibration

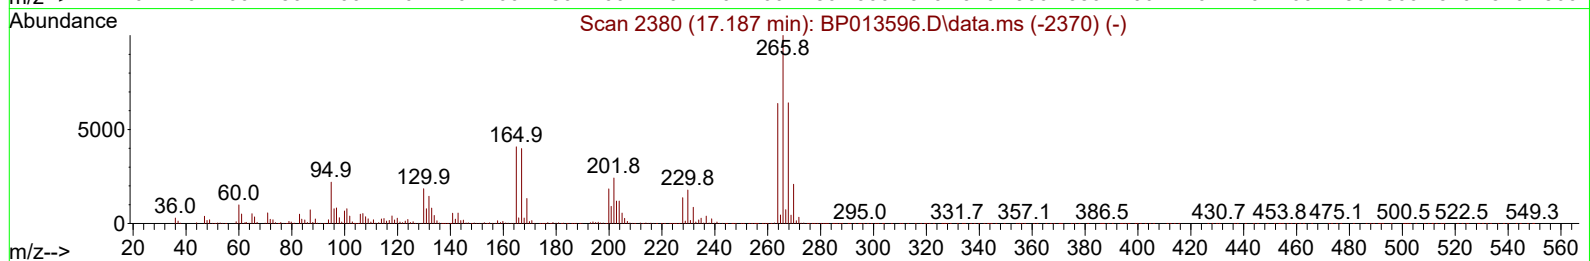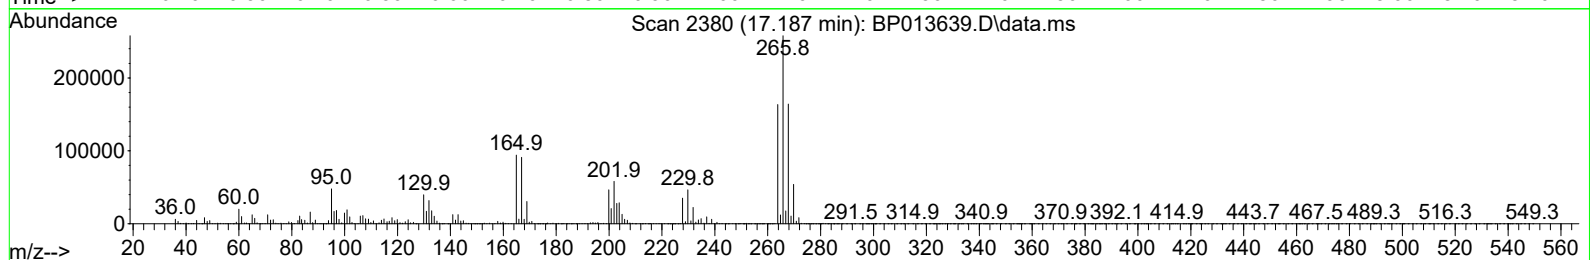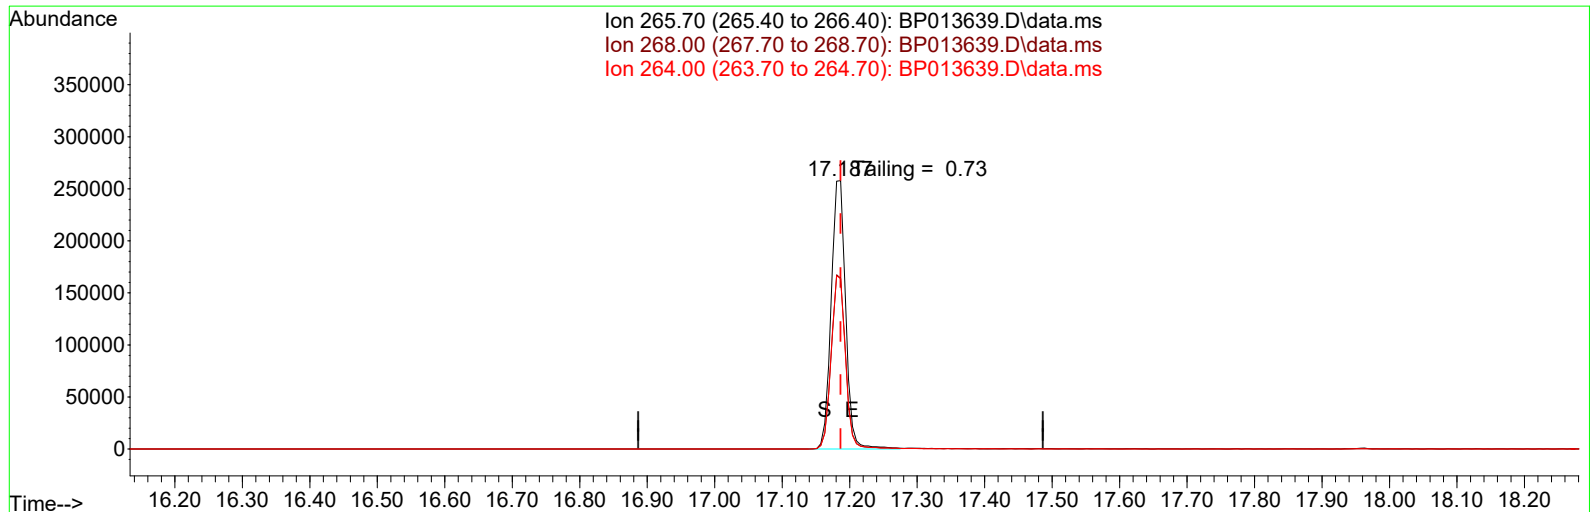

TIC: BP013639.D\data.ms

(70) Pentachlorophenol (C)

17.187min (-0.000) 165123.34 ng




response 384792

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.64
264.00	63.80	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013639.D
Acq On : 30 Jan 2023 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 31 06:06:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 04:38:43 2023
Response via : Initial Calibration

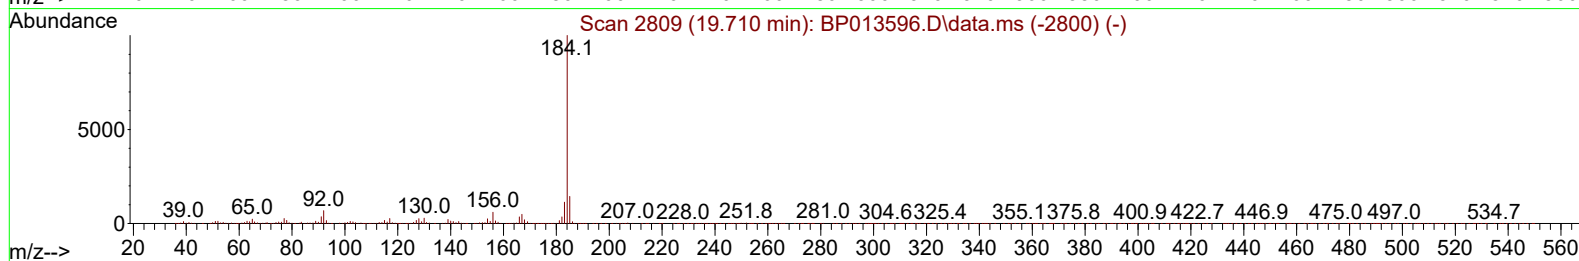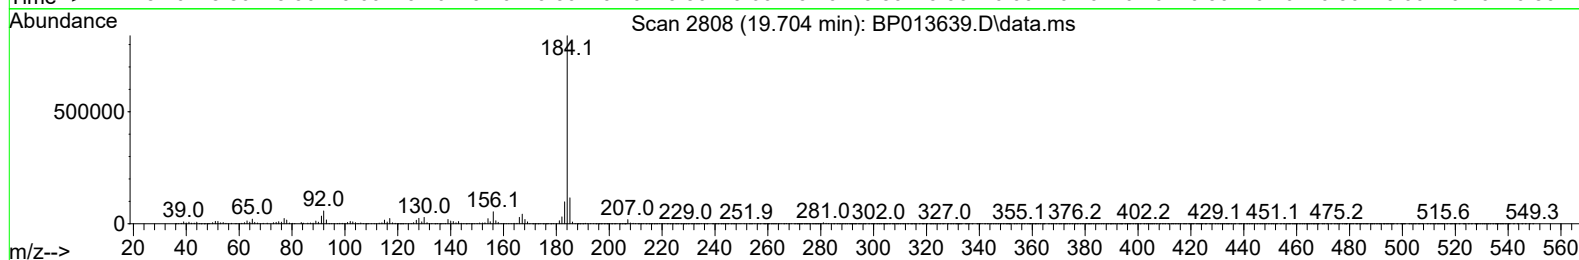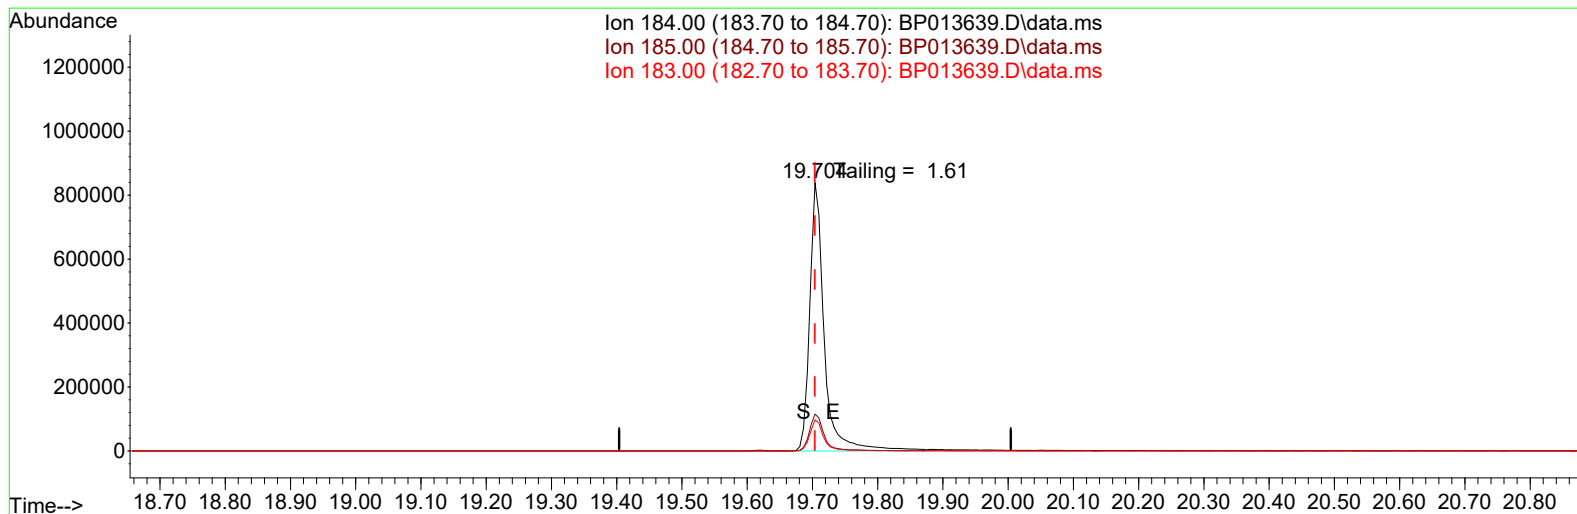

TIC: BP013639.D\data.ms

(77) Benzidine

19.704min (-0.000) 71421.36 ng

response 1293939

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.77
183.00	11.30	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2023	BNA_P	<u>BP013639.D</u>
Compound Name	Response	Retention Time
DDT	638862	20.904
DDD	11743	20.469
DDE	1125	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12868	651730	1.97

Instrument :
BNA_P
ClientSampleId :
DFTPP