


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
Data File : BP013647.D
Acq On : 30 Jan 2023 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 31 04:38:43 2023

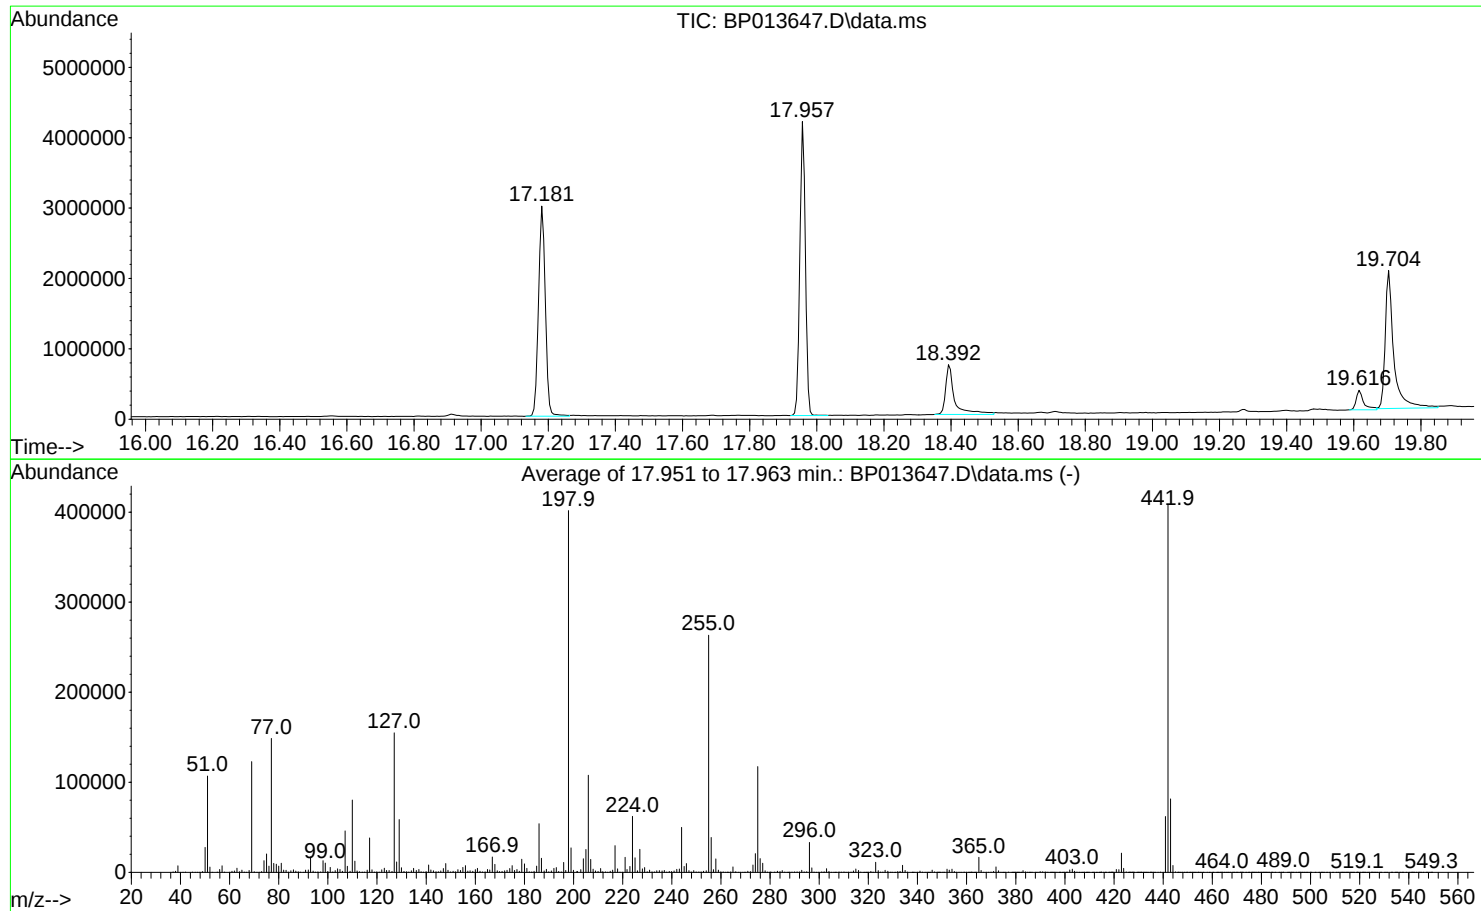




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	106900	PASS
68	69	0.00	2	1.7	2035	PASS
69	198	0.00	100	30.6	122977	PASS
70	69	0.00	2	0.5	602	PASS
127	198	10	80	38.5	154849	PASS
197	198	0.00	2	0.5	2003	PASS
198	198	100	100	100.0	401710	PASS
199	198	5	9	6.8	27197	PASS
275	198	10	60	29.2	117384	PASS
365	198	1	100	4.1	16622	PASS
441	198	0.01	100	15.4	61949	PASS
442	442	100	100	100.0	408552	PASS
443	442	15	24	20.0	81517	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
 Data File : BP013647.D
 Acq On : 30 Jan 2023 16:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 31 06:07:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 04:38:43 2023
 Response via : Initial Calibration

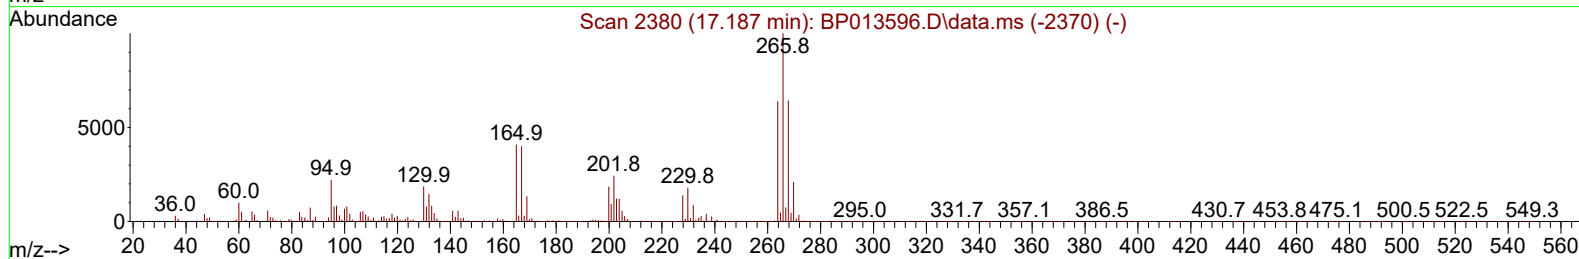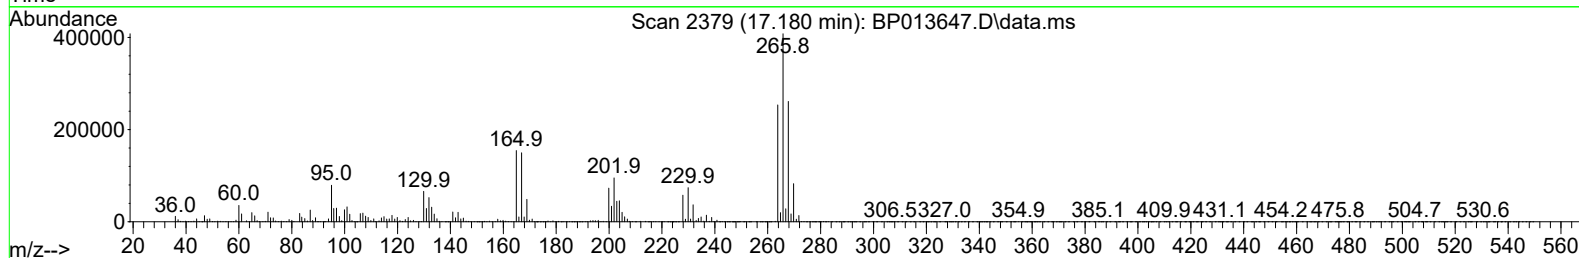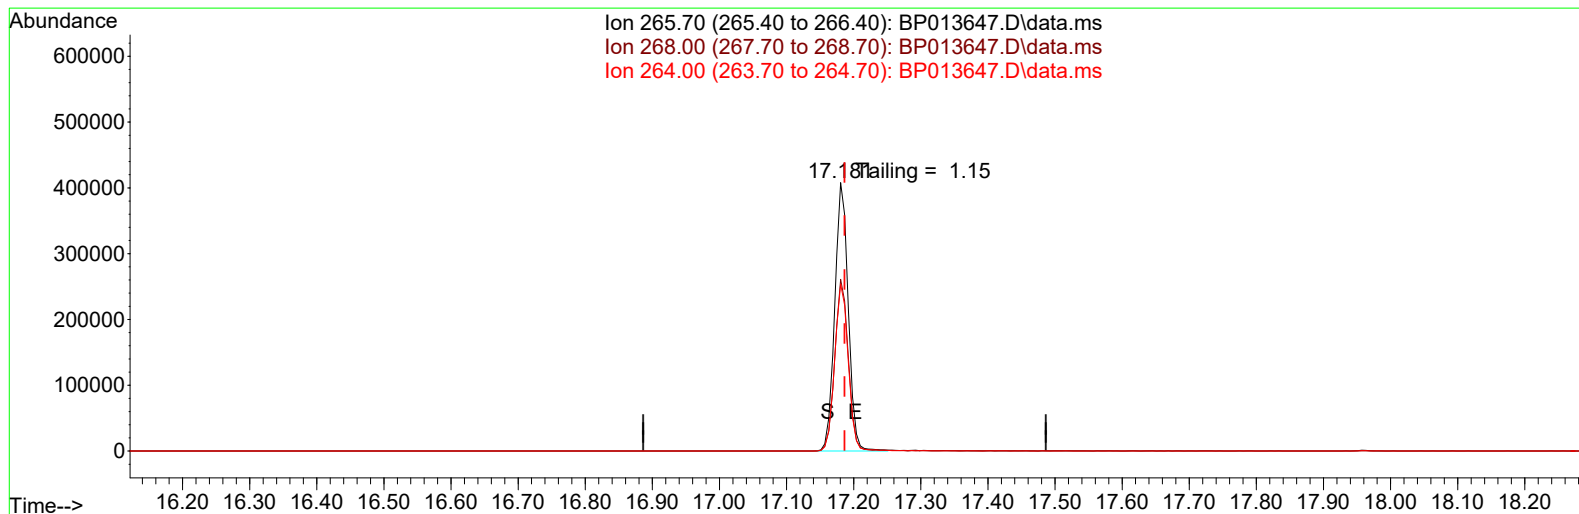

TIC: BP013647.D\data.ms

(70) Pentachlorophenol (C)

17.180min (-0.006) 119887.25 ng




response 574014

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.97
264.00	63.80	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013023\
 Data File : BP013647.D
 Acq On : 30 Jan 2023 16:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 31 06:07:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 04:38:43 2023
 Response via : Initial Calibration

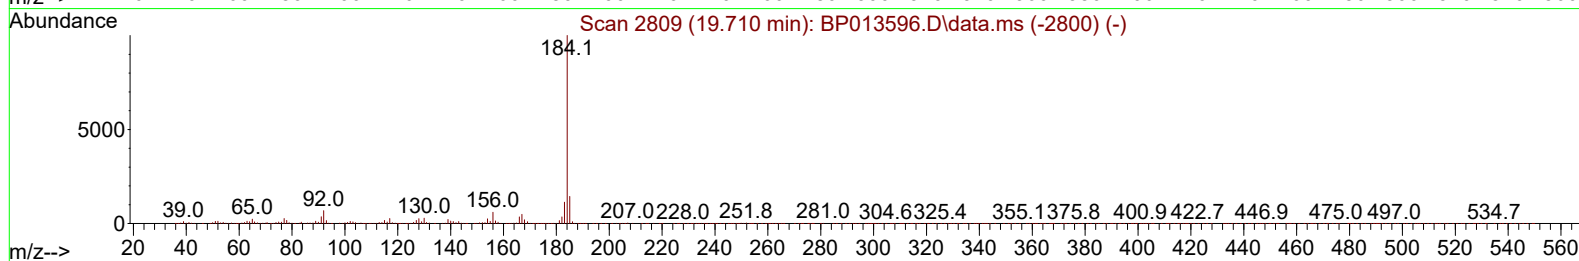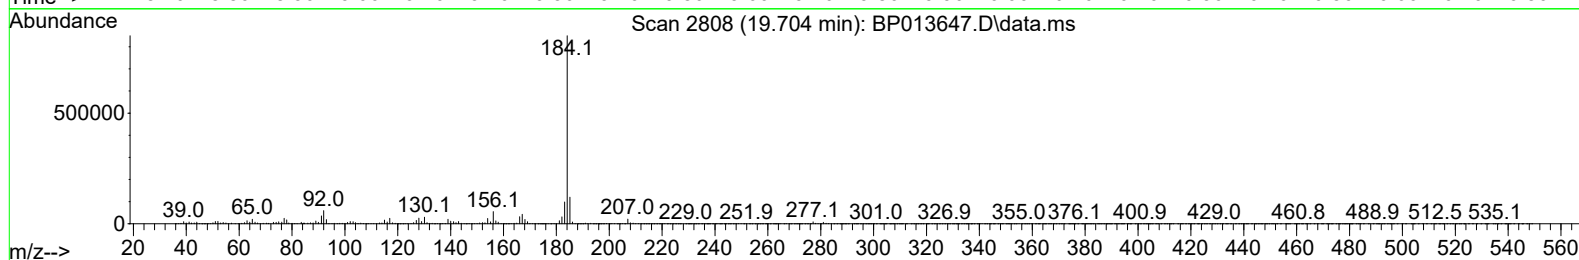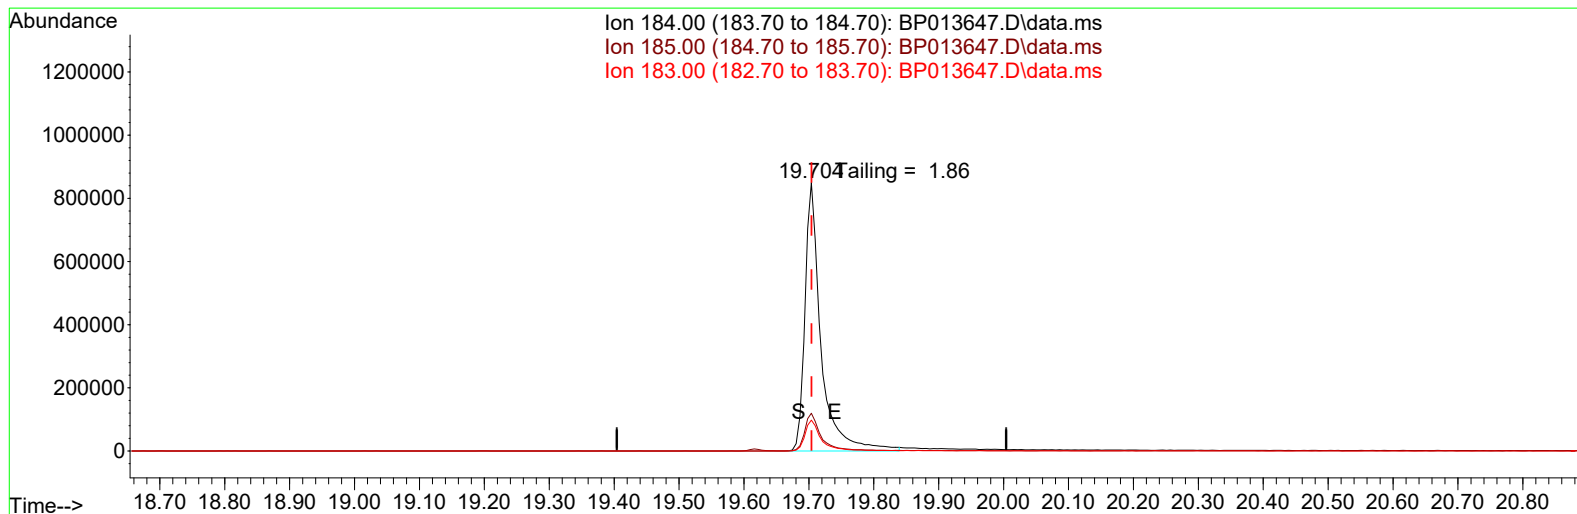

TIC: BP013647.D\data.ms

(77) Benzidine

19.704min (-0.000) 57009.23 ng

response 1490677

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.30	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2023	BNA_P	<u>BP013647.D</u>
Compound Name	Response	Retention Time
DDT	1214487	20.904
DDD	21712	20.469
DDE	2634	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24346	1238833	1.97

Instrument :
BNA_P
ClientSampleId :
DFTPP