

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013024\
Data File : BP019490.D
Acq On : 30 Jan 2024 19:51
Operator : MA/JU
Sample : PB158676BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158676BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	402	409	420	rBV	1510344	2203550	58.34%	11.564%
2	7.087	672	680	688	rBV	1421992	2251064	59.60%	11.814%
3	7.916	812	821	833	rBV	288165	461843	12.23%	2.424%
4	9.087	1010	1020	1028	rBV	883576	1481489	39.23%	7.775%
5	10.716	1289	1297	1305	rBV	334896	573732	15.19%	3.011%
6	13.181	1706	1716	1725	rBV	1994574	3021258	79.99%	15.856%
7	14.545	1941	1948	1957	rBV	471752	718905	19.03%	3.773%
8	16.040	2195	2202	2215	rBV	1556228	2216147	58.68%	11.631%
9	17.304	2410	2417	2427	rBV	539002	805221	21.32%	4.226%
10	19.869	2847	2853	2859	rBV	2965815	3776829	100.00%	19.821%
11	21.392	3107	3112	3118	rBV	586485	748817	19.83%	3.930%
12	23.810	3516	3523	3532	rVB	374757	795701	21.07%	4.176%




Sum of corrected areas: 19054556

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013024\
Data File : BP019490.D
Acq On : 30 Jan 2024 19:51
Operator : MA/JU
Sample : PB158676BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

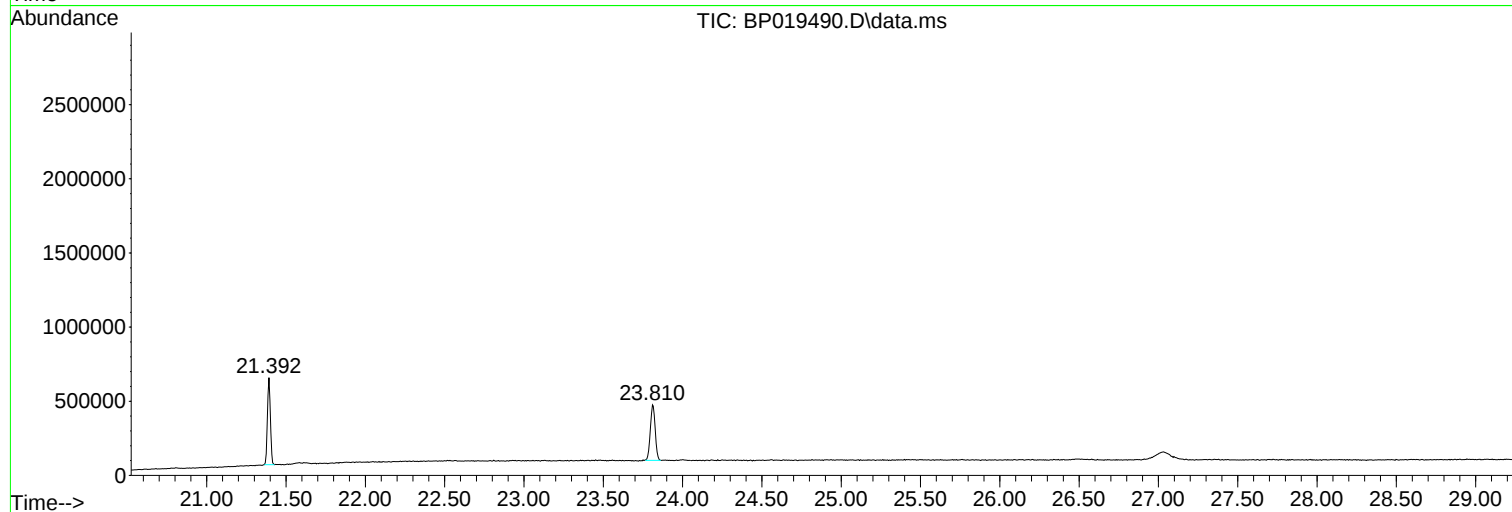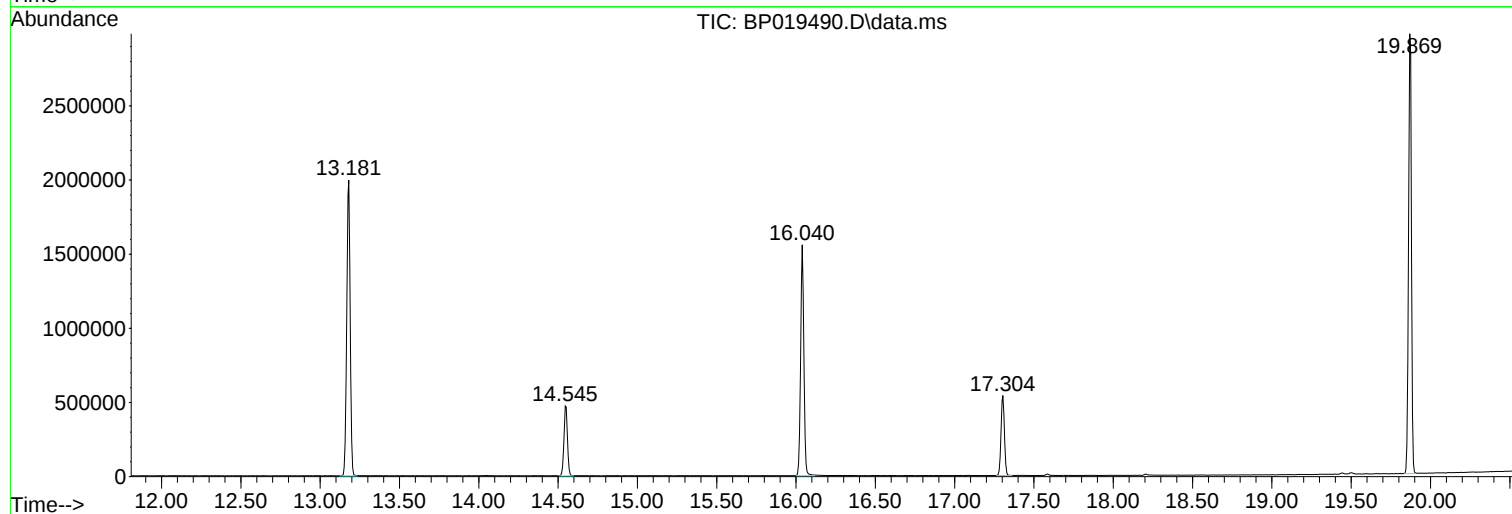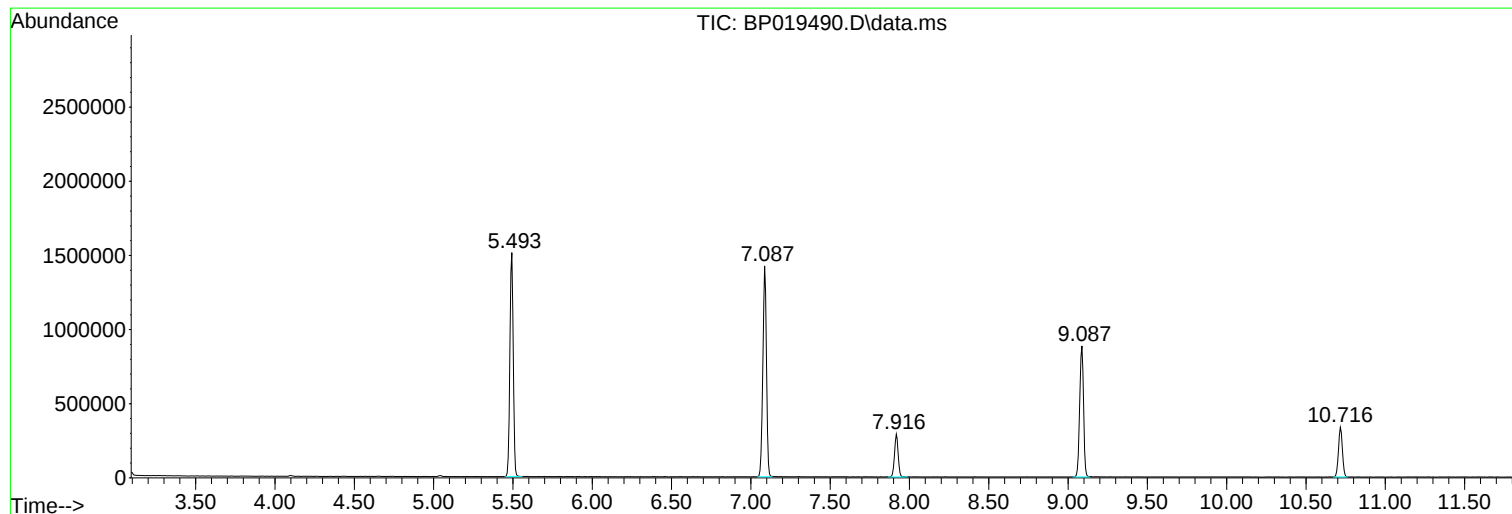

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013024\
Data File : BP019490.D
Acq On : 30 Jan 2024 19:51
Operator : MA/JU
Sample : PB158676BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013024\
Data File : BP019490.D
Acq On : 30 Jan 2024 19:51
Operator : MA/JU
Sample : PB158676BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------