

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
 Data File : BP023806.D
 Acq On : 30 Jan 2025 20:28
 Operator : RC/JU
 Sample : Q1189-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44R3

Quant Time: Jan 31 08:14:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 08:09:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	494806	20.000	ng/u1	0.02
20) Naphthalene-d8	10.557	136	2089902	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.404	164	1347791	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	2724252	20.000	ng/u1	-0.01
79) Chrysene-d12	21.645	240	2921654	20.000	ng/u1	0.00
88) Perylene-d12	25.021	264	3201585	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	41670	3.499	ng/uL	0.01
4) Pyridine-d5	3.711	84	562758	16.376	ng/u1	0.02
7) Phenol-d5	6.964	99	768729	17.555	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.117	67	425694	18.366	ng/u1	0.02
11) 2-Chlorophenol-d4	7.328	132	623793	18.141	ng/u1	0.02
15) 4-Methylphenol-d8	8.487	113	605847	16.937	ng/u1	0.02
21) Nitrobenzene-d5	8.928	128	300684	17.983	ng/u1	0.02
24) 2-Nitrophenol-d4	9.646	143	314072	17.408	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.193	165	585047	17.676	ng/u1	0.02
31) 4-Chloroaniline-d4	10.687	131	771673	15.590	ng/u1	0.00
46) Dimethylphthalate-d6	13.810	166	1932780	19.225	ng/u1	0.00
49) Acenaphthylene-d8	14.093	160	1867628	16.472	ng/u1	0.00
54) 4-Nitrophenol-d4	14.616	143	316846	15.870	ng/u1	0.00
60) Fluorene-d10	15.404	176	1305187	15.417	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	187075	11.131	ng/u1	-0.02
73) Anthracene-d10	17.298	188	1893379	14.155	ng/u1	-0.02
81) Pyrene-d10	19.669	212	1995480	12.747	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.786	264	1648899	9.871	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.993	94	45900	1.021	ng/u1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
Data File : BP023806.D
Acq On : 30 Jan 2025 20:28
Operator : RC/JU
Sample : Q1189-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44R3

Quant Time: Jan 31 08:14:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 08:09:38 2025
Response via : Initial Calibration

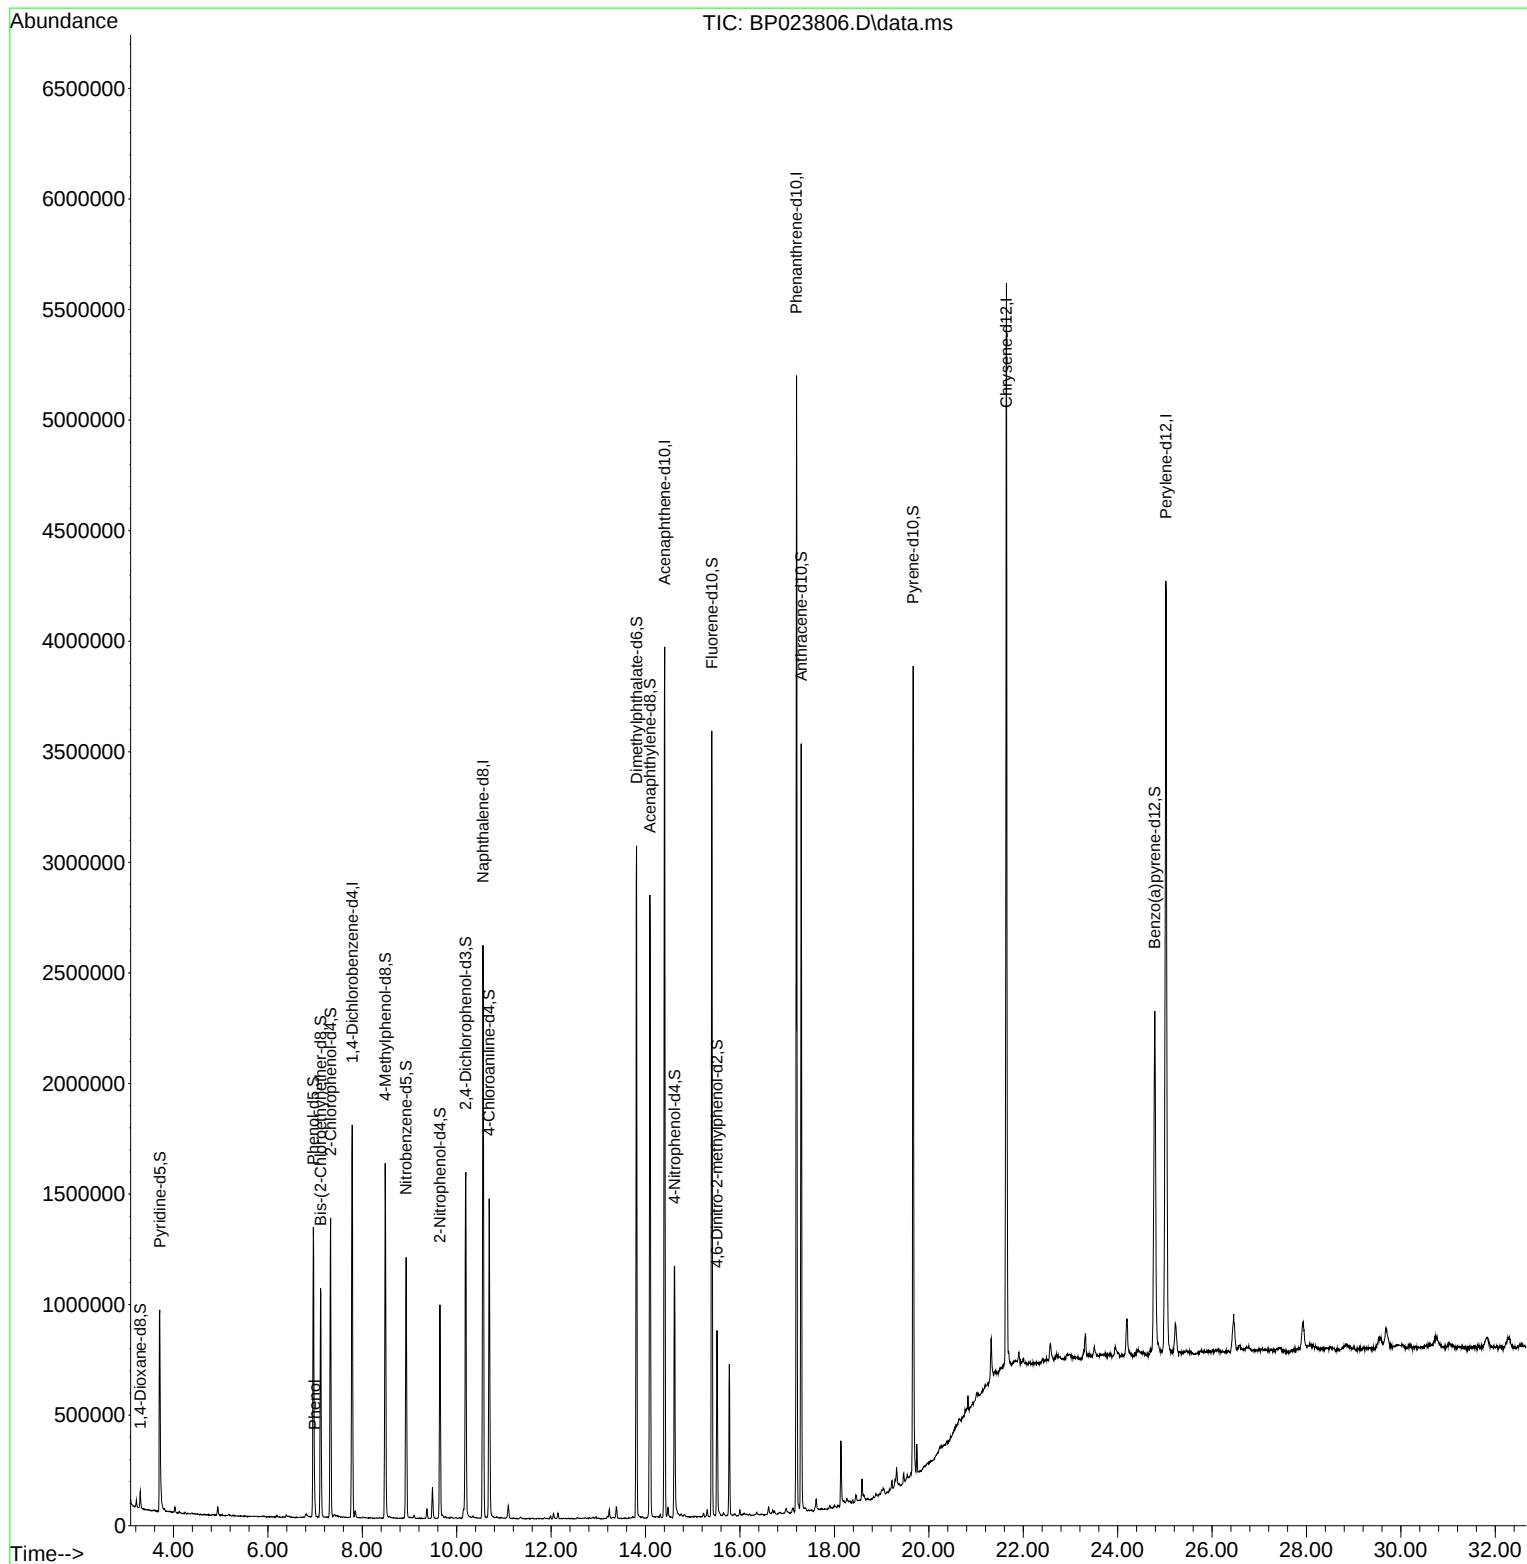

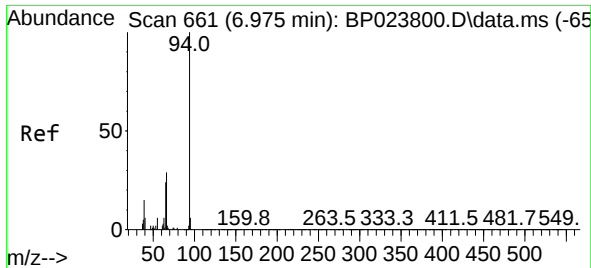

#8
Phenol
Concen: 1.021 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. 0.018 min
Lab File: BP023806.D
Acq: 30 Jan 2025 20:28

Instrument :
BNA_P
ClientSampleId :
A44R3

Tgt Ion: 94	Resp:	45900
Ion	Ratio	Lower Upper
94	100	
65	29.3	20.1 30.1
66	36.0	26.0 39.0

