

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
 Data File : BP023810.D
 Acq On : 30 Jan 2025 23:10
 Operator : RC/JU
 Sample : Q1192-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	42	rVB	101637	122516	0.85%	0.104%
2	3.717	103	107	122	rBV	280364	449741	3.13%	0.380%
3	4.034	157	161	166	rVB	23802	35199	0.25%	0.030%
4	4.128	173	177	186	rVB4	27957	41629	0.29%	0.035%
5	4.940	310	315	320	rVB2	15157	27511	0.19%	0.023%
6	6.193	523	528	535	rVB3	22216	33627	0.23%	0.028%
7	6.964	650	659	667	rBV	519396	793481	5.53%	0.671%
8	7.122	678	686	696	rBV	1465500	2341737	16.32%	1.980%
9	7.328	713	721	733	rBV	1696162	2564849	17.87%	2.168%
10	7.781	791	798	807	rBV	1692582	2467774	17.20%	2.086%
11	8.481	911	917	926	rBV	1478412	2237193	15.59%	1.891%
12	8.922	983	992	1005	rBV	1696848	2736483	19.07%	2.314%
13	9.369	1061	1068	1079	rVB	224861	352075	2.45%	0.298%
14	9.640	1107	1114	1130	rBV	1267271	2152001	15.00%	1.819%
15	10.187	1198	1207	1224	rBV	2284497	3559060	24.80%	3.009%
16	10.558	1263	1270	1283	rVB	2239816	3613686	25.18%	3.055%
17	10.687	1285	1292	1303	rBV	1971454	3033266	21.14%	2.565%
18	11.352	1399	1405	1411	rBV10	7578	18029	0.13%	0.015%
19	11.857	1485	1491	1498	rVB	152402	231124	1.61%	0.195%
20	12.146	1534	1540	1548	rVB	34013	61622	0.43%	0.052%
21	13.810	1815	1823	1828	rBV	4371114	6135990	42.76%	5.188%
22	13.857	1828	1831	1837	rVB2	36228	57068	0.40%	0.048%
23	14.093	1864	1871	1883	rBV	4958789	7094993	49.44%	5.999%
24	14.404	1917	1924	1933	rBV	3673539	5061901	35.27%	4.280%
25	14.610	1953	1959	1973	rBV	460378	754359	5.26%	0.638%
26	14.828	1991	1996	2001	rBV8	10536	19209	0.13%	0.016%
27	15.234	2060	2065	2070	rVB2	14302	24223	0.17%	0.020%
28	15.410	2088	2095	2107	rBV	6612538	9519112	66.33%	8.048%
29	15.516	2107	2113	2127	rVV	1978778	2581813	17.99%	2.183%
30	15.645	2132	2135	2146	rVB	28304	53004	0.37%	0.045%
31	16.869	2335	2343	2347	rBV10	11166	20393	0.14%	0.017%
32	16.975	2357	2361	2366	rVB2	15624	24631	0.17%	0.021%
33	17.192	2391	2398	2408	rBV2	4258922	6005982	41.85%	5.078%
34	17.292	2408	2415	2427	rBV2	8042959	11389470	79.37%	9.629%
35	17.892	2513	2517	2525	rVB10	17403	24145	0.17%	0.020%
36	18.128	2553	2557	2562	rBV7	23971	43497	0.30%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
Data File : BP023810.D
Acq On : 30 Jan 2025 23:10
Operator : RC/JU
Sample : Q1192-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	19.210	2736	2741	2747	rBV2	83385	132768	0.93%	0.112%
38	19.286	2749	2754	2758	rBV	87584	117091	0.82%	0.099%
39	19.663	2812	2818	2828	rBV	11586000	13884609	96.75%	11.739%
40	21.628	3147	3152	3161	rBV2	4345704	6830417	47.60%	5.775%
41	24.786	3678	3689	3708	rVB	4940932	14350421	100.00%	12.133%
42	25.016	3719	3728	3742	rVB	2644292	7280516	50.73%	6.155%




Sum of corrected areas: 118278215

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
Data File : BP023810.D
Acq On : 30 Jan 2025 23:10
Operator : RC/JU
Sample : Q1192-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

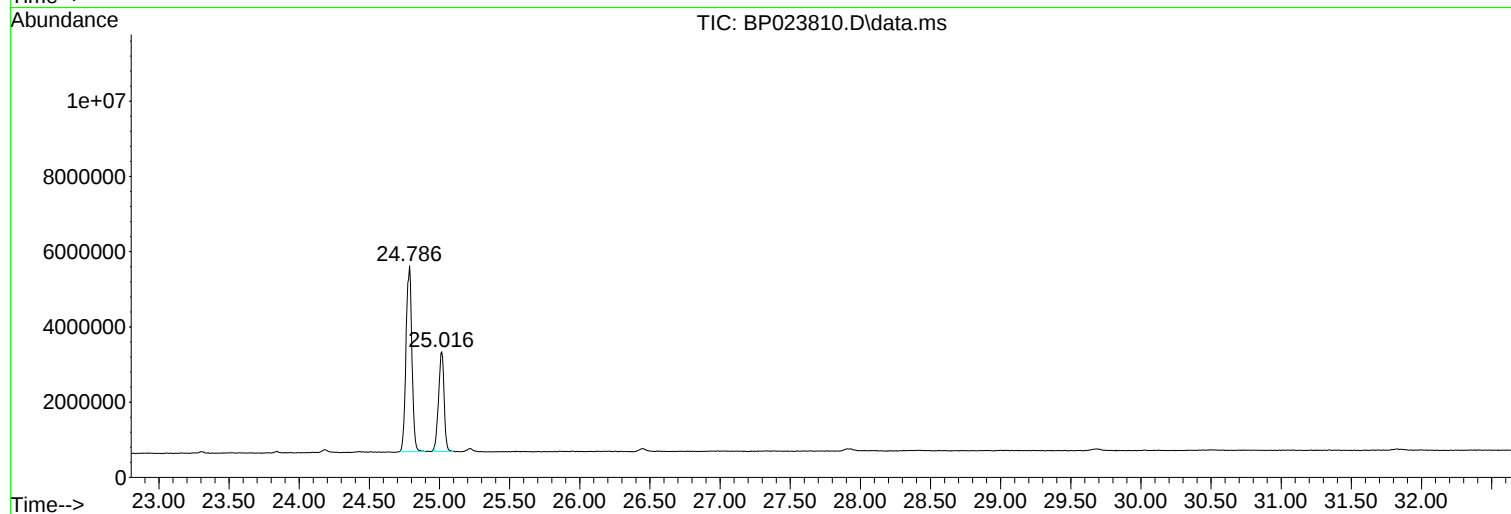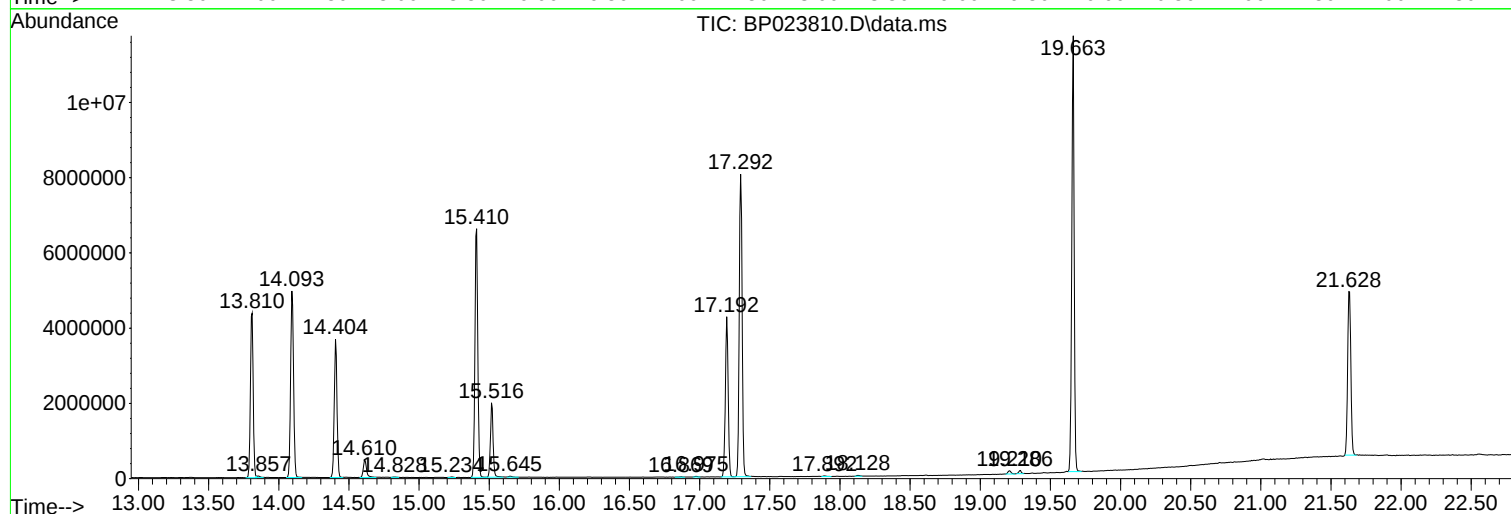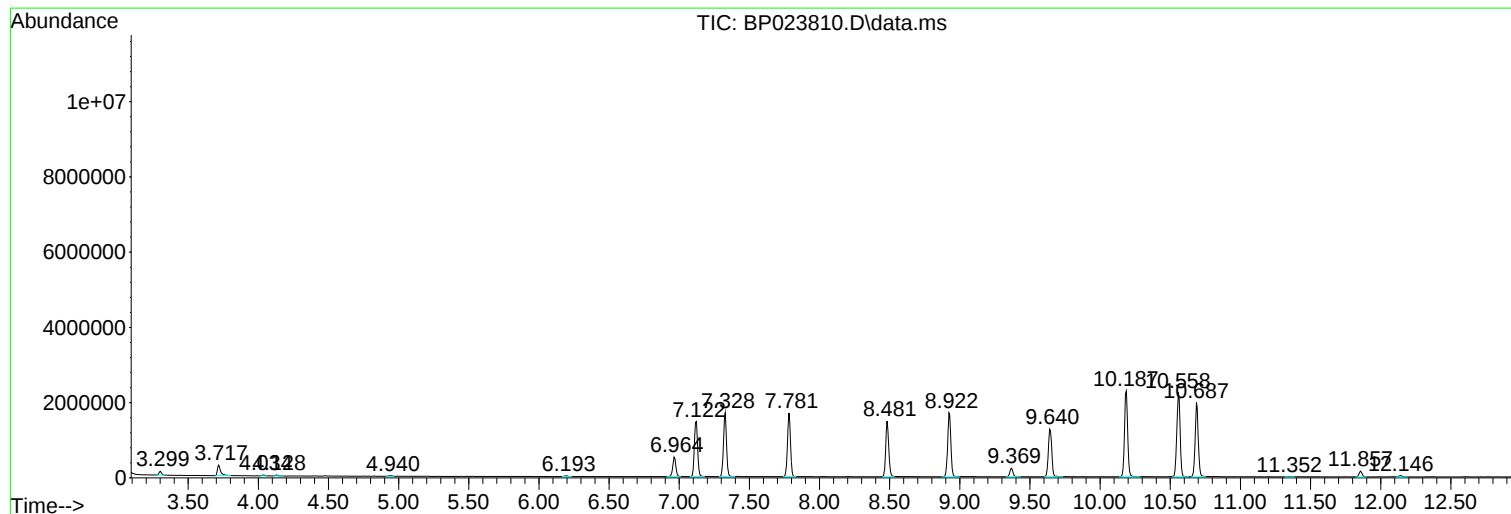

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
Data File : BP023810.D
Acq On : 30 Jan 2025 23:10
Operator : RC/JU
Sample : Q1192-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013025\
Data File : BP023810.D
Acq On : 30 Jan 2025 23:10
Operator : RC/JU
Sample : Q1192-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
