
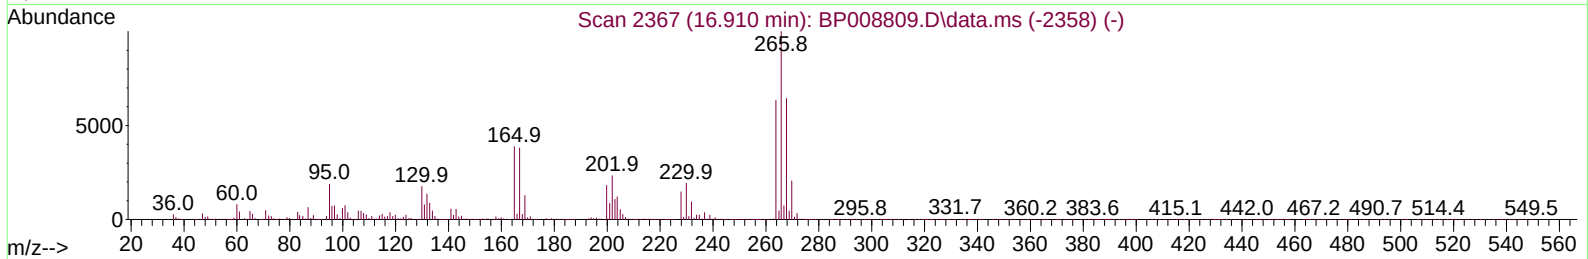
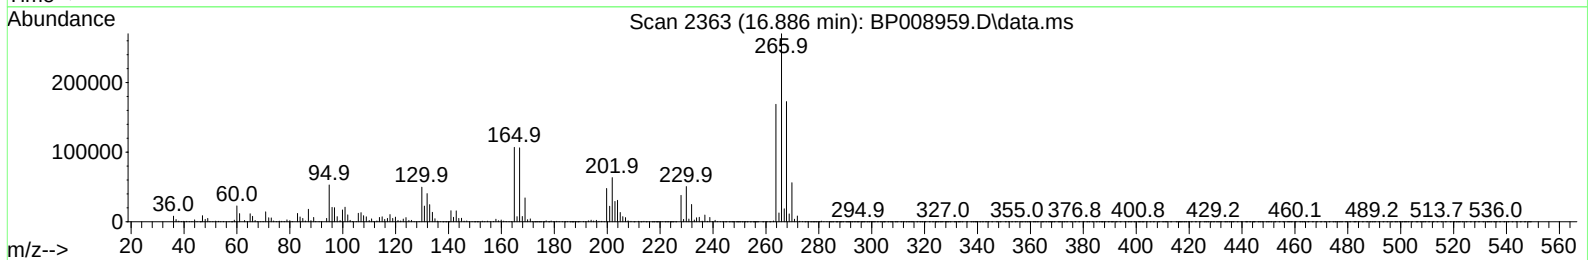


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013122\
 Data File : BP008959.D
 Acq On : 31 Jan 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 06:36:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 04:16:03 2022
 Response via : Initial Calibration

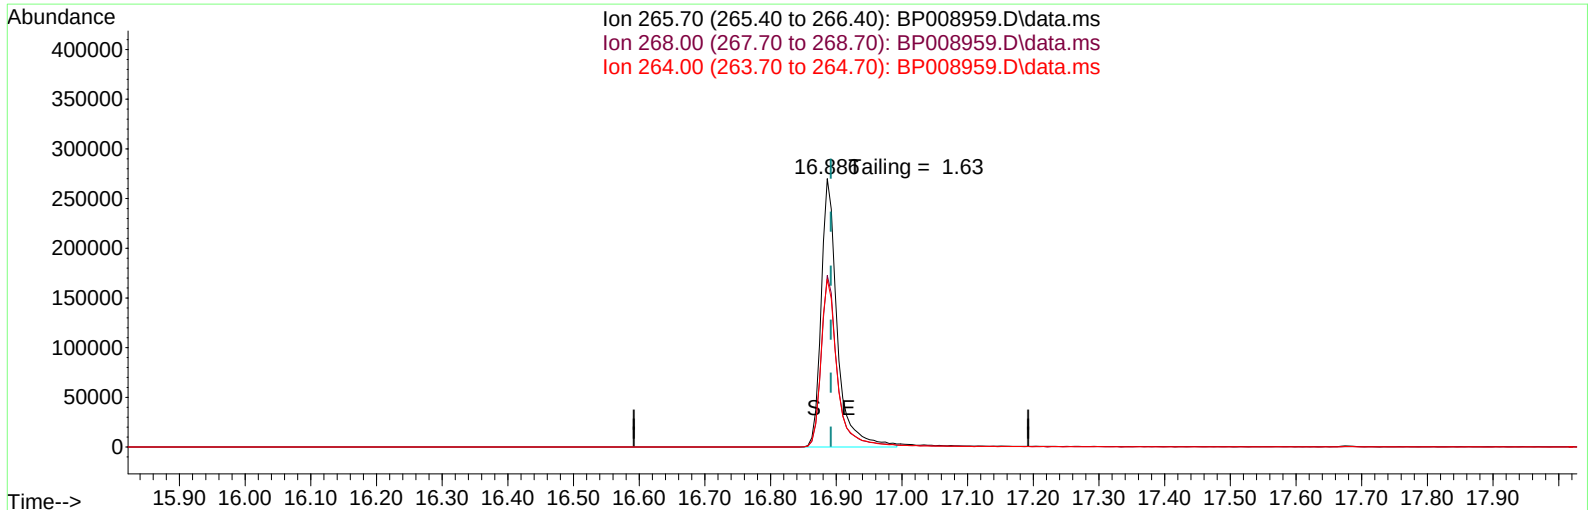

TIC: BP008959.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.006) 1654010.60 ng

response 466446

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.93
264.00	62.90	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013122\
Data File : BP008959.D
Acq On : 31 Jan 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 06:36:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

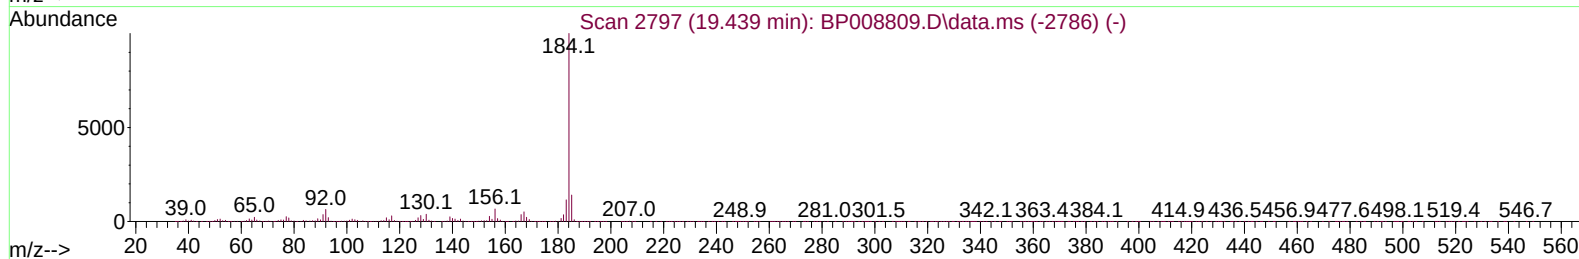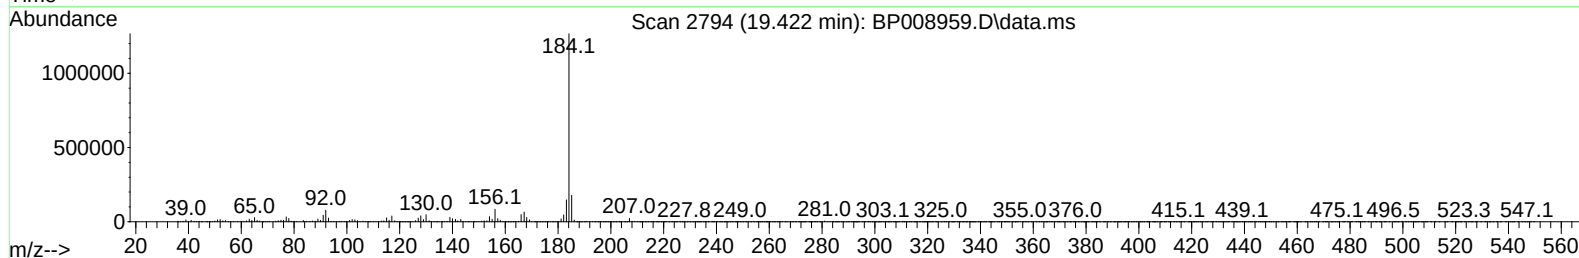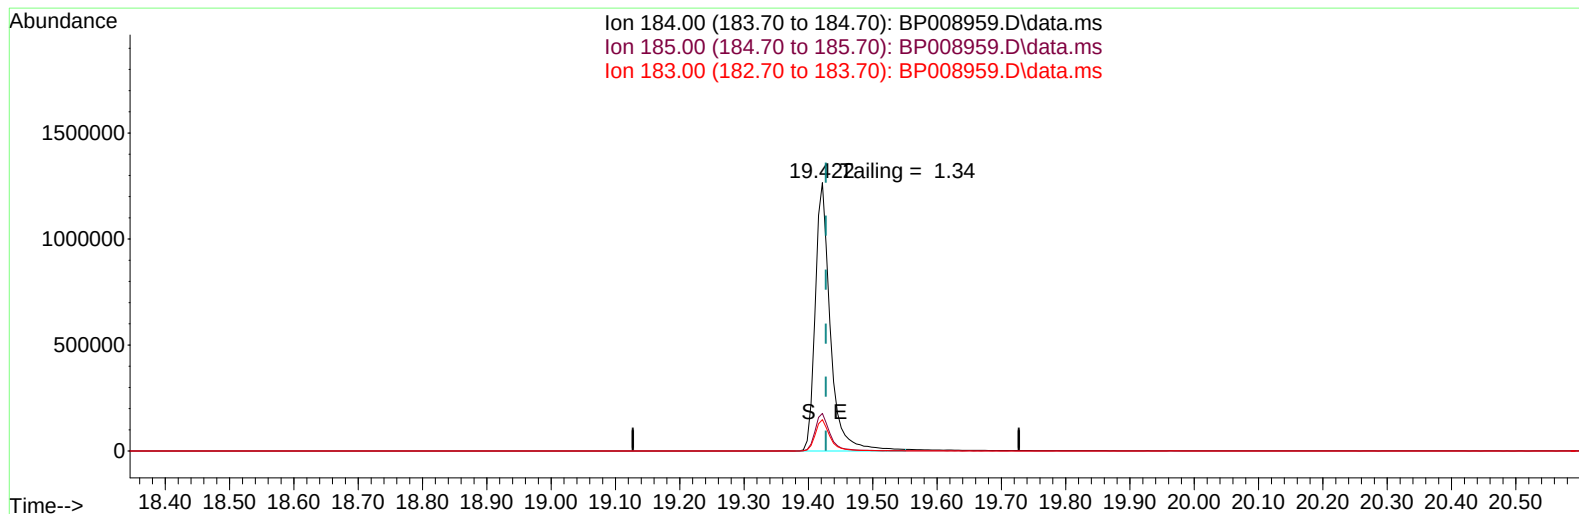

TIC: BP008959.D\data.ms

(77) Benzidine

19.422min (-0.006) 579216.03 ng

response 2087167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.90	11.70
0.00	0.00	0.00