
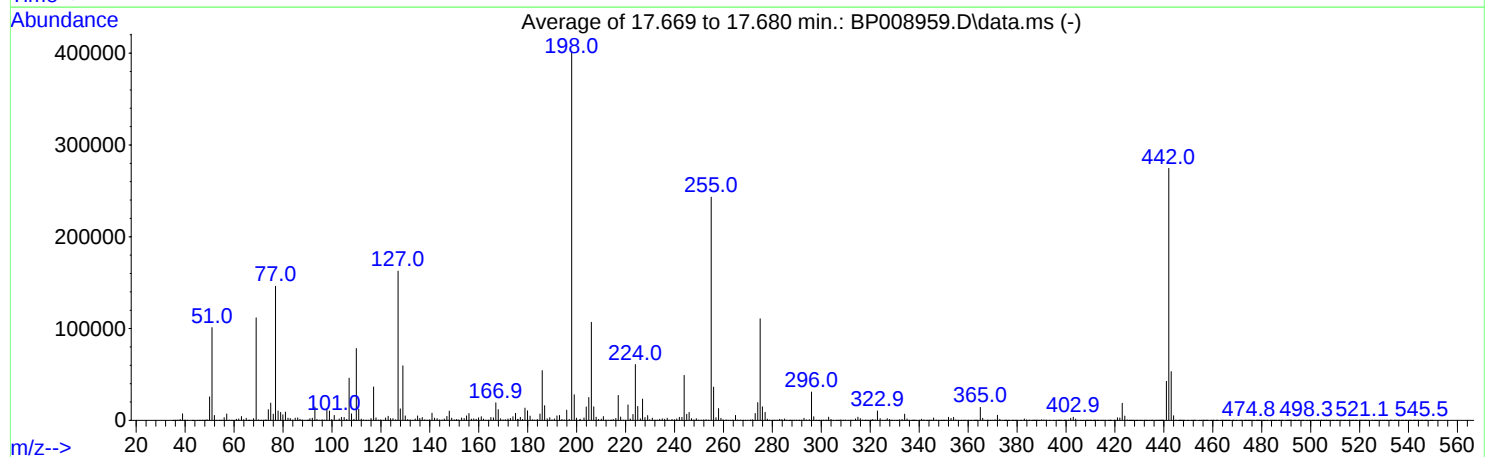


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013122\
 Data File : BP008959.D
 Acq On : 31 Jan 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 01 04:16:03 2022

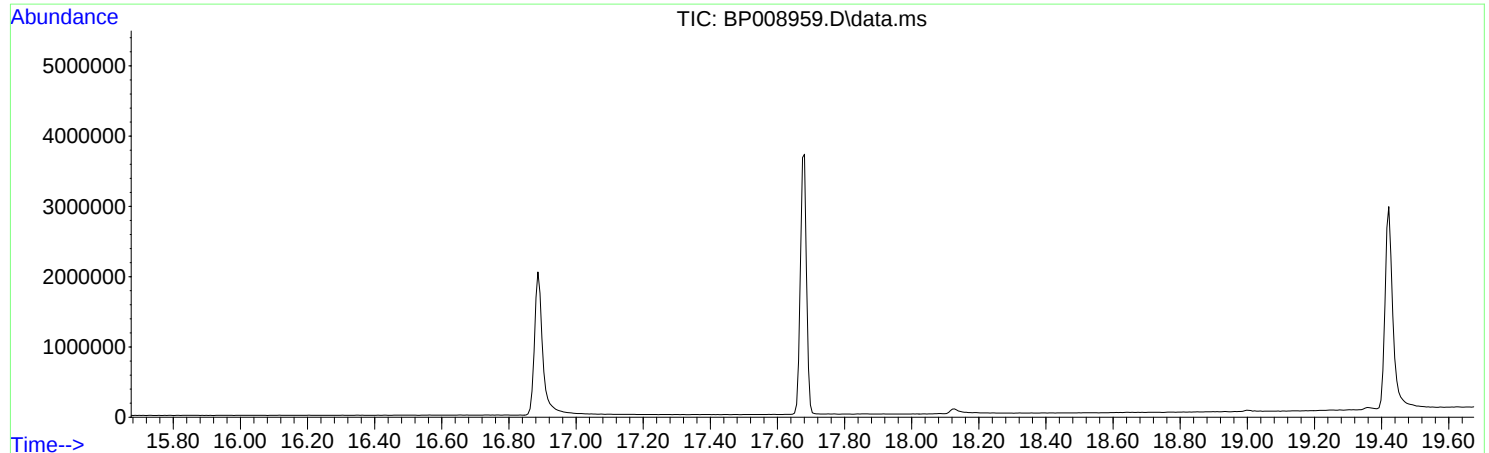




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	101182	PASS
68	69	0.00	2	1.7	1877	PASS
69	198	0.00	100	27.9	111666	PASS
70	69	0.00	2	0.5	547	PASS
127	198	10	80	40.6	162553	PASS
197	198	0.00	2	0.3	1060	PASS
198	198	100	100	100.0	400712	PASS
199	198	5	9	7.0	27955	PASS
275	198	10	60	27.6	110748	PASS
365	198	1	100	3.5	14197	PASS
441	198	0.01	100	10.6	42480	PASS
442	442	100	100	100.0	274453	PASS
443	442	15	24	19.4	53147	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013122\
Data File : BP008959.D
Acq On : 31 Jan 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 01 06:36:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

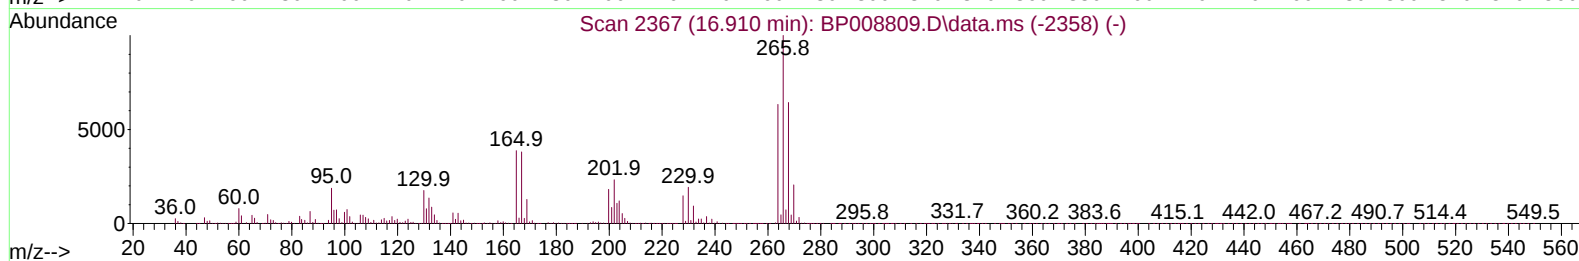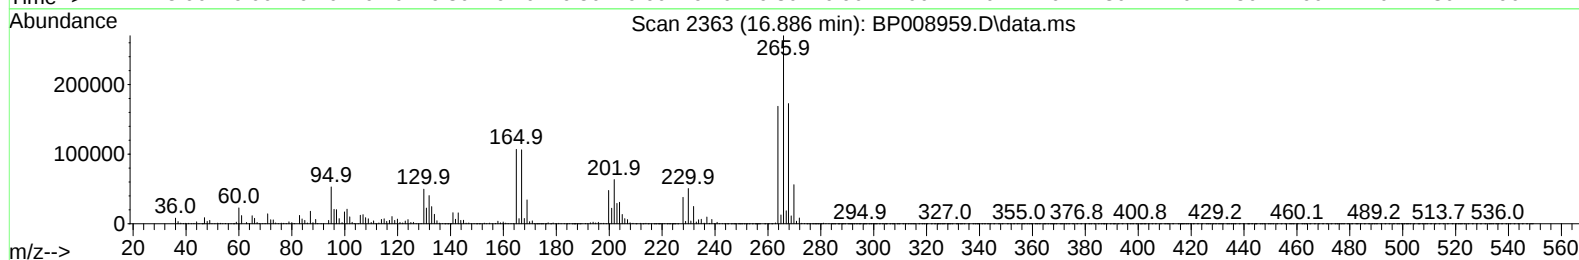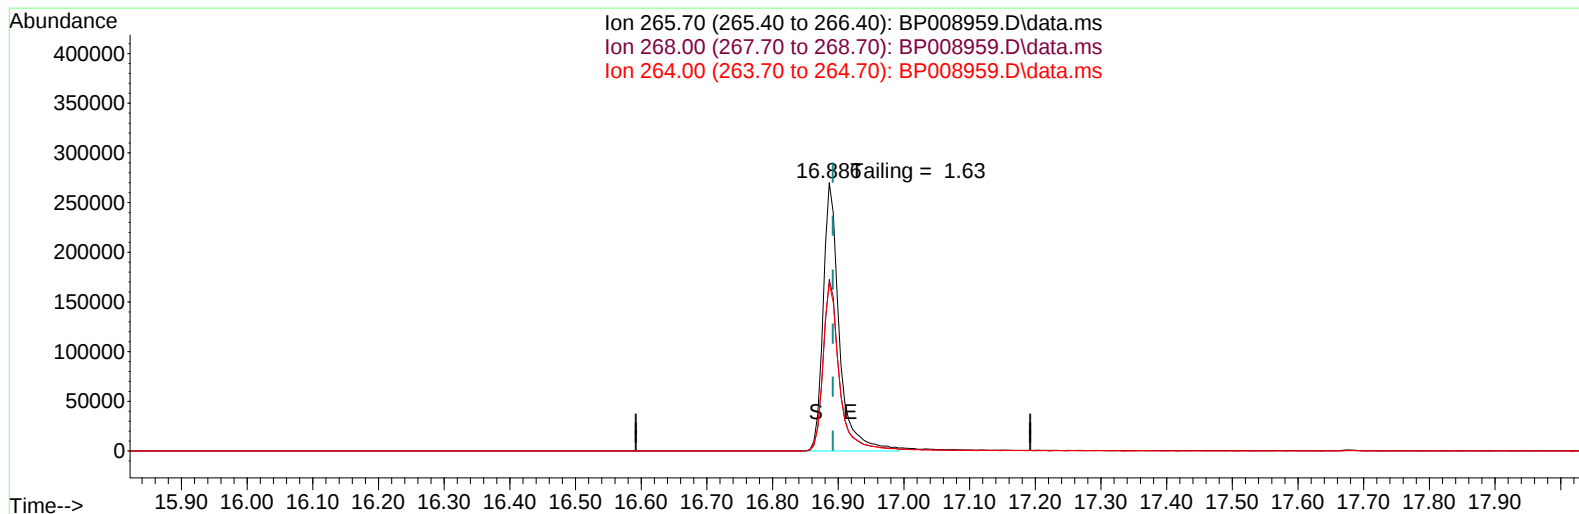

TIC: BP008959.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 1654010.60 ng




response 466446

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.93
264.00	62.90	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013122\
Data File : BP008959.D
Acq On : 31 Jan 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 01 06:36:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 04:16:03 2022
Response via : Initial Calibration

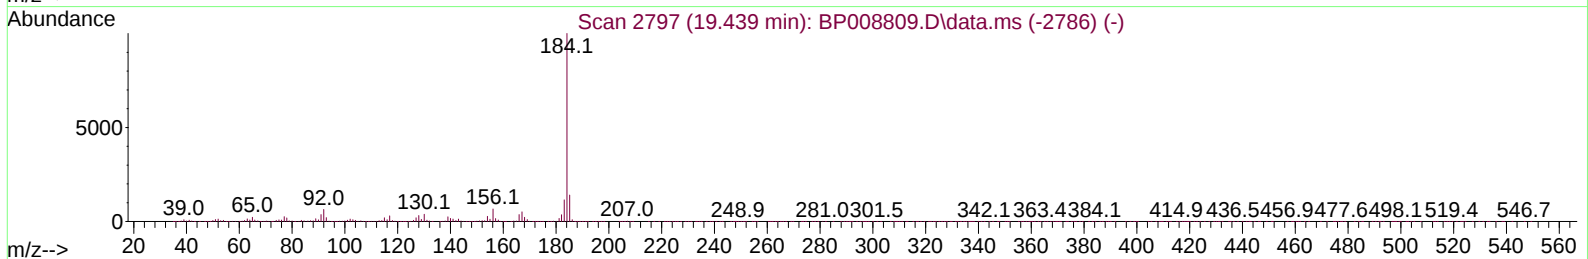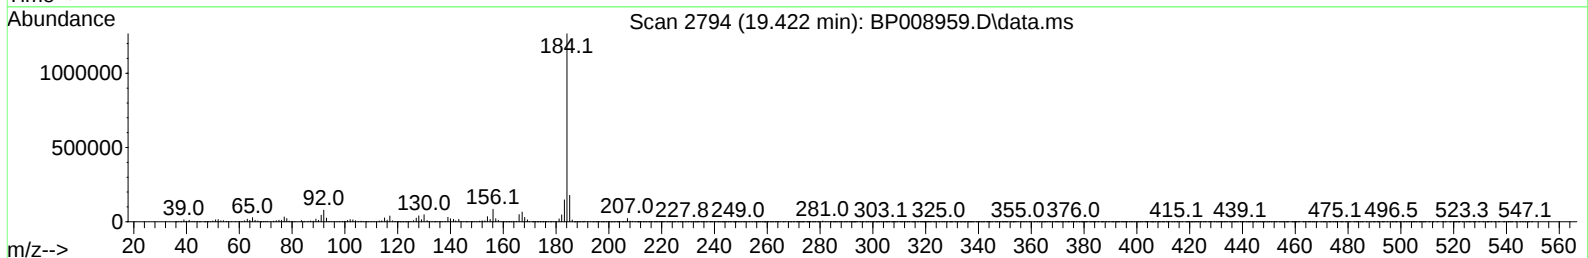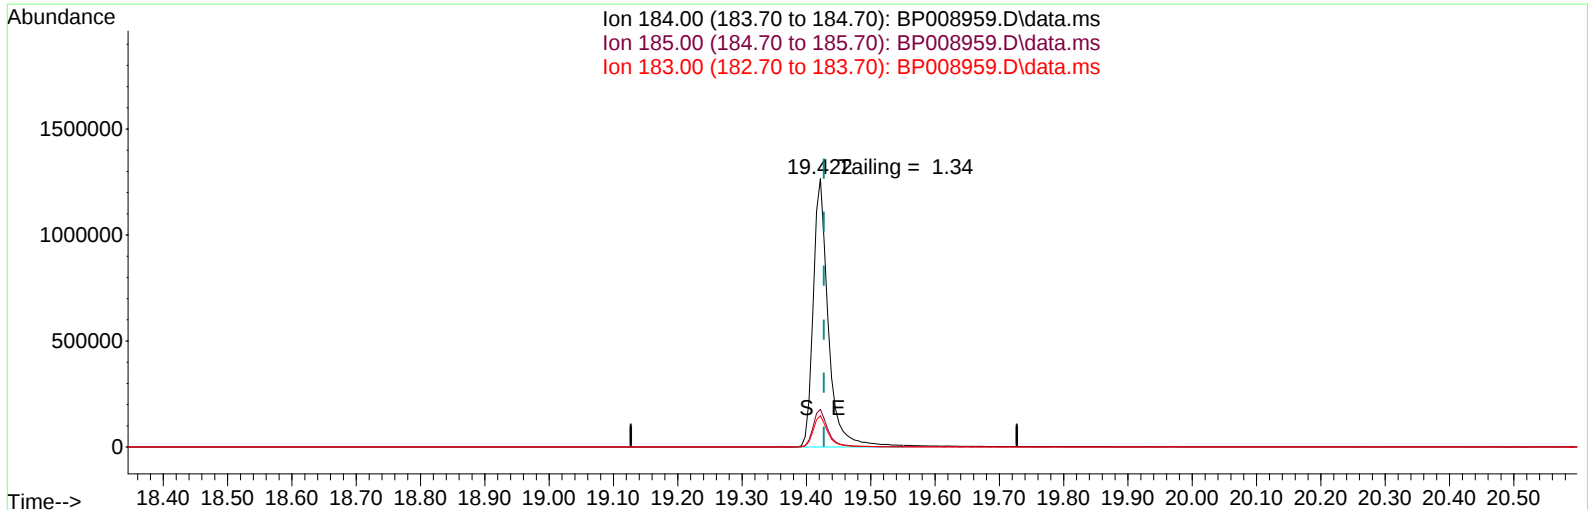

TIC: BP008959.D\data.ms

(77) Benzidine

19.422min (-0.006) 579216.03 ng

response 2087167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.90	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2022	BNA_P	<u>BP008959.D</u>
Compound Name	Response	Retention Time
DDT	1227261	20.622
DDD	44462	20.192
DDE	4801	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49263	1276524	3.86

Instrument :
BNA_P
ClientSampleId :
DFTPP