
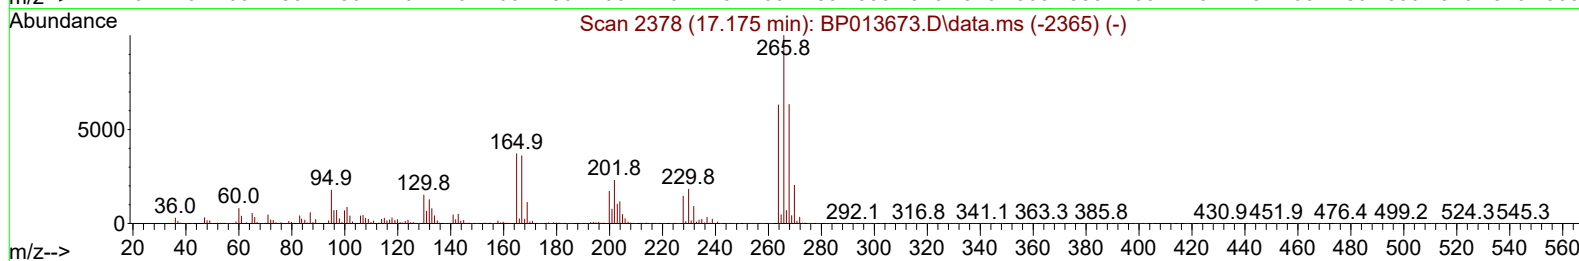
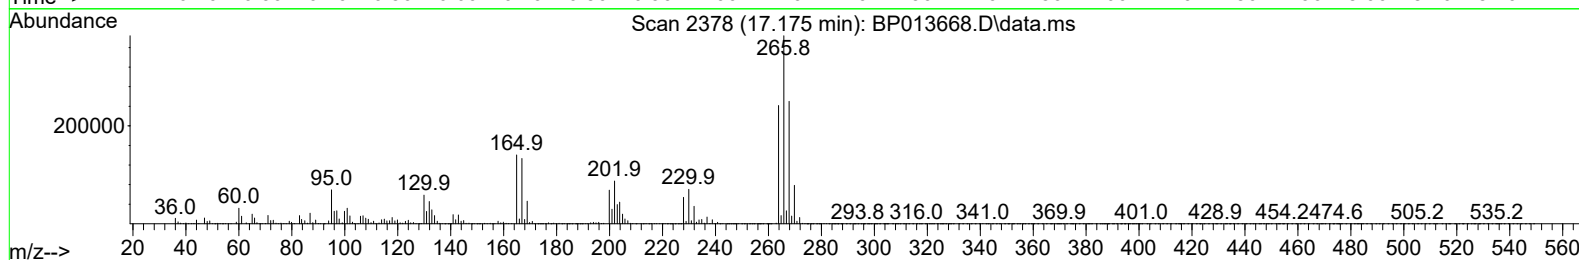


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
Data File : BP013668.D
Acq On : 31 Jan 2023 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 08:00:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 03:43:48 2023
Response via : Initial Calibration

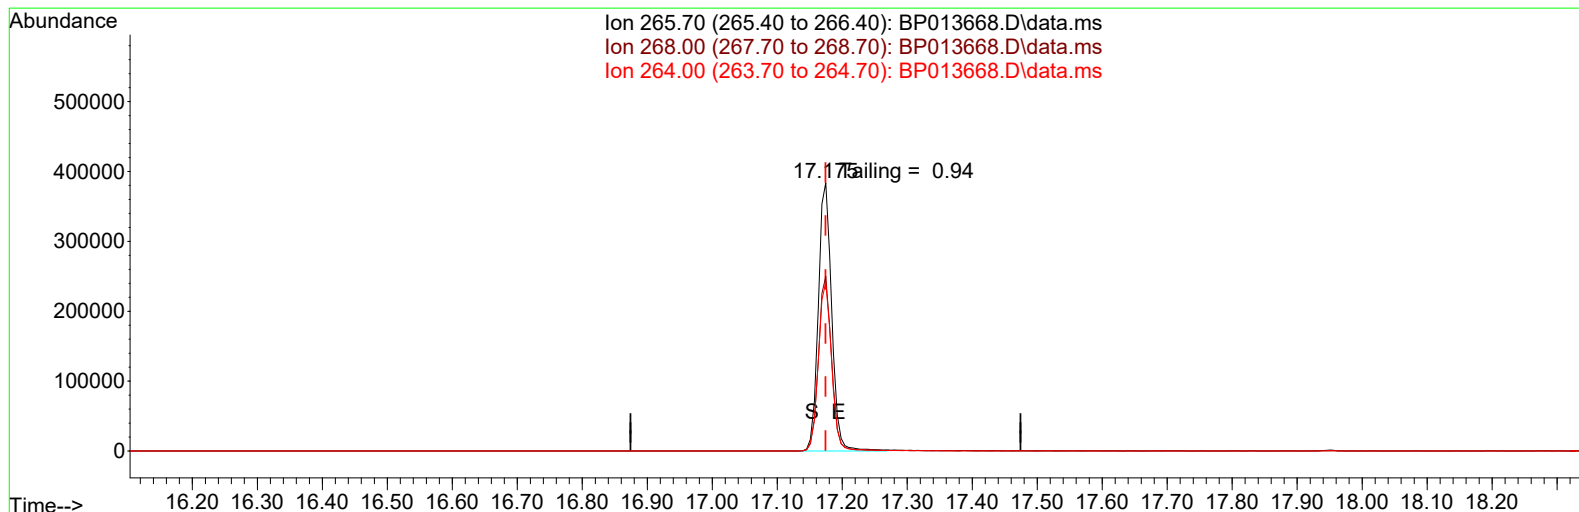

TIC: BP013668.D\data.ms

(70) Pentachlorophenol (C)




17.175min (+ 0.000) 2464284.36 ng

response 553780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	65.07
264.00	63.10	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
Data File : BP013668.D
Acq On : 31 Jan 2023 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 08:00:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 03:43:48 2023
Response via : Initial Calibration

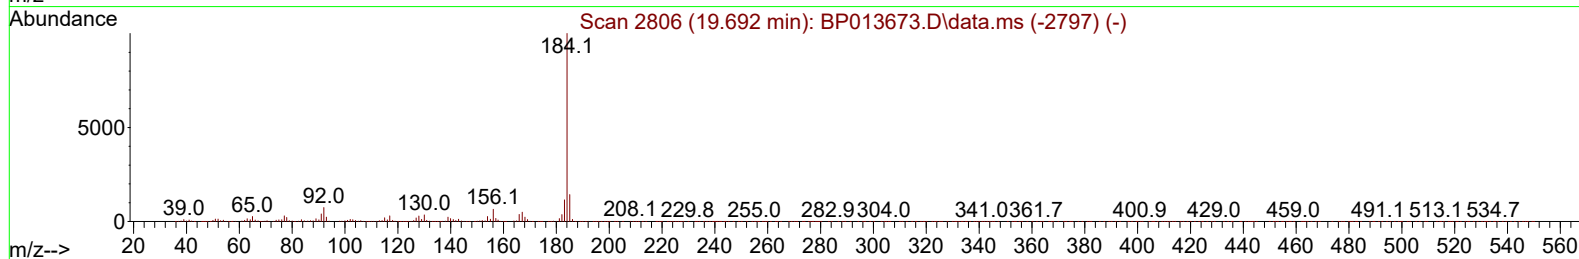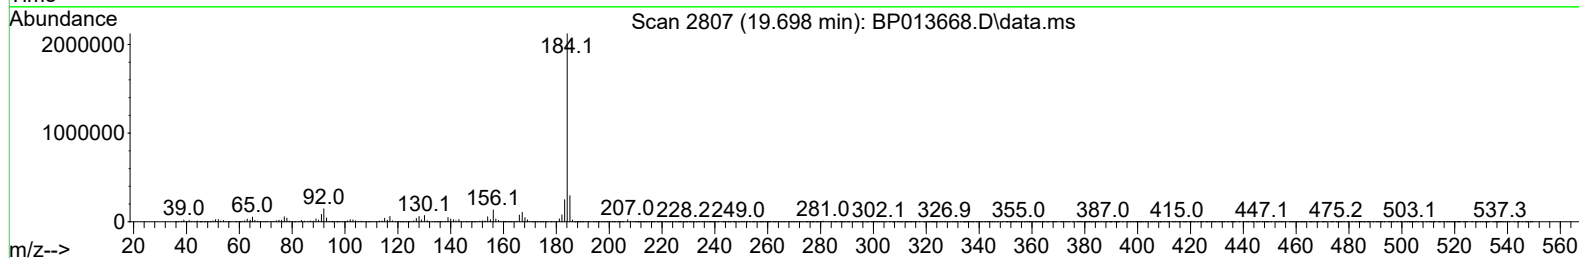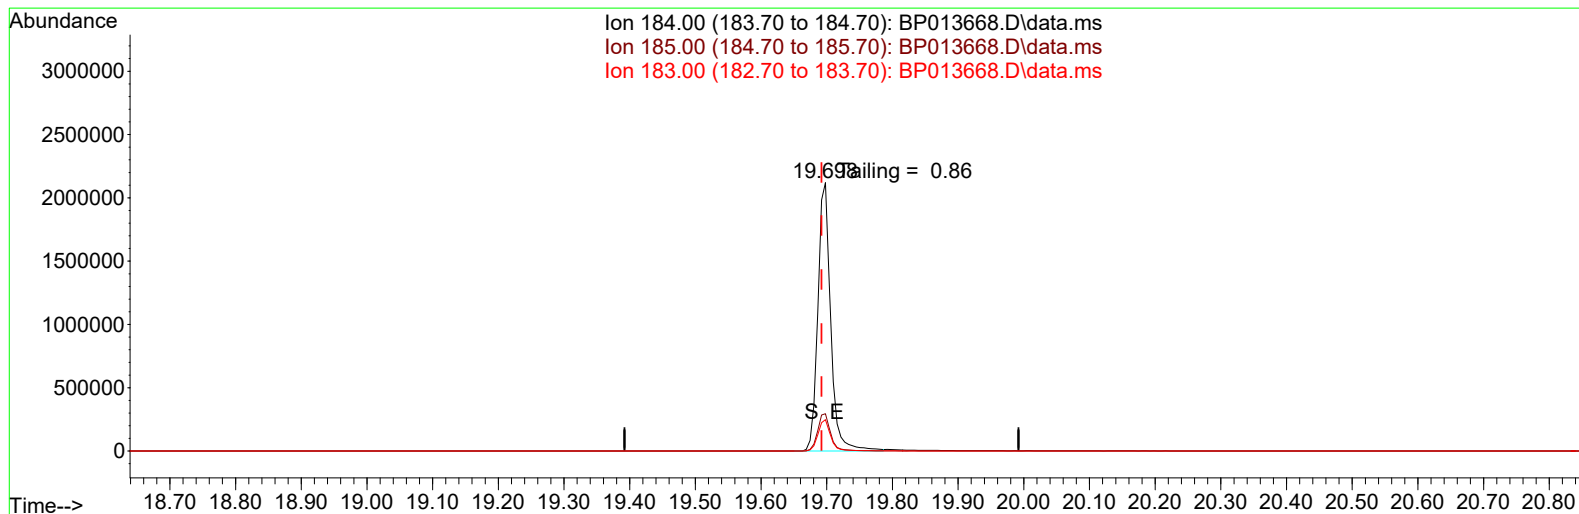

TIC: BP013668.D\data.ms

(77) Benzidine**19.698min (+ 0.006) 2755273.69 ng****response 2916120**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.90
183.00	11.50	11.72
0.00	0.00	0.00