

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
 Data File : BP013683.D
 Acq On : 31 Jan 2023 20:30
 Operator : CG/JU
 Sample : PB150501BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150501BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	337	343	354	rBV	2242175	3086571	17.86%	3.763%
2	5.675	414	423	439	rBV	5595236	8265850	47.82%	10.077%
3	7.287	688	697	715	rBV	5144738	8370362	48.43%	10.205%
4	8.140	833	842	850	rBV	1077568	1666473	9.64%	2.032%
5	9.316	1033	1042	1055	rBV	2912725	4860245	28.12%	5.925%
6	10.969	1312	1323	1333	rBV	1311081	2240600	12.96%	2.732%
7	13.404	1729	1737	1750	rBV	8681426	12899145	74.63%	15.726%
8	14.775	1963	1970	1984	rBV	2092311	3120068	18.05%	3.804%
9	16.263	2214	2223	2245	rBV	6886178	9660299	55.89%	11.777%
10	17.527	2431	2438	2451	rBV	2591603	3709152	21.46%	4.522%
11	19.751	2812	2816	2820	rBV	167833	194604	1.13%	0.237%
12	20.057	2863	2868	2882	rBV	13497019	17284642	100.00%	21.072%
13	21.604	3126	3131	3137	rBV	2535734	3436060	19.88%	4.189%
14	24.180	3562	3569	3580	rVB2	1466745	3231292	18.69%	3.939%




Sum of corrected areas: 82025363

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
Data File : BP013683.D
Acq On : 31 Jan 2023 20:30
Operator : CG/JU
Sample : PB150501BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150501BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

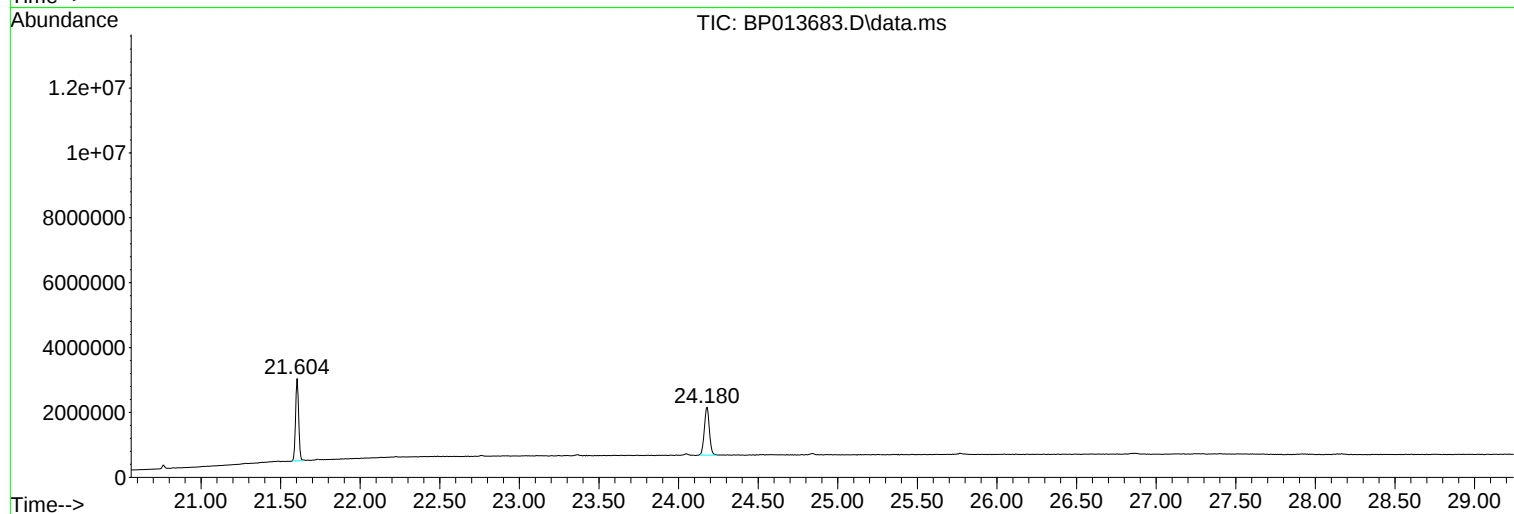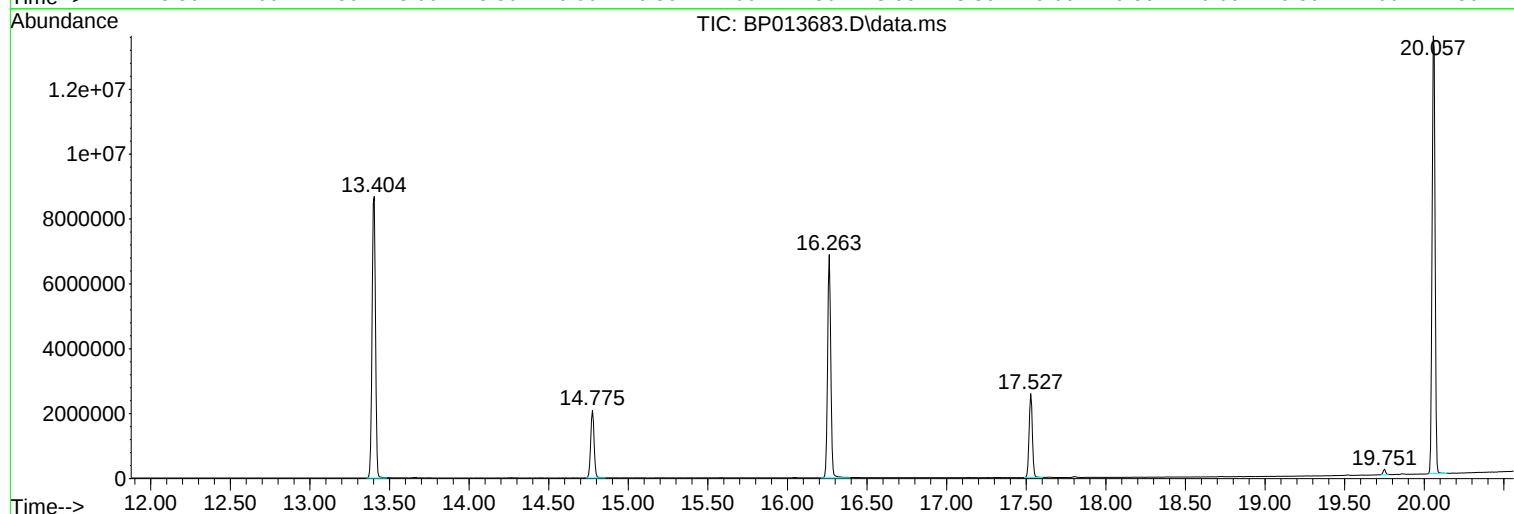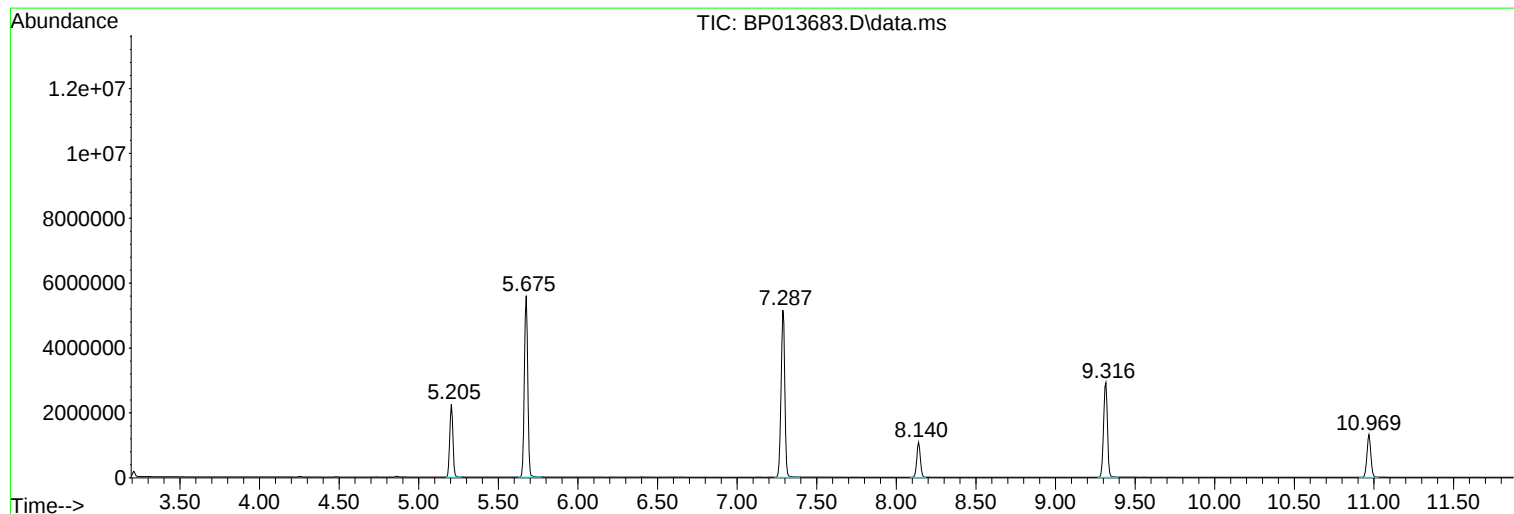

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
Data File : BP013683.D
Acq On : 31 Jan 2023 20:30
Operator : CG/JU
Sample : PB150501BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150501BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.205	37.04 ng	3086570	1,4-Dichlorobenzene-d4	8.140

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5			5-Hexen-2-one	98	C6H10O	000109-49-9	9

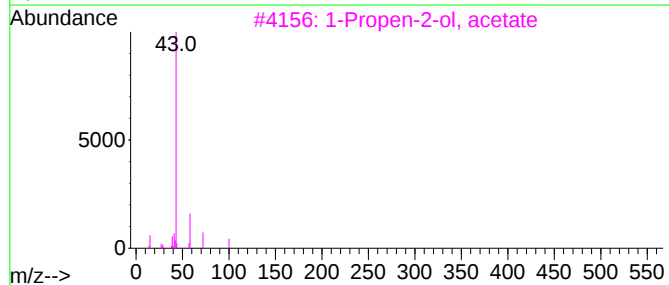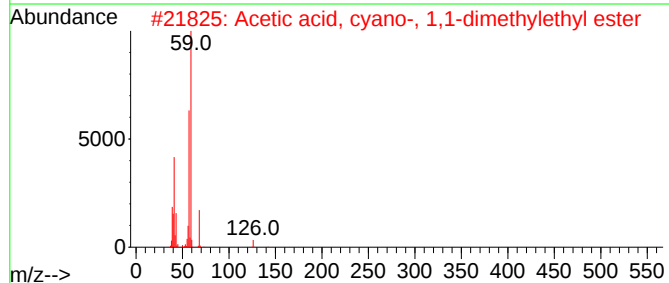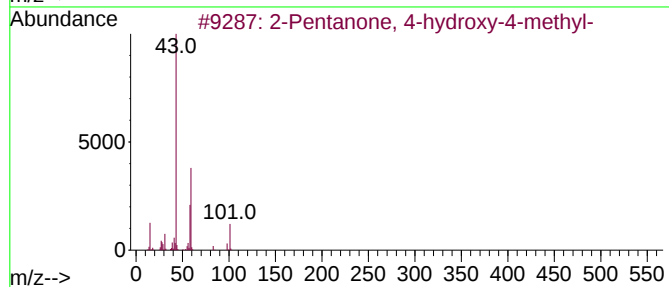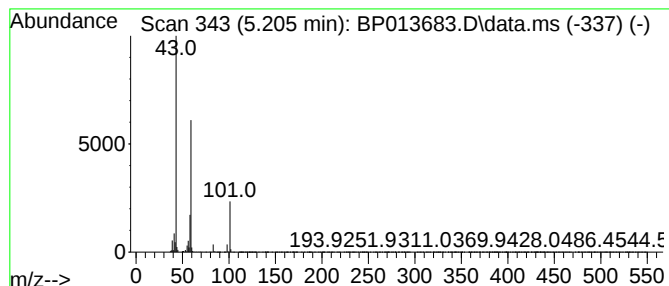

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013123\
Data File : BP013683.D
Acq On : 31 Jan 2023 20:30
Operator : CG/JU
Sample : PB150501BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150501BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.205	37.0	ng	3086570	1	8.140	1666470	20.0