
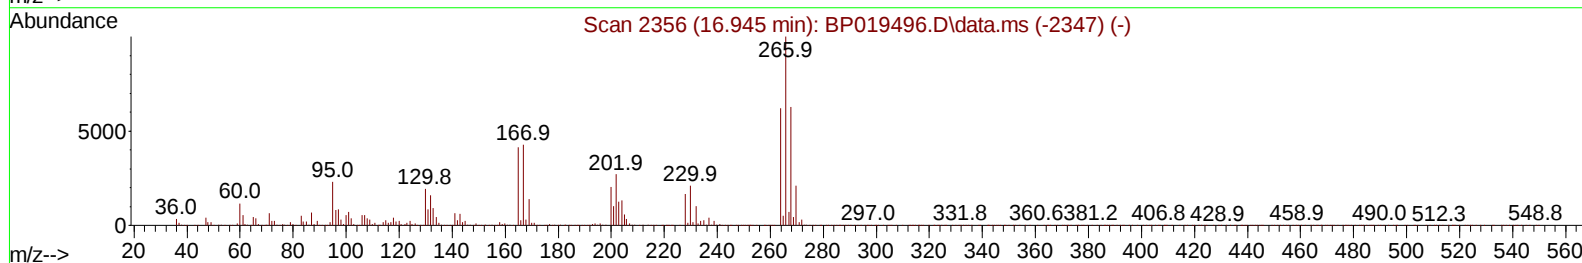
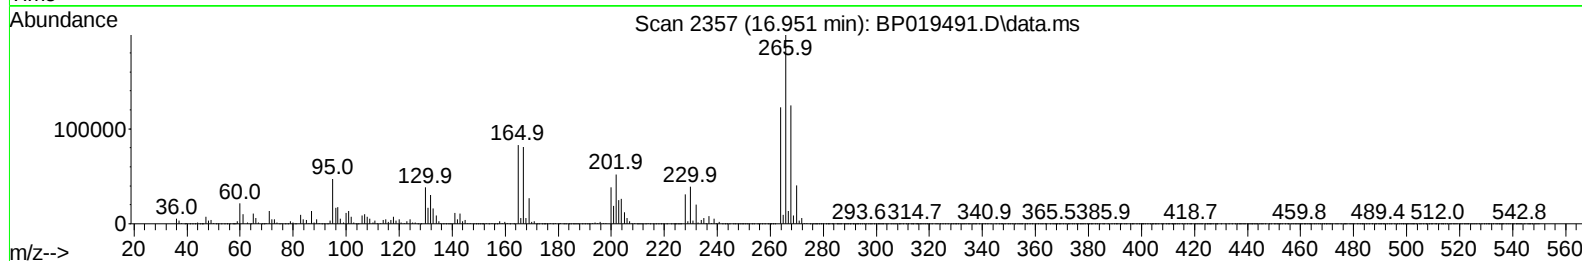


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013124\
Data File : BP019491.D
Acq On : 31 Jan 2024 13:42
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 01:37:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

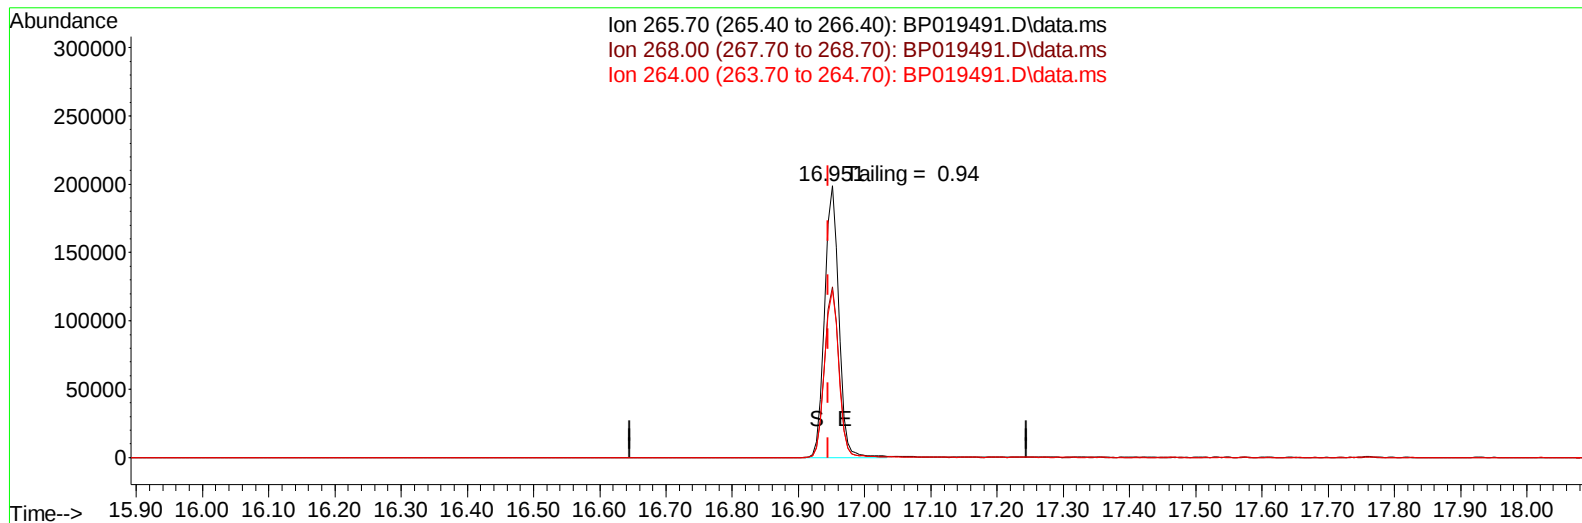

TIC: BP019491.D\data.ms

(70) Pentachlorophenol (C)




16.951min (+ 0.006) 189422.55 ng

response 292753

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.74
264.00	62.10	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013124\
Data File : BP019491.D
Acq On : 31 Jan 2024 13:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 01:37:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

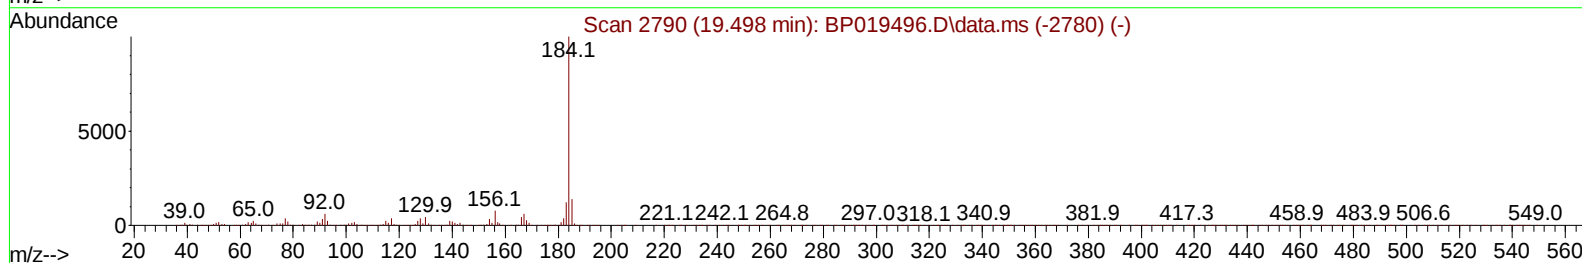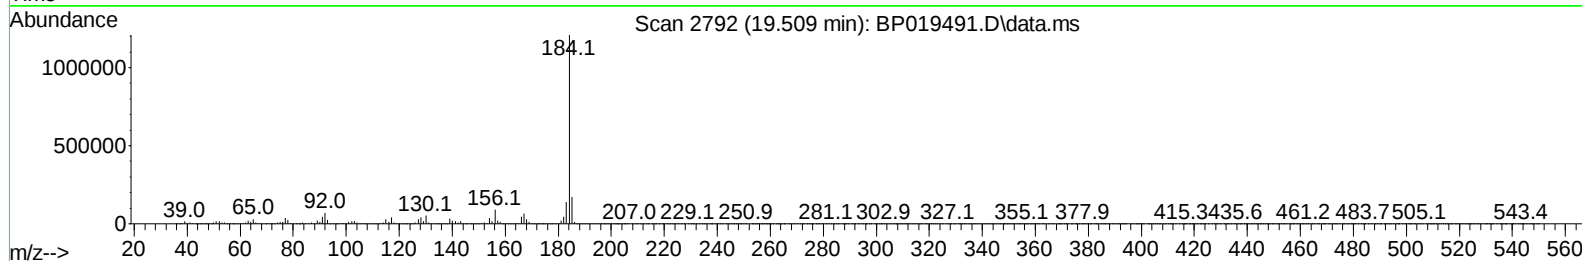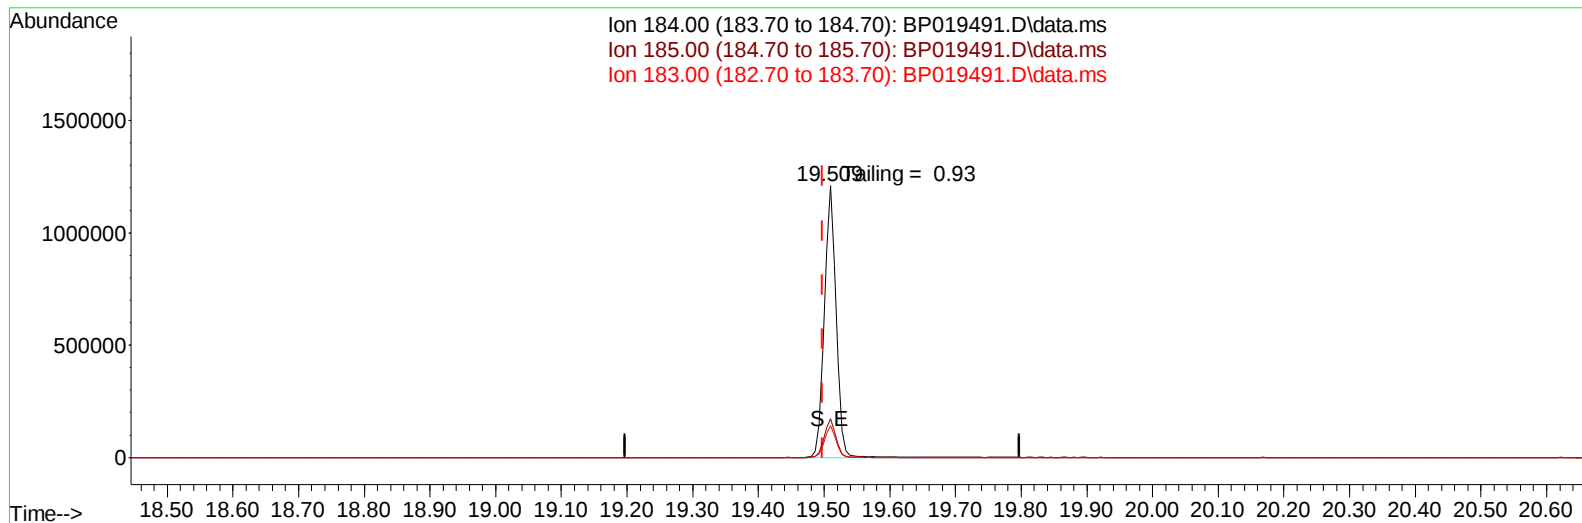

TIC: BP019491.D\data.ms

(77) Benzidine**19.509min (+ 0.012) 41749.72 ng****response 1508281**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.22
183.00	12.10	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2024	BNA_P	<u>BP019491.D</u>
Compound Name	Response	Retention Time
DDT	747332	20.709
DDD	14745	20.28
DDE	353	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15098	762430	1.98