
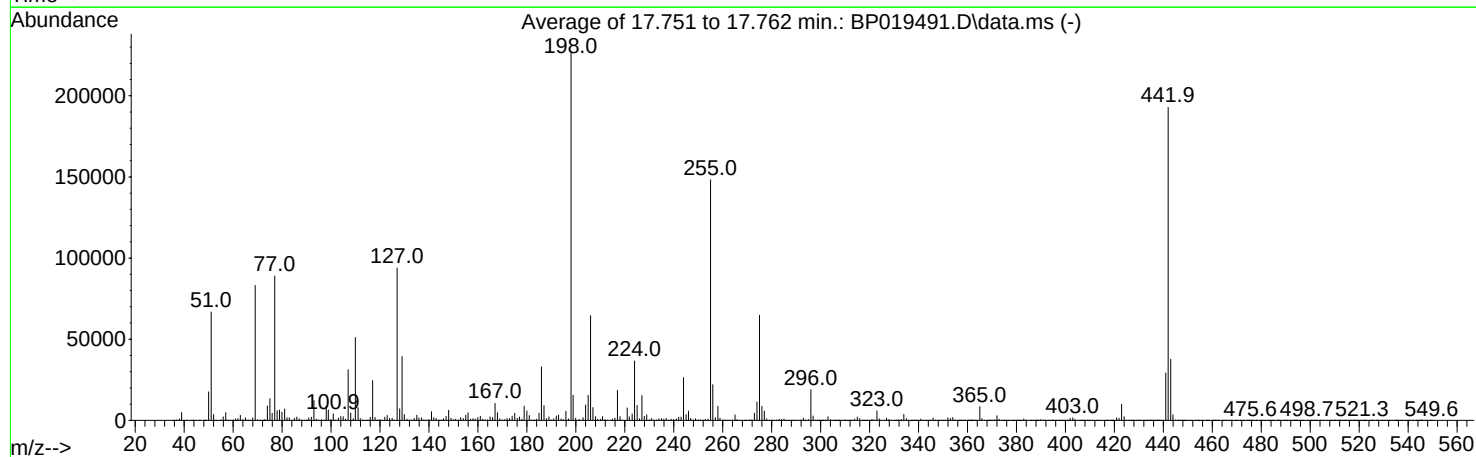


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013124\
Data File : BP019491.D
Acq On : 31 Jan 2024 13:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

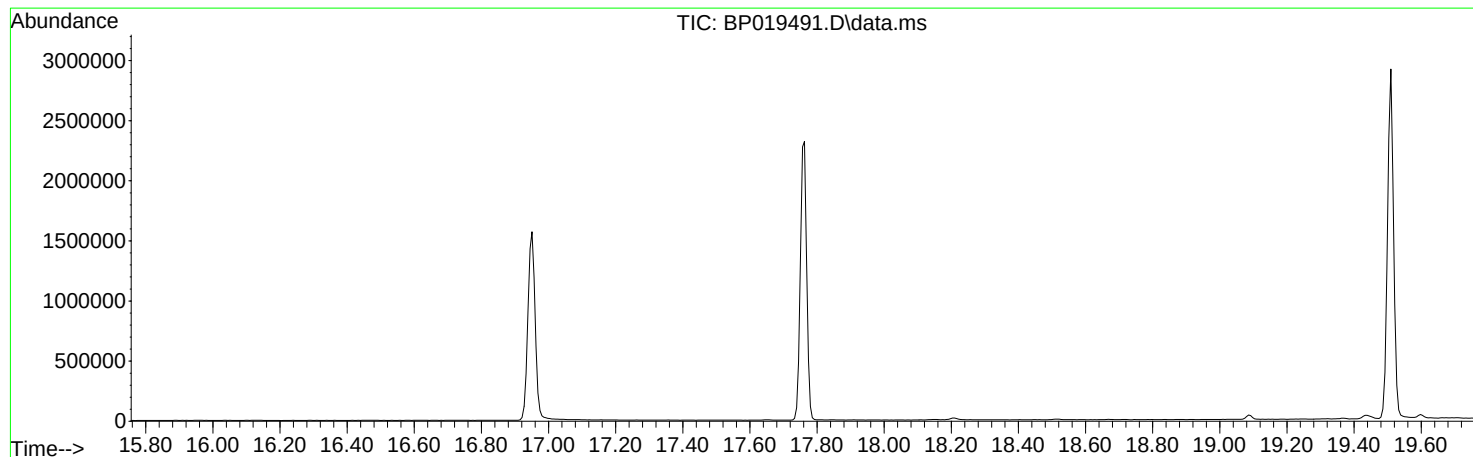




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	29.4	66751	PASS
68	69	0.00	2	1.7	1445	PASS
69	198	0.00	100	36.7	83163	PASS
70	69	0.00	2	0.5	448	PASS
127	198	10	80	41.4	93891	PASS
197	198	0.00	2	0.4	921	PASS
198	198	100	100	100.0	226660	PASS
199	198	5	9	6.8	15462	PASS
275	198	10	60	28.6	64801	PASS
365	198	1	100	3.8	8500	PASS
441	198	0.01	100	12.9	29140	PASS
442	442	100	100	100.0	192843	PASS
443	442	15	24	19.6	37712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013124\
 Data File : BP019491.D
 Acq On : 31 Jan 2024 13:42
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 01 01:37:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 00:51:48 2024
 Response via : Initial Calibration

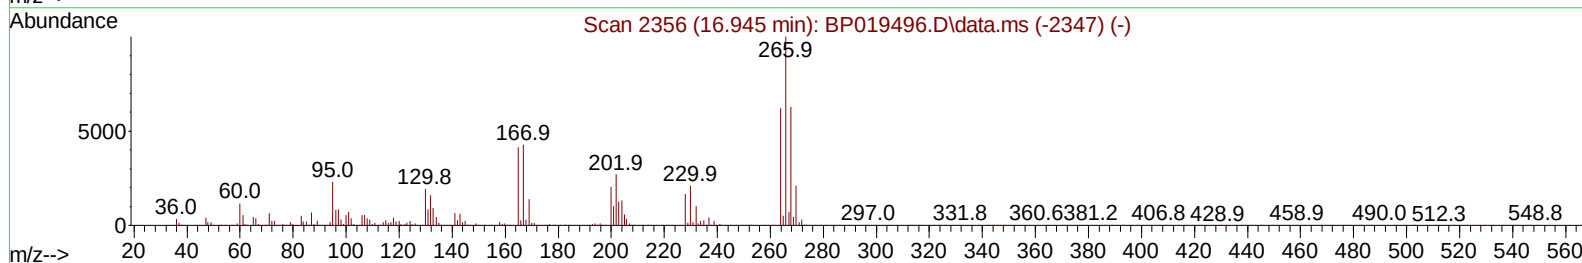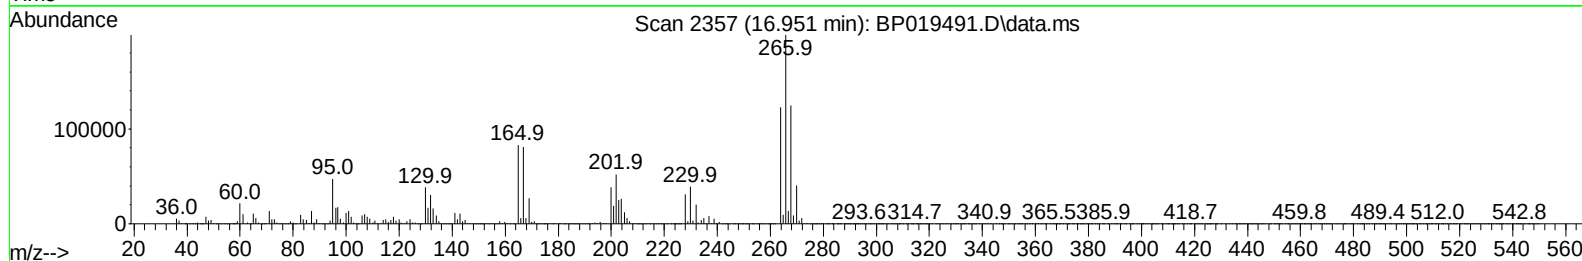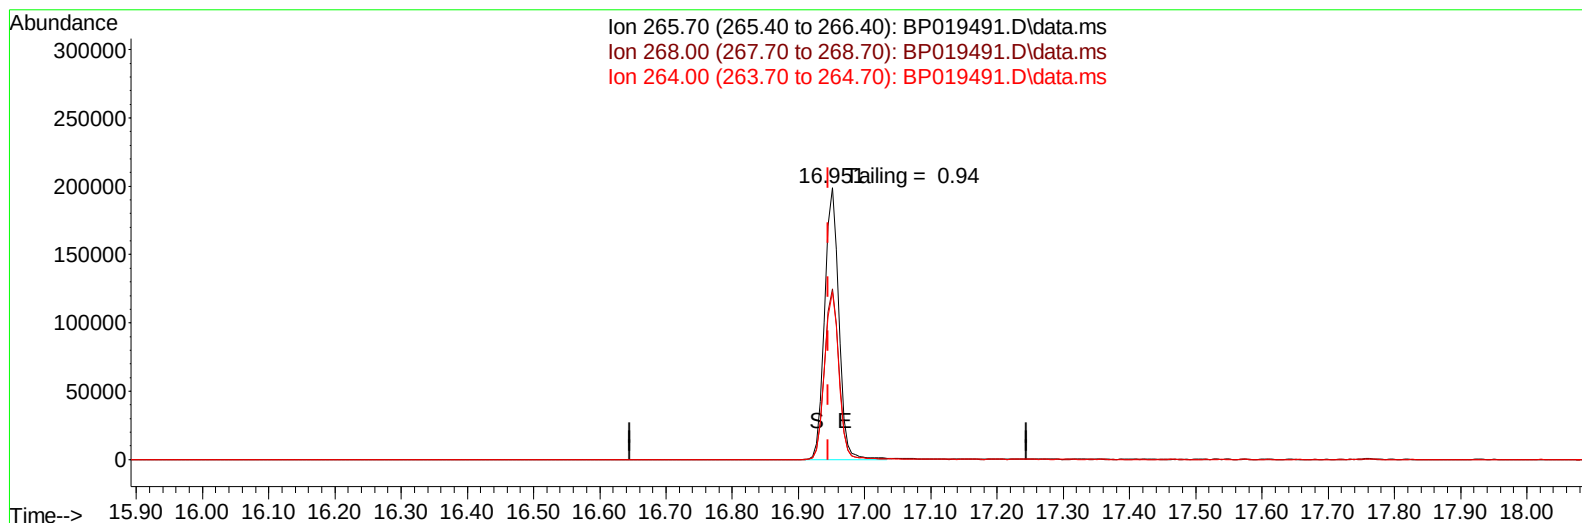

TIC: BP019491.D\data.ms

(70) Pentachlorophenol (C)

16.951min (+ 0.006) 189422.55 ng




response 292753

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.74
264.00	62.10	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013124\
Data File : BP019491.D
Acq On : 31 Jan 2024 13:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 01 01:37:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

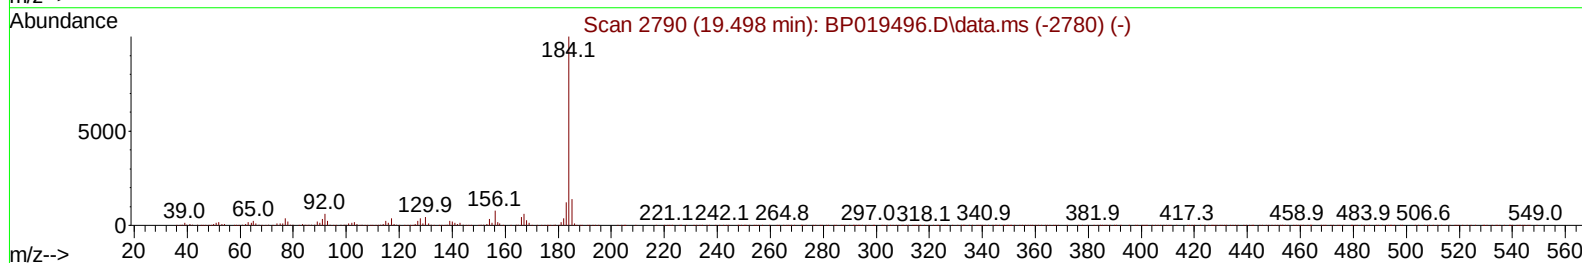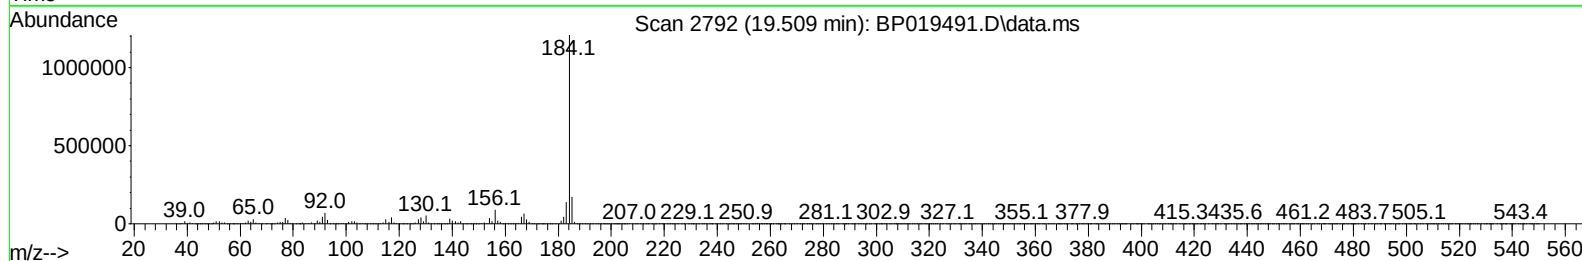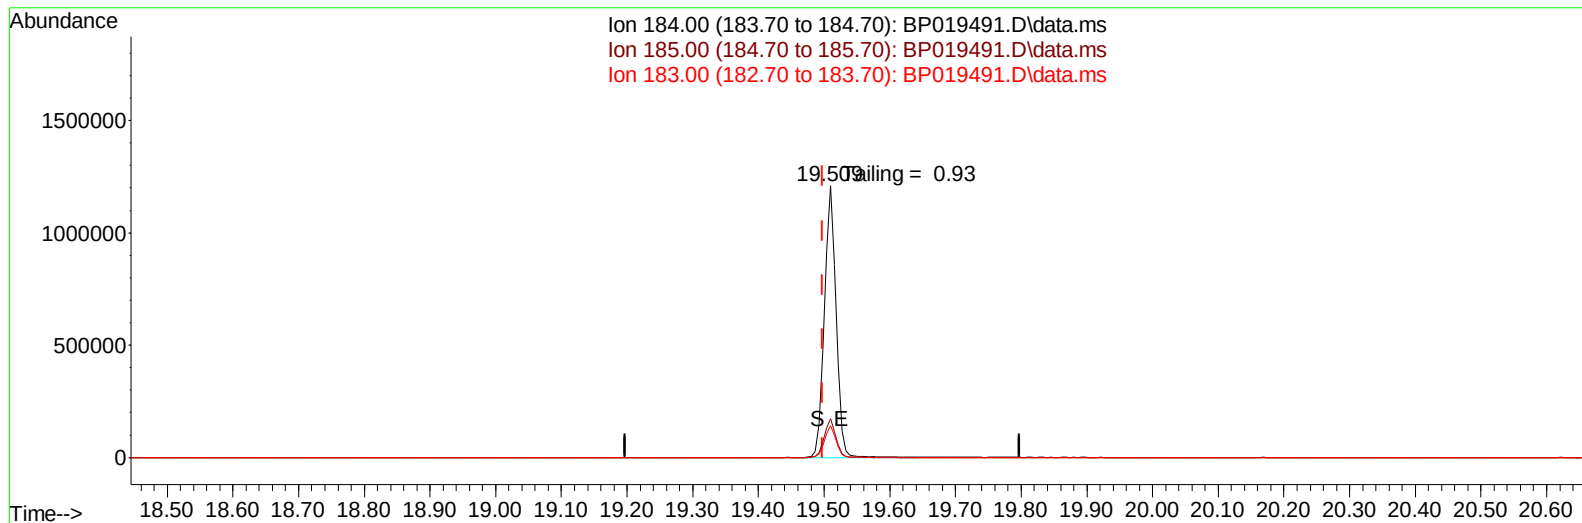

TIC: BP019491.D\data.ms

(77) Benzidine

19.509min (+ 0.012) 41749.72 ng

response 1508281

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.22
183.00	12.10	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2024	BNA_P	<u>BP019491.D</u>
Compound Name	Response	Retention Time
DDT	747332	20.709
DDD	14745	20.28
DDE	353	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15098	762430	1.98

Instrument :
BNA_P
ClientSampleId :
DFTPP