
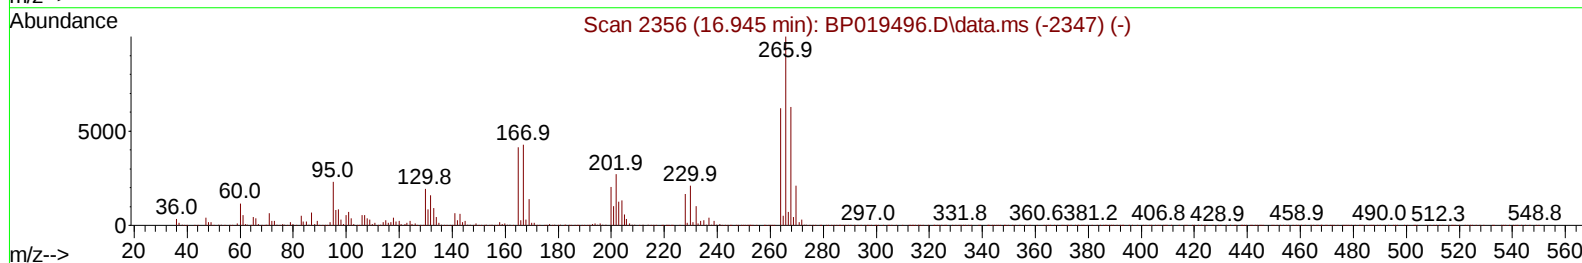
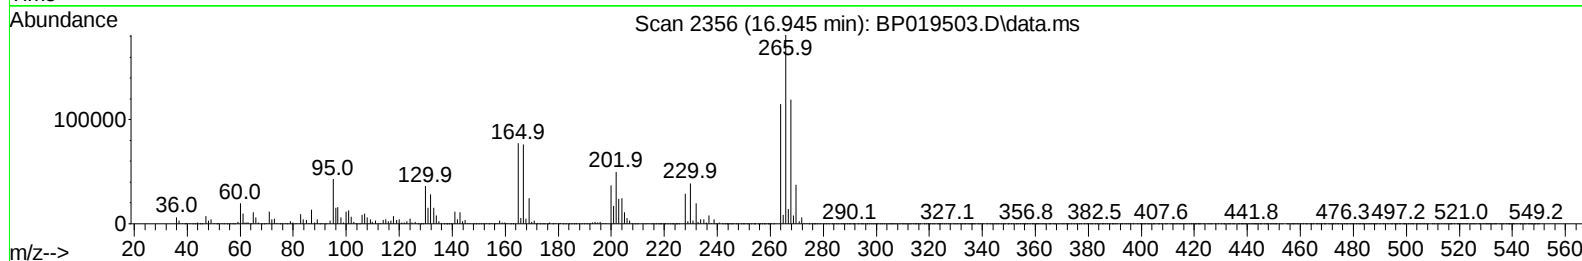


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020124\
Data File : BP019503.D
Acq On : 01 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 08:12:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

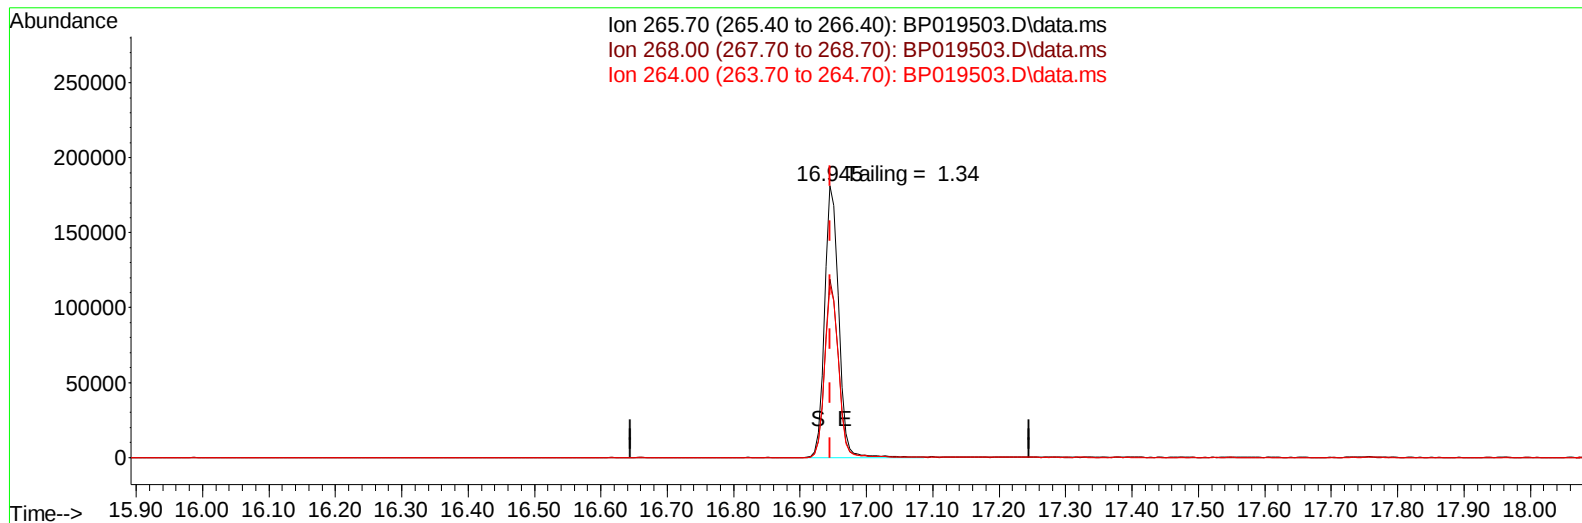

TIC: BP019503.D\data.ms

(70) Pentachlorophenol (C)




16.945min (+ 0.000) 72731.46 ng

response 263825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.63
264.00	62.10	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020124\
Data File : BP019503.D
Acq On : 01 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 08:12:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

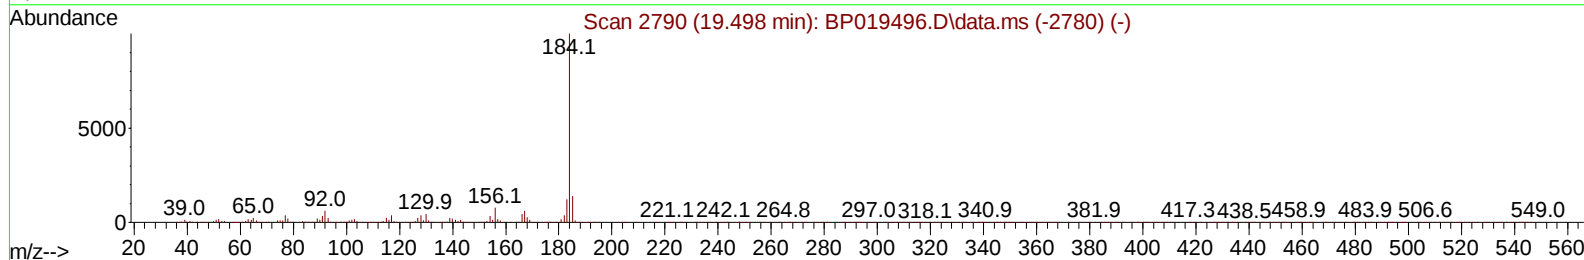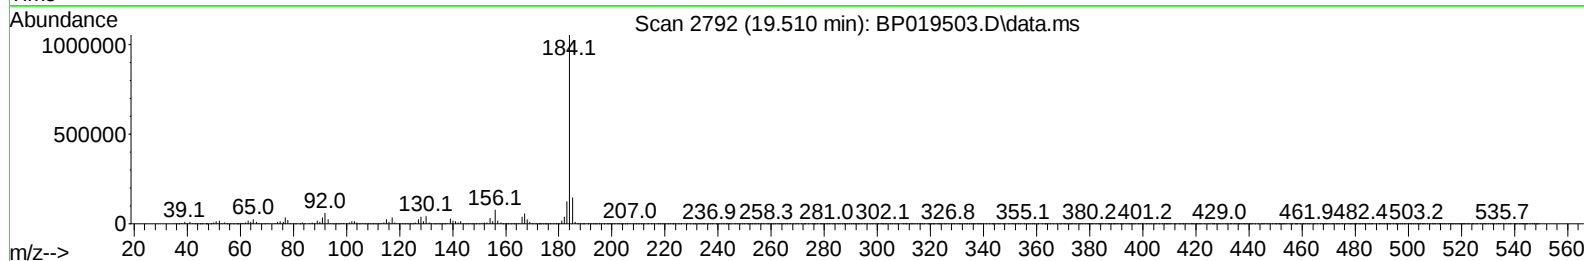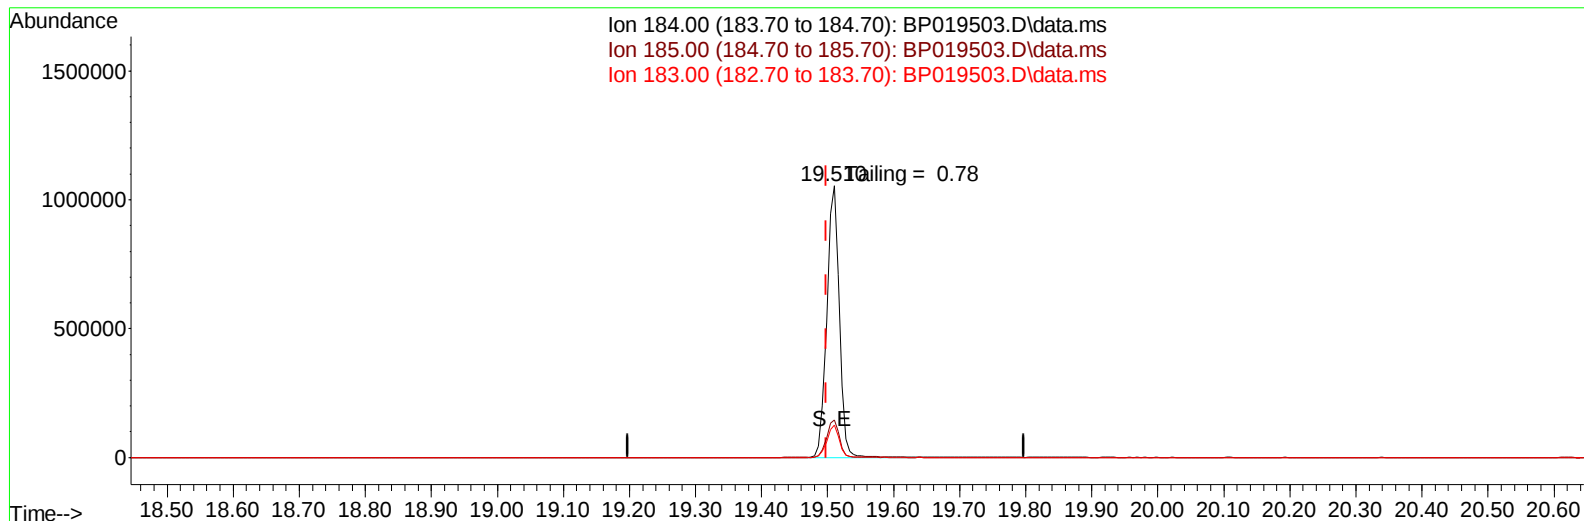

TIC: BP019503.D\data.ms

(77) Benzidine**19.510min (+ 0.012) 5657.20 ng****response 1383798**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.84
183.00	12.10	11.91
0.00	0.00	0.00