
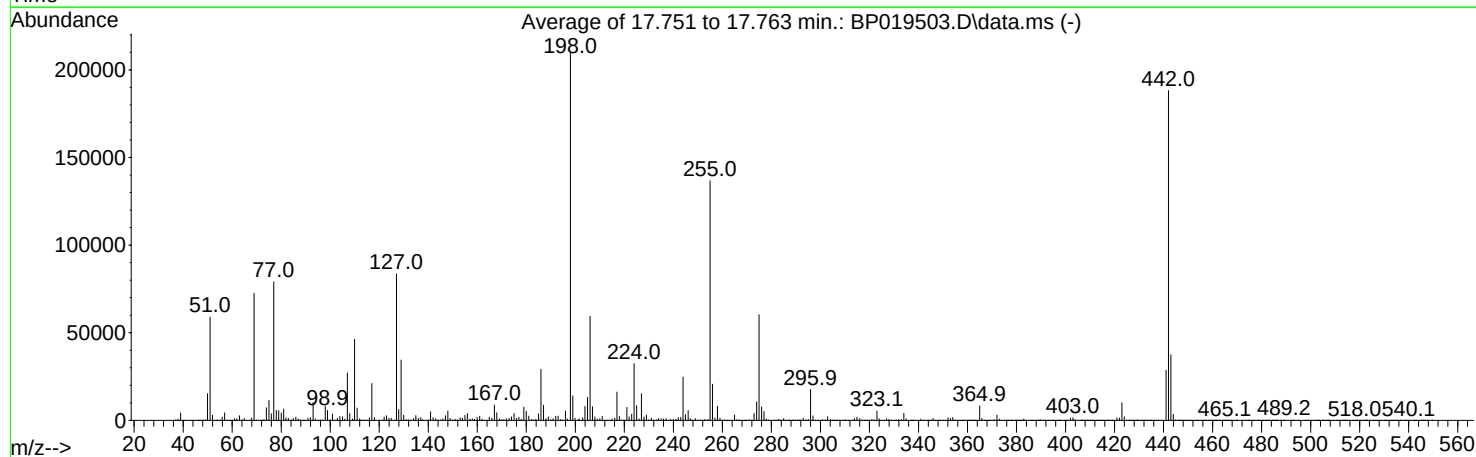


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020124\
Data File : BP019503.D
Acq On : 01 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

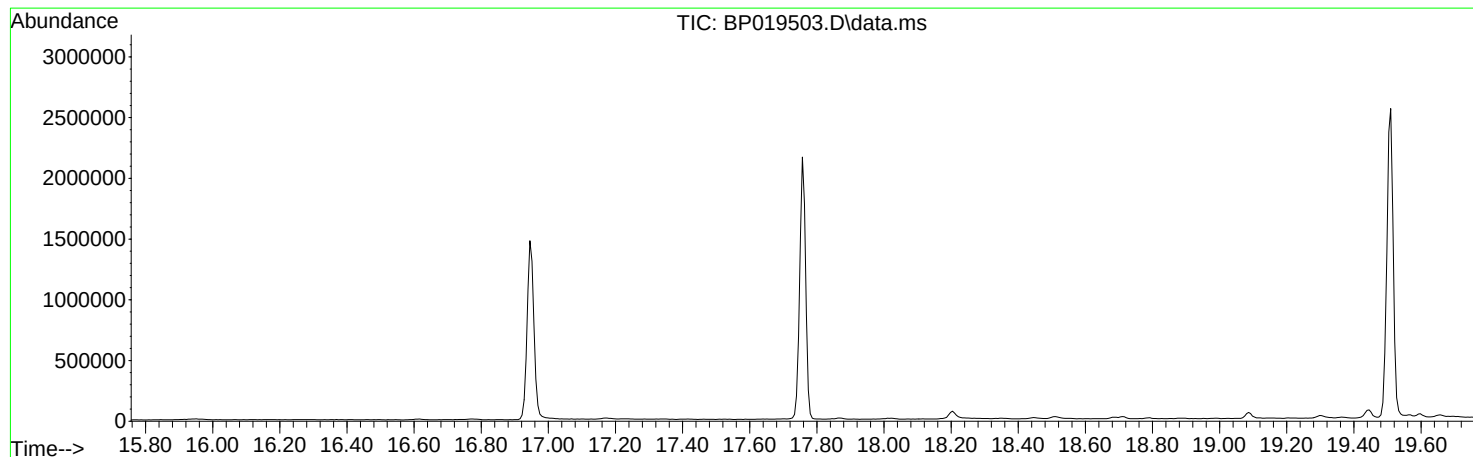




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	28.1	58979	PASS
68	69	0.00	2	1.7	1262	PASS
69	198	0.00	100	34.5	72499	PASS
70	69	0.00	2	0.3	236	PASS
127	198	10	80	39.8	83591	PASS
197	198	0.00	2	0.4	787	PASS
198	198	100	100	100.0	209941	PASS
199	198	5	9	6.7	13994	PASS
275	198	10	60	28.7	60283	PASS
365	198	1	100	3.9	8178	PASS
441	198	0.01	100	13.6	28573	PASS
442	442	100	100	100.0	188171	PASS
443	442	15	24	19.9	37474	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020124\
Data File : BP019503.D
Acq On : 01 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 02 08:12:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

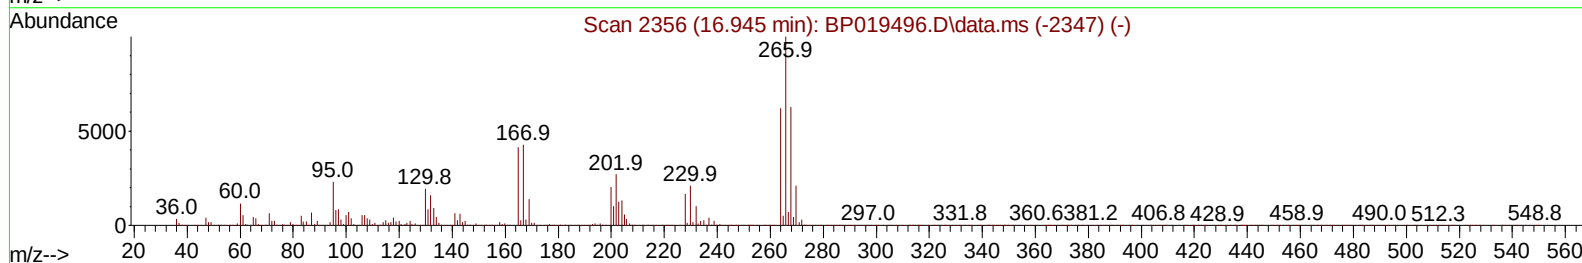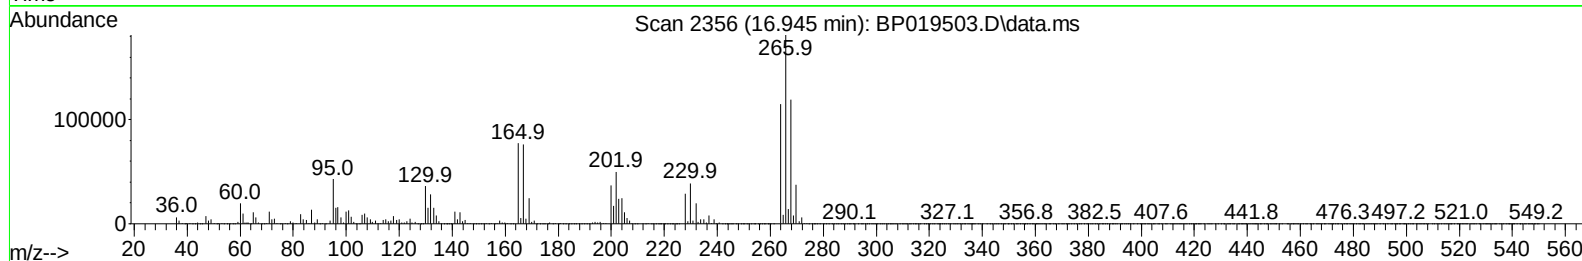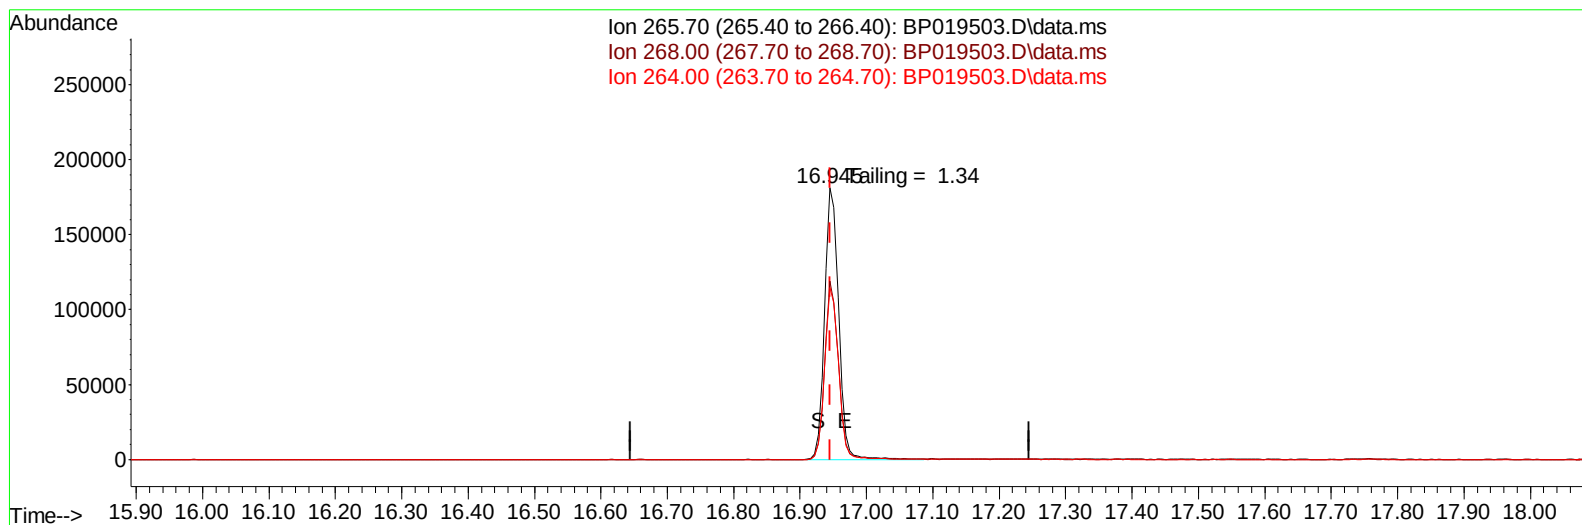

TIC: BP019503.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 72731.46 ng




response 263825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.63
264.00	62.10	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020124\
Data File : BP019503.D
Acq On : 01 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 02 08:12:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

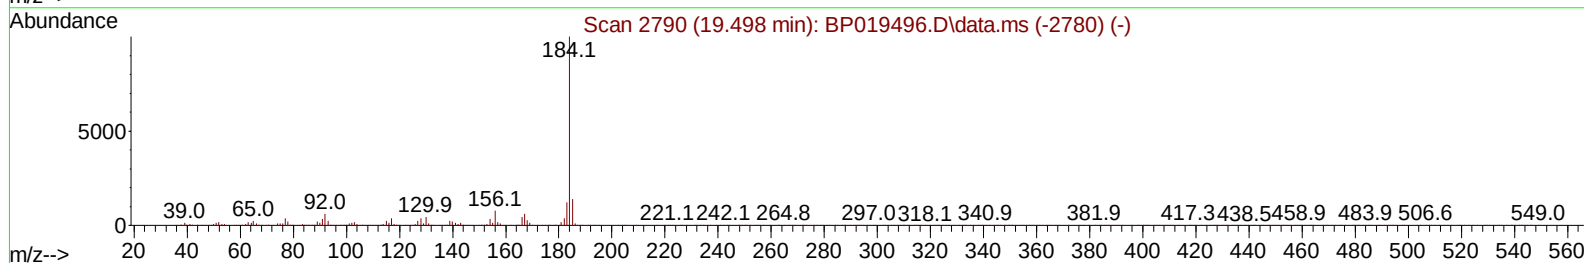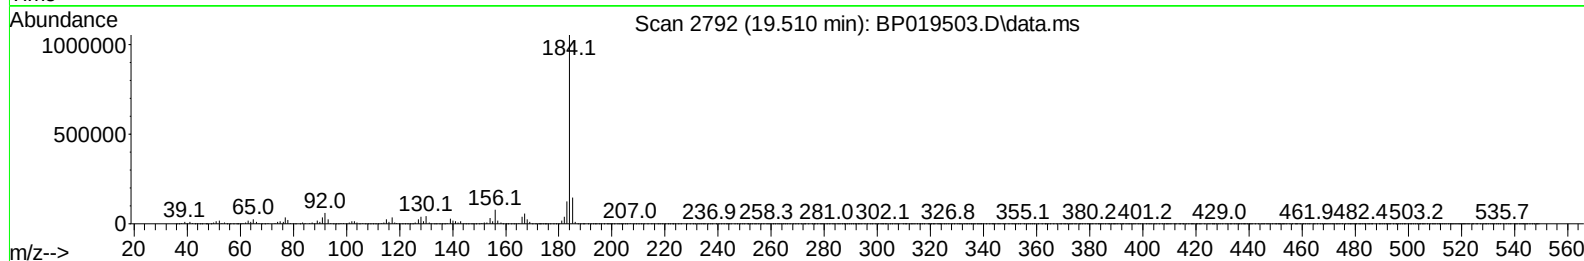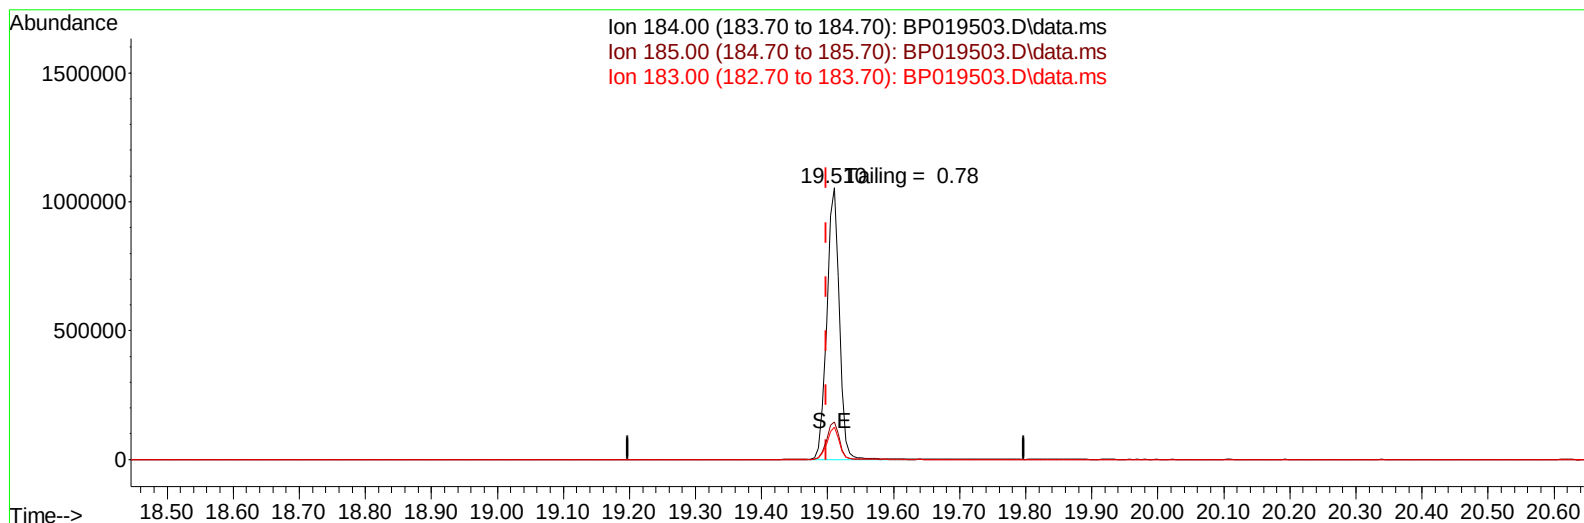

TIC: BP019503.D\data.ms

(77) Benzidine

19.510min (+ 0.012) 5657.20 ng

response 1383798

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.84
183.00	12.10	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2024	BNA_P	<u>BP019503.D</u>
Compound Name	Response	Retention Time
DDT	743291	20.71
DDD	16323	20.28
DDE	743	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17066	760357	2.24

Instrument :
BNA_P
ClientSampleId :
DFTPP