

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
 Data File : BP009016.D
 Acq On : 02 Feb 2022 20:31
 Operator : CG/JU
 Sample : N1357-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GROUNDWATER

Quant Time: Feb 03 06:26:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 03 06:20:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	207945	20.000	ng	0.00
21) Naphthalene-d8	10.622	136	749387	20.000	ng	0.00
39) Acenaphthene-d10	14.469	164	456282	20.000	ng	0.00
64) Phenanthrene-d10	17.222	188	927819	20.000	ng	0.00
76) Chrysene-d12	21.310	240	1036179	20.000	ng	-0.01
86) Perylene-d12	23.715	264	1150073	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	733007	54.511	ng	0.01
7) Phenol-d6	7.022	99	553143	33.970	ng	0.01
23) Nitrobenzene-d5	8.987	82	1241702	94.071	ng	0.00
42) 2,4,6-Tribromophenol	15.969	330	861024	129.640	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	2913748	84.213	ng	0.00
79) Terphenyl-d14	19.780	244	4360182	71.028	ng	0.00
Target Compounds						Qvalue
6) Aniline	7.152	93	969899	47.722	ng	96
9) Benzaldehyde	6.969	77	33779	3.104	ng	# 1
10) Phenol	7.046	94	1819208	109.586	ng	96
11) bis(2-Chloroethyl)ether	7.152	93	969899	73.432	ng	# 30
14) 1,2-Dichlorobenzene	8.175	146	77348	4.693	ng	99
15) Benzyl Alcohol	8.093	79	122608	10.733	ng	94
17) 2-Methylphenol	8.293	107	1074498	96.614	ng	97
18) Hexachloroethane	8.928	117	27755	4.731	ng	# 1
20) 3+4-Methylphenols	8.640	107	264341	17.904	ng	# 82
22) Acetophenone	8.657	105	220436	11.547	ng	# 82
27) 2,4-Dimethylphenol	9.851	122	621406	51.995	ng	95
30) 1,2,4-Trichlorobenzene	10.487	180	30901	2.023	ng	97
31) Naphthalene	10.675	128	2349130	57.715	ng	100
32) Benzoic acid	9.904	122	223924	32.648	ng	# 16
33) 4-Chloroaniline	10.957	127	22646011	1365.332	ng	94
35) Caprolactam	11.622	113	86997	24.198	ng	# 1
37) 2-Methylnaphthalene	12.304	142	93488	3.142	ng	# 80
38) 1-Methylnaphthalene	12.528	142	186200	6.818	ng	# 97
46) 1,1'-Biphenyl	13.304	154	91867	2.475	ng	97
60) Diethylphthalate	15.298	149	547932	17.041	ng	96
66) n-Nitrosodiphenylamine	15.728	169	130273	4.363	ng	99
71) Phenanthrene	17.357	178	125028	2.393	ng	99
72) Anthracene	17.357	178	125028	2.386	ng	97
74) Di-n-butylphthalate	18.180	149	140756	2.596	ng	# 98
80) Butylbenzylphthalate	20.457	149	1116616	38.401	ng	98
84) Bis(2-ethylhexyl)phtha...	21.221	149	123683	2.747	ng	95
85) Di-n-octyl phthalate	22.204	149	642902	8.440	ng	# 49

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009016.D
Acq On : 02 Feb 2022 20:31
Operator : CG/JU
Sample : N1357-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GROUNDWATER

Quant Time: Feb 03 06:26:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 03 06:20:22 2022
Response via : Initial Calibration




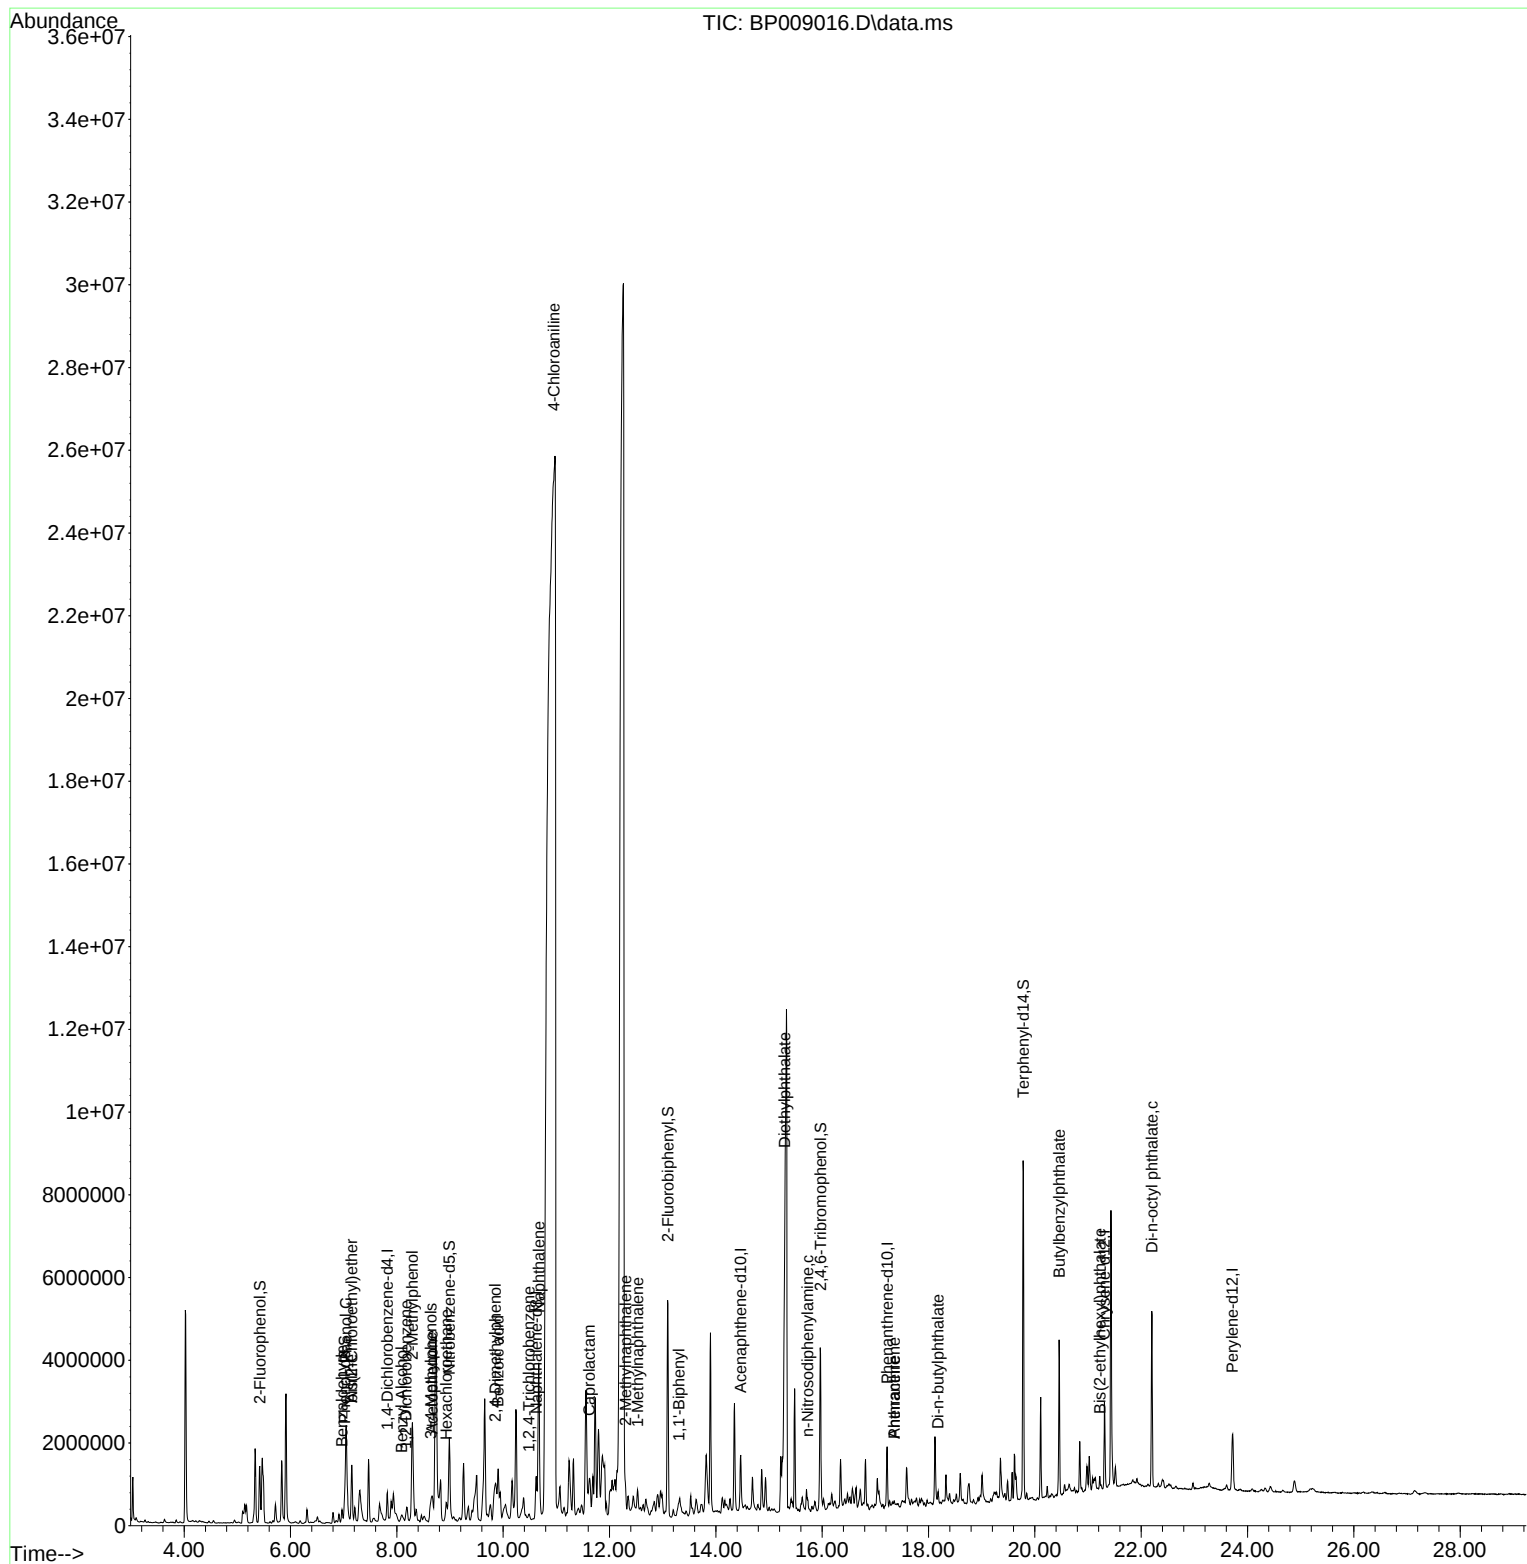




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.822 min Scan# 81
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:152 Resp: 207945
Ion Ratio Lower Upper
152 100
150 157.9 127.0 190.6
115 56.4 43.7 65.5



#5
2-Fluorophenol
Concen: 54.511 ng
RT: 5.422 min Scan# 414
Delta R.T. 0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:112 Resp: 733007
Ion Ratio Lower Upper
112 100
64 52.6 39.7 59.5
63 27.8 20.0 30.0









#6
Aniline
Concen: 47.722 ng
RT: 7.152 min Scan# 70
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion: 93 Resp: 969899
Ion Ratio Lower Upper
93 100
66 36.8 27.8 41.6
65 18.9 14.0 21.0

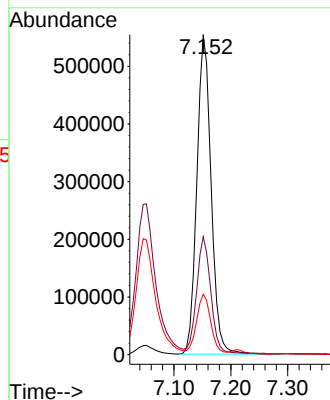

#7
Phenol-d6
Concen: 33.970 ng
RT: 7.022 min Scan# 686
Delta R.T. 0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion: 99 Resp: 553143
Ion Ratio Lower Upper
99 100
42 16.8 10.8 16.2#
71 32.6 23.8 35.6



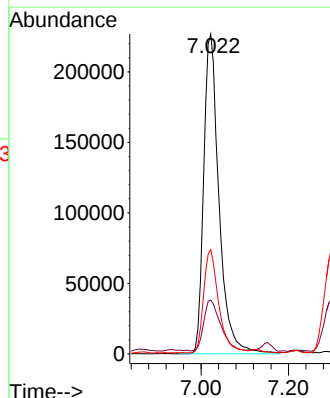





#9
Benzaldehyde
Concen: 3.104 ng
RT: 6.969 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion: 77 Resp: 33779
Ion Ratio Lower Upper
77 100
105 496.5 84.2 124.2#
106 83.6 80.6 120.6



#10
Phenol
Concen: 109.586 ng
RT: 7.046 min Scan# 690
Delta R.T. 0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion: 94 Resp: 1819208
Ion Ratio Lower Upper
94 100
65 26.3 4.1 44.1
66 34.0 12.4 52.4









#11
bis(2-Chloroethyl)ether
Concen: 73.432 ng
RT: 7.152 min Scan# 708
Delta R.T. -0.100 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion: 93 Resp: 969899
Ion Ratio Lower Upper
93 100
63 5.1 46.0 86.0#
95 0.3 12.2 52.2#

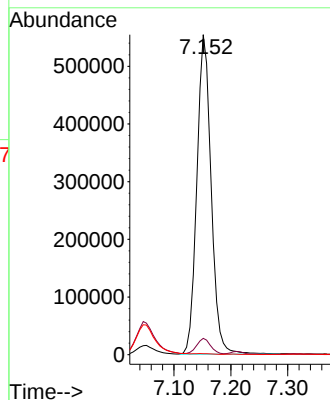

#14
1,2-Dichlorobenzene
Concen: 4.693 ng
RT: 8.175 min Scan# 882
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:146 Resp: 77348
Ion Ratio Lower Upper
146 100
148 64.8 52.2 78.2
111 40.4 31.1 46.7



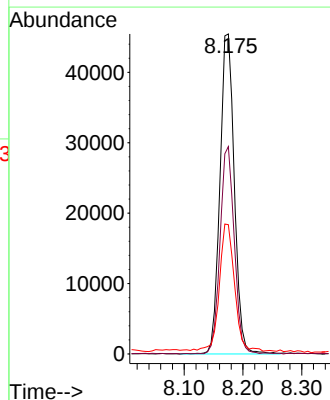





#15
Benzyl Alcohol
Concen: 10.733 ng
RT: 8.093 min Scan# 80
Delta R.T. 0.018 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion: 79 Resp: 122608
Ion Ratio Lower Upper
79 100
108 77.9 67.8 101.8
77 65.9 50.7 76.1



#17
2-Methylphenol
Concen: 96.614 ng
RT: 8.293 min Scan# 902
Delta R.T. 0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:107 Resp: 1074498
Ion Ratio Lower Upper
107 100
108 113.2 90.0 135.0
77 46.1 32.7 49.1
79 43.8 32.1 48.1







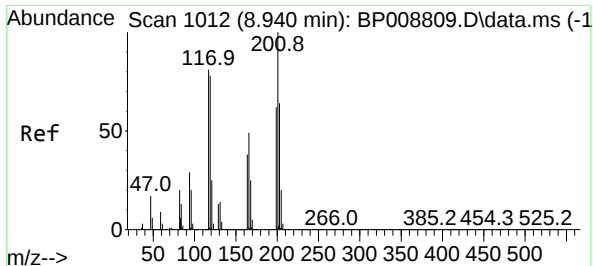

#18
Hexachloroethane
Concen: 4.731 ng
RT: 8.928 min Scan# 1012
Delta R.T. 0.029 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:117 Resp: 27755
Ion Ratio Lower Upper
117 100
119 444.9 76.9 115.3#
201 0.1 93.7 140.5#

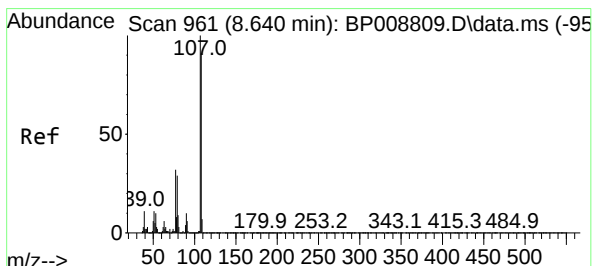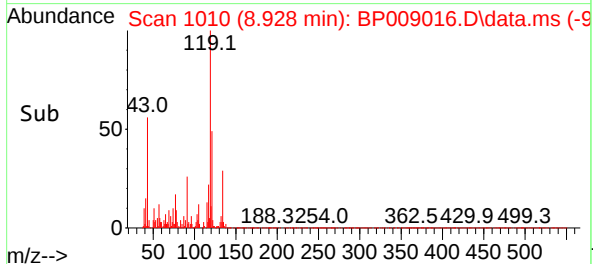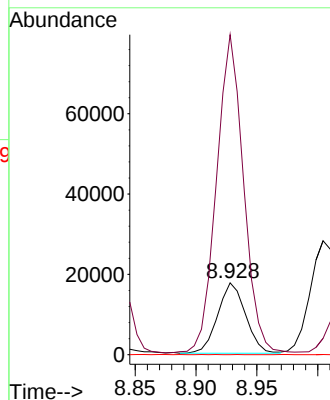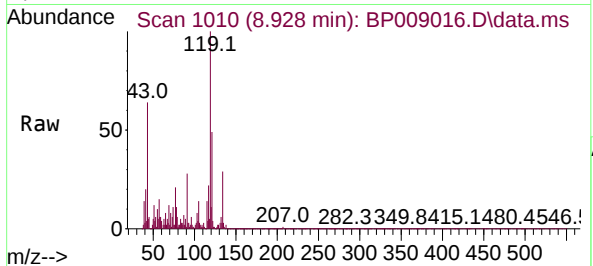

#20
3+4-Methylphenols
Concen: 17.904 ng
RT: 8.640 min Scan# 961
Delta R.T. 0.024 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:107 Resp: 264341
Ion Ratio Lower Upper
107 100
108 84.3 69.8 109.8
77 65.8 10.4 50.4#
79 29.4 6.4 46.4


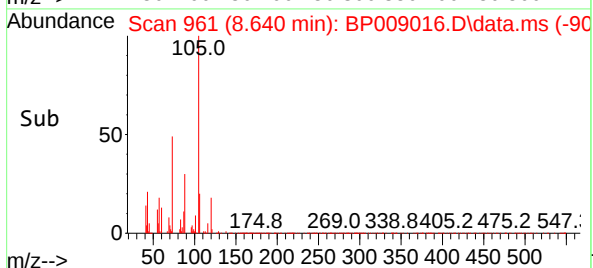
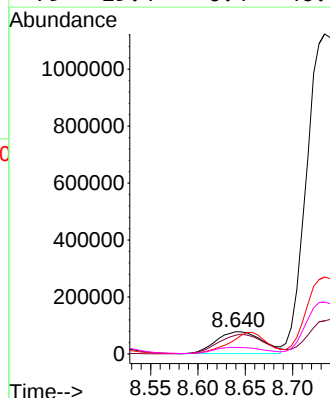
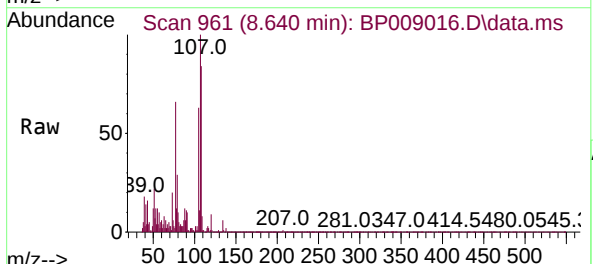




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.622 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:	136	Resp:	749387
Ion Ratio	Lower	Upper	
136	100		
137	11.0	9.0	13.4
54	6.3	4.9	7.3
68	5.1	4.3	6.5

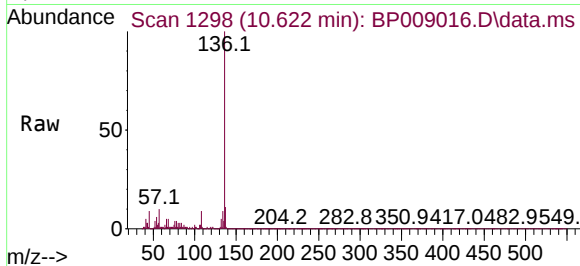

#22
Acetophenone
Concen: 11.547 ng
RT: 8.657 min Scan# 964
Delta R.T. 0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:	105	Resp:	220436
Ion Ratio	Lower	Upper	
105	100		
71	2.5	5.3	7.9#
51	37.0	16.3	24.5#
120	21.7	19.2	28.8




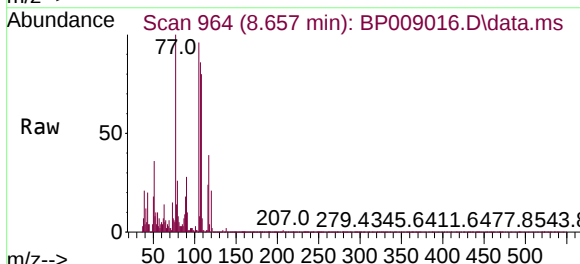




#23
Nitrobenzene-d5
Concen: 94.071 ng
RT: 8.987 min Scan# 1020
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion: 82 Resp: 1241702
Ion Ratio Lower Upper
82 100
128 45.7 39.4 59.2
54 43.0 32.6 48.8



#27
2,4-Dimethylphenol
Concen: 51.995 ng
RT: 9.851 min Scan# 1167
Delta R.T. 0.041 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:122 Resp: 621406
Ion Ratio Lower Upper
122 100
107 109.4 89.6 134.4
121 52.2 47.8 71.8









#30
1,2,4-Trichlorobenzene
Concen: 2.023 ng
RT: 10.487 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:180 Resp: 30901
Ion Ratio Lower Upper
180 100
182 97.6 76.7 115.1
145 30.9 22.4 33.6



#31
Naphthalene
Concen: 57.715 ng
RT: 10.675 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:128 Resp: 2349130
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 13.0 10.4 15.6









#32
Benzoic acid
Concen: 32.648 ng
RT: 9.904 min Scan# 1176
Delta R.T. -0.106 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:122 Resp: 223924
Ion Ratio Lower Upper
122 100
105 4.1 100.1 140.1#
77 35.1 65.5 105.5#



#33
4-Chloroaniline
Concen: 1365.332 ng
RT: 10.957 min Scan# 1355
Delta R.T. 0.165 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:127 Resp:22646011
Ion Ratio Lower Upper
127 100
129 36.4 26.0 39.0
65 22.3 20.5 30.7
92 19.5 14.1 21.1









#35
Caprolactam
Concen: 24.198 ng
RT: 11.622 min Scan# 1467
Delta R.T. 0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:113 Resp: 86997
Ion Ratio Lower Upper
113 100
55 352.5 107.1 147.1#
56 105.9 74.1 114.1

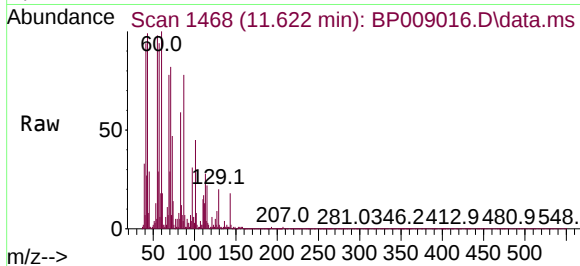

#37
2-Methylnaphthalene
Concen: 3.142 ng
RT: 12.304 min Scan# 1584
Delta R.T. 0.018 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:142 Resp: 93488
Ion Ratio Lower Upper
142 100
141 90.4 70.5 105.7
115 69.0 24.6 36.8#




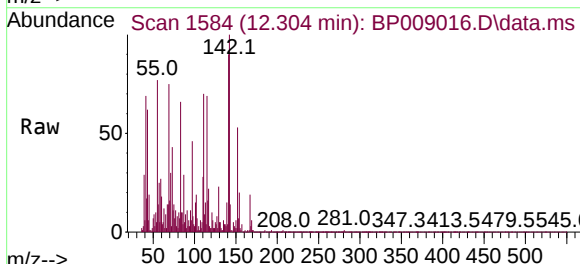




#38
1-Methylnaphthalene
Concen: 6.818 ng
RT: 12.528 min Scan# 1
Delta R.T. 0.018 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:142 Resp: 186200
Ion Ratio Lower Upper
142 100
141 88.4 73.2 109.8
116 4.9 2.7 4.1#



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.469 min Scan# 1952
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:164 Resp: 456282
Ion Ratio Lower Upper
164 100
162 96.8 79.9 119.9
160 45.1 35.5 53.3


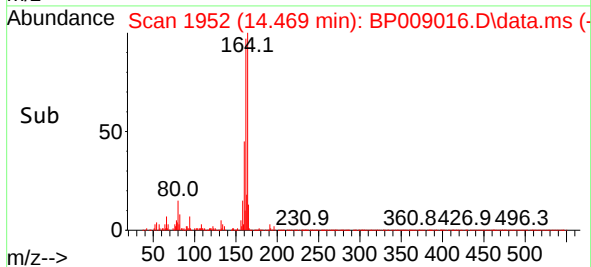

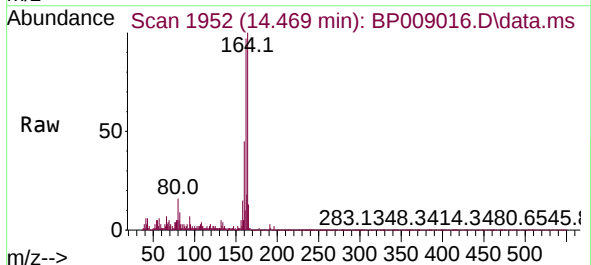




#42
2,4,6-Tribromophenol
Concen: 129.640 ng
RT: 15.969 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:330 Resp: 861024
Ion Ratio Lower Upper
330 100
332 96.5 77.0 115.4
141 28.3 21.3 31.9

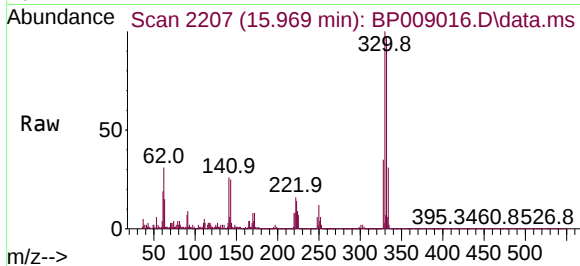

#45
2-Fluorobiphenyl
Concen: 84.213 ng
RT: 13.098 min Scan# 1719
Delta R.T. 0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:172 Resp: 2913748
Ion Ratio Lower Upper
172 100
171 34.9 29.3 43.9
170 23.5 19.5 29.3




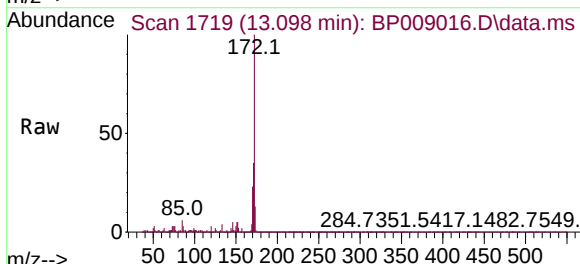




#46
1,1'-Biphenyl
Concen: 2.475 ng
RT: 13.304 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:154	Resp:	91867
Ion Ratio	Lower	Upper
154	100	
153	41.3	20.3 60.3
76	13.8	0.0 31.1



#60
Diethylphthalate
Concen: 17.041 ng
RT: 15.298 min Scan# 2093
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:149	Resp:	547932
Ion Ratio	Lower	Upper
149	100	
177	27.9	19.9 29.9
150	12.8	10.3 15.5









#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.222 min Scan# 2425
Delta R.T. -0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:188 Resp: 927819
Ion Ratio Lower Upper
188 100
94 7.7 6.8 10.2
80 8.3 7.2 10.8

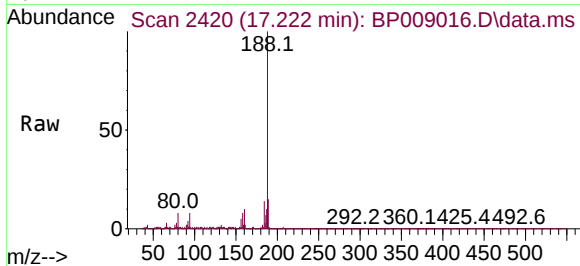

#66
n-Nitrosodiphenylamine
Concen: 4.363 ng
RT: 15.728 min Scan# 2166
Delta R.T. -0.006 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:169 Resp: 130273
Ion Ratio Lower Upper
169 100
168 67.6 53.3 79.9
167 36.4 29.0 43.6




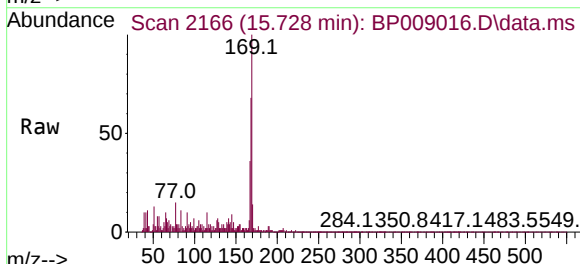




#71
Phenanthrene
Concen: 2.393 ng
RT: 17.357 min Scan# 2443
Delta R.T. 0.088 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:178 Resp: 125028
Ion Ratio Lower Upper
178 100
176 20.2 16.0 24.0
179 17.0 13.0 19.4



#72
Anthracene
Concen: 2.386 ng
RT: 17.357 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:178 Resp: 125028
Ion Ratio Lower Upper
178 100
176 20.2 15.1 22.7
179 17.0 12.8 19.2



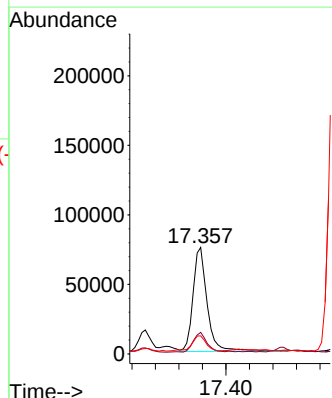





#74
Di-n-butylphthalate
Concen: 2.596 ng
RT: 18.180 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:149 Resp: 140756
Ion Ratio Lower Upper
149 100
150 9.5 7.9 11.9
104 5.8 3.7 5.5#



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.310 min Scan# 3115
Delta R.T. -0.012 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:240 Resp: 1036179
Ion Ratio Lower Upper
240 100
120 8.9 7.7 11.5
236 26.2 21.2 31.8


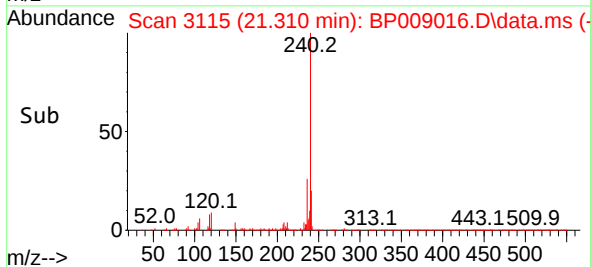

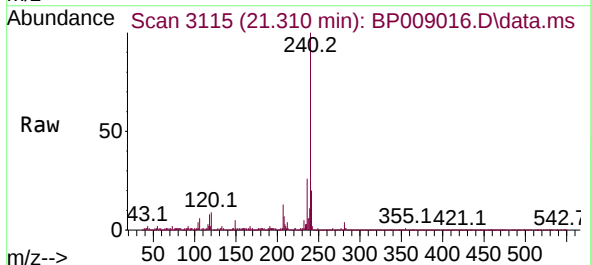




#79
 Terphenyl-d14
 Concen: 71.028 ng
 RT: 19.780 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP009016.D
 Acq: 02 Feb 2022 20:31




Instrument :
 BNA_P
 ClientSampleId :
 GROUNDWATER


Tgt Ion:244 Resp: 4360182
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.5 9.7
 122 8.6 9.2 13.8#

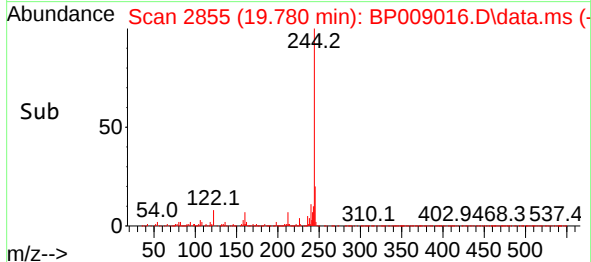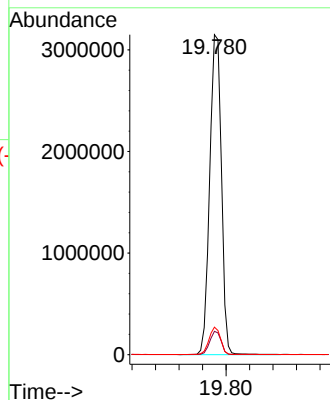

#80
 Butylbenzylphthalate
 Concen: 38.401 ng
 RT: 20.457 min Scan# 2970
 Delta R.T. -0.006 min
 Lab File: BP009016.D
 Acq: 02 Feb 2022 20:31

Tgt Ion:149 Resp: 1116616
 Ion Ratio Lower Upper
 149 100
 91 64.9 50.6 76.0
 206 23.6 19.7 29.5


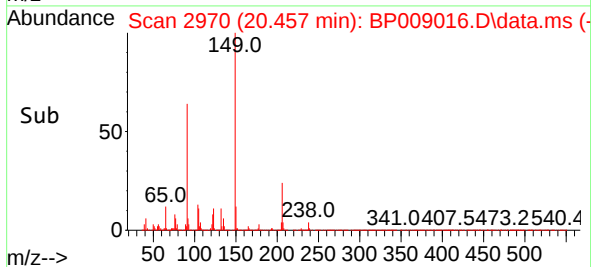
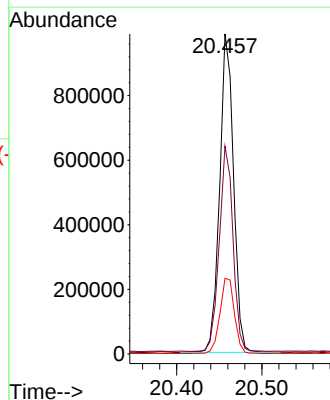
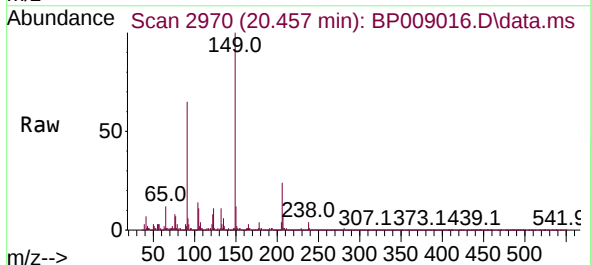




#84
Bis(2-ethylhexyl)phthalate
Concen: 2.747 ng
RT: 21.221 min Scan# 3100
Delta R.T. 0.000 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31




Instrument :
BNA_P
ClientSampleId :
GROUNDWATER


Tgt Ion:149 Resp: 123683
Ion Ratio Lower Upper
149 100
167 27.8 25.0 37.4
279 6.0 4.8 7.2

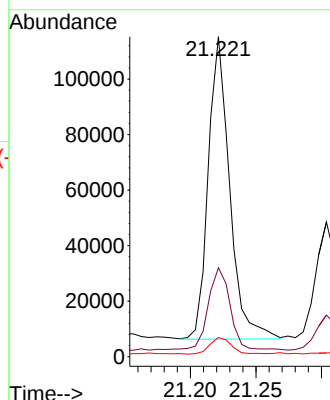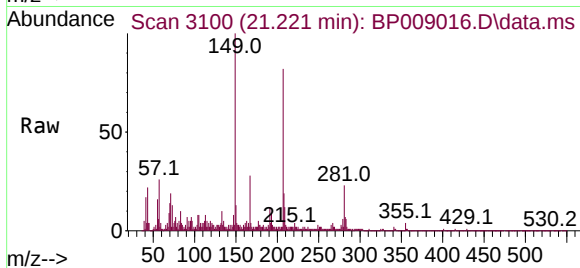

#85
Di-n-octyl phthalate
Concen: 8.440 ng
RT: 22.204 min Scan# 3267
Delta R.T. 0.059 min
Lab File: BP009016.D
Acq: 02 Feb 2022 20:31

Tgt Ion:149 Resp: 642902
Ion Ratio Lower Upper
149 100
167 52.6 1.4 2.0#
43 16.8 5.4 8.2#

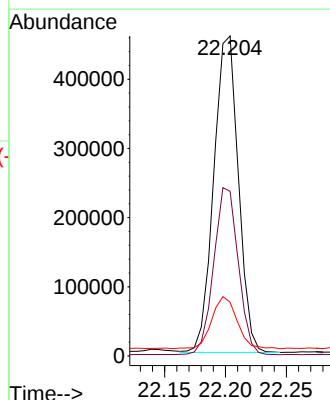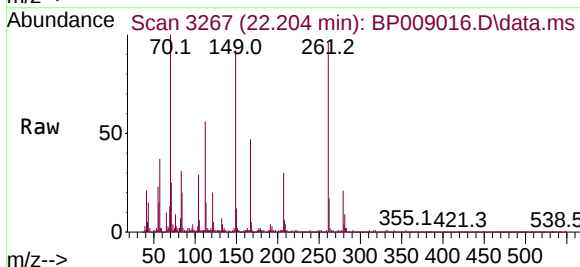



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.715 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP009016.D
 Acq: 02 Feb 2022 20:31

Instrument :
 BNA_P
 ClientSampleId :
 GROUNDWATER

Tgt Ion:264 Resp: 1150073
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.1 28.7
 265 22.1 17.1 25.7

