

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
 Data File : BP009001.D
 Acq On : 02 Feb 2022 11:21
 Operator : CG/JU
 Sample : PB142410BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142410BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	406	413	433	rBV	4026236	6325471	33.11%	8.466%
2	7.011	676	684	708	rBV	3564608	6450517	33.76%	8.634%
3	7.822	814	822	838	rBV	852951	1433836	7.50%	1.919%
4	8.987	1012	1020	1042	rBV	2479369	4417447	23.12%	5.913%
5	10.622	1291	1298	1325	rBV	1079477	2041471	10.68%	2.732%
6	13.087	1708	1717	1744	rBV	7161783	11823529	61.88%	15.825%
7	14.469	1944	1952	1978	rBV	1811084	3026122	15.84%	4.050%
8	15.963	2198	2206	2240	rBV	5629444	9537802	49.92%	12.766%
9	17.222	2413	2420	2435	rBV	2354803	3730581	19.53%	4.993%
10	19.786	2850	2856	2869	rBV	15406826	19106079	100.00%	25.572%
11	21.316	3111	3116	3128	rBV	2674046	3681068	19.27%	4.927%
12	23.727	3519	3526	3537	rVB2	1420699	3139650	16.43%	4.202%




Sum of corrected areas: 74713573

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009001.D
Acq On : 02 Feb 2022 11:21
Operator : CG/JU
Sample : PB142410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

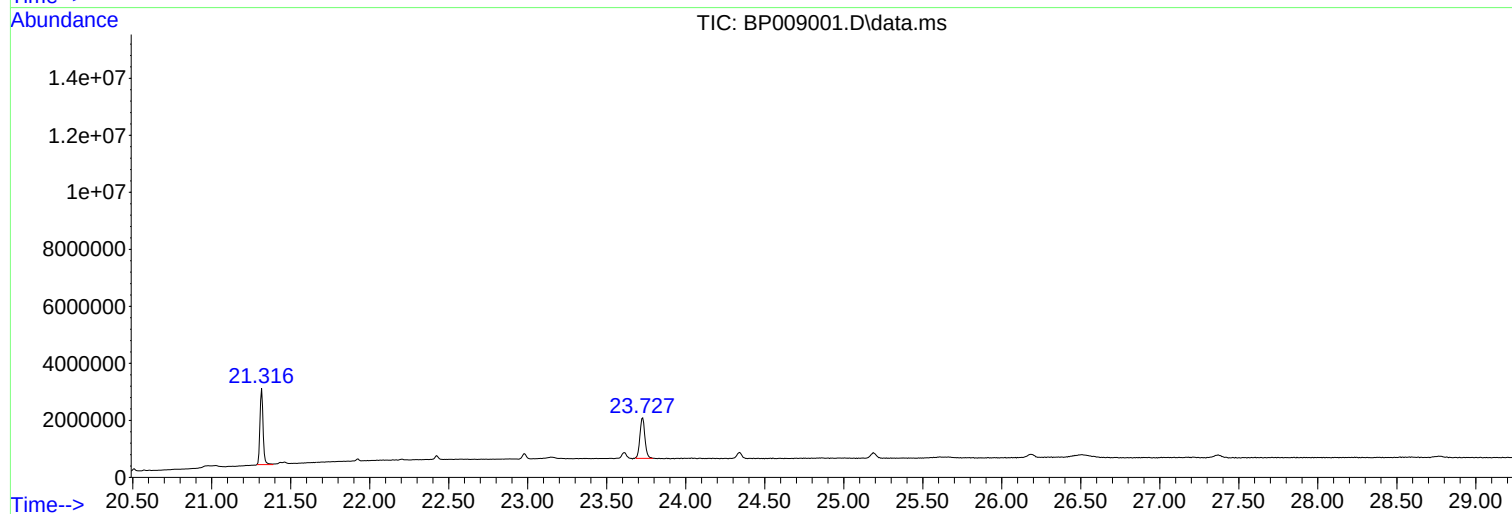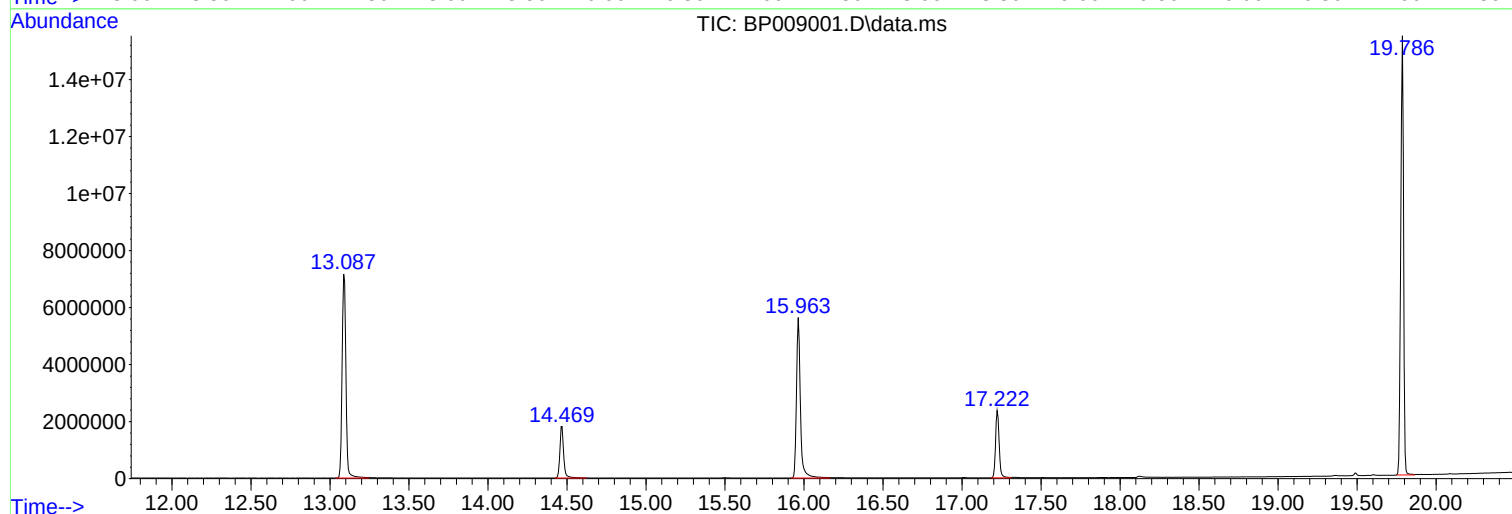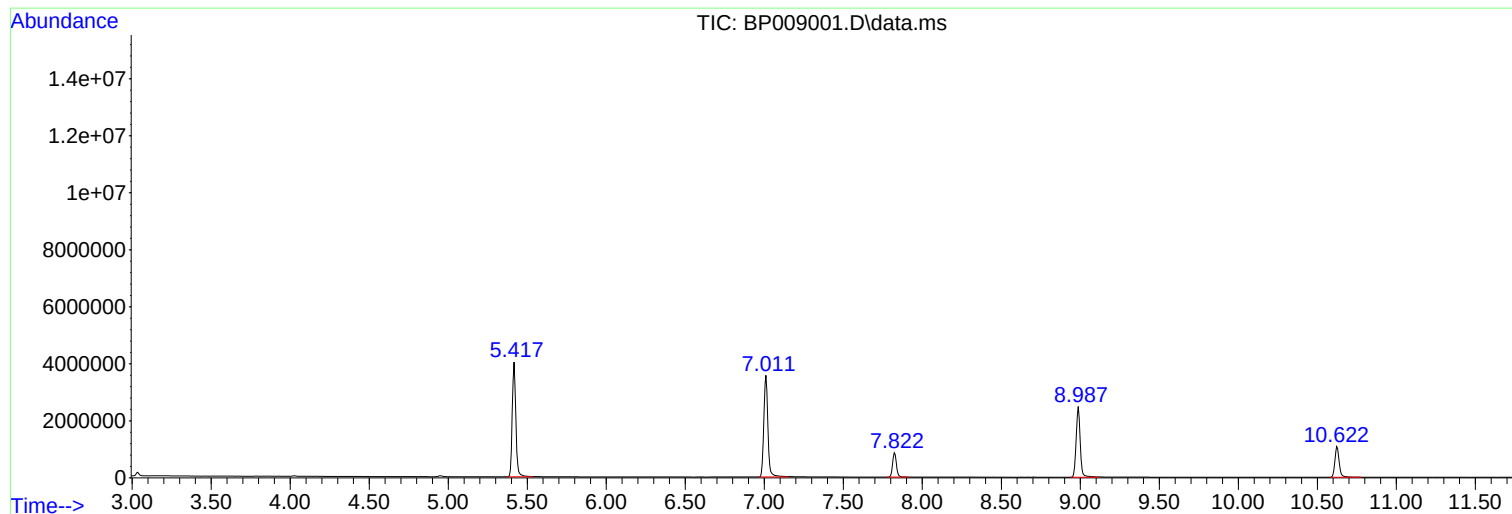

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009001.D
Acq On : 02 Feb 2022 11:21
Operator : CG/JU
Sample : PB142410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009001.D
Acq On : 02 Feb 2022 11:21
Operator : CG/JU
Sample : PB142410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142410BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------