

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009004.D
Acq On : 02 Feb 2022 13:48
Operator : CG/JU
Sample : PB142428BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142428BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	406	413	445	rBV	3737396	5976262	34.67%	8.732%
2	7.011	676	684	718	rBV	3282593	6049349	35.10%	8.839%
3	7.822	815	822	833	rBV	770061	1329500	7.71%	1.942%
4	8.987	1012	1020	1049	rBV	2263392	4145859	24.05%	6.057%
5	10.628	1291	1299	1319	rBV	962566	1901923	11.03%	2.779%
6	13.093	1709	1718	1742	rBV	6457842	10796713	62.64%	15.775%
7	14.469	1942	1952	1976	rBV	1574740	2713664	15.74%	3.965%
8	15.963	2199	2206	2236	rBV	4582784	8404783	48.76%	12.280%
9	17.228	2414	2421	2437	rBV	1906272	3315232	19.23%	4.844%
10	19.786	2850	2856	2869	rBV	14081253	17236954	100.00%	25.184%
11	21.316	3111	3116	3129	rBV	2419666	3540373	20.54%	5.173%
12	23.727	3519	3526	3537	rVB	1396060	3032515	17.59%	4.431%




Sum of corrected areas: 68443127

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009004.D
Acq On : 02 Feb 2022 13:48
Operator : CG/JU
Sample : PB142428BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142428BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

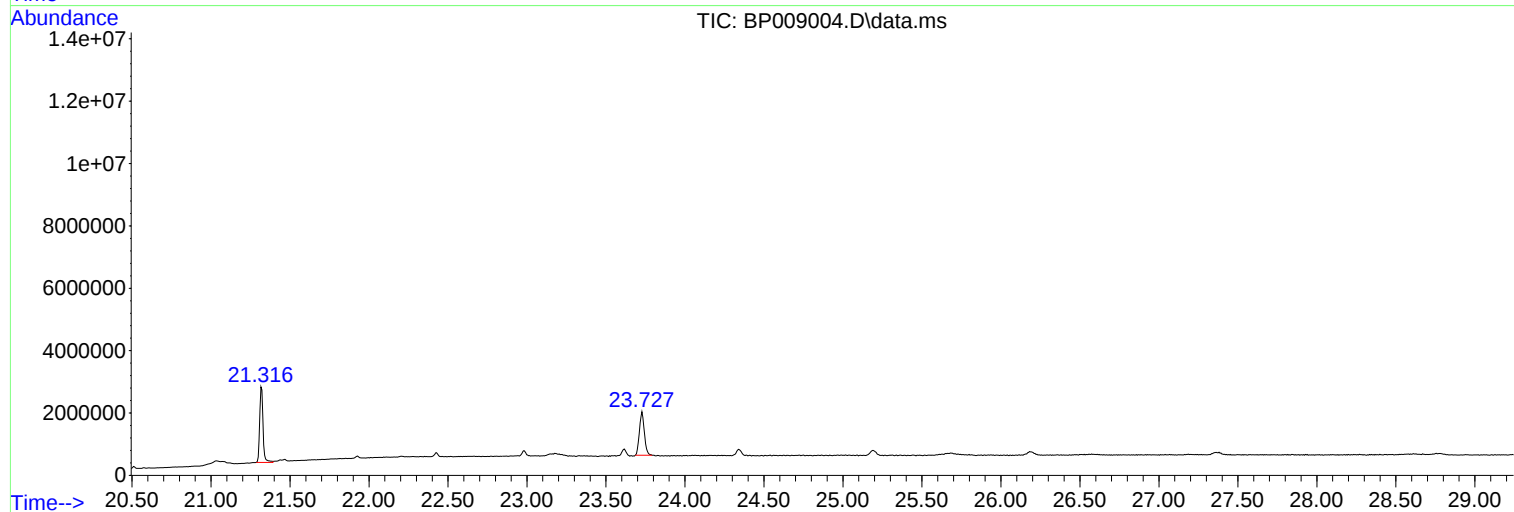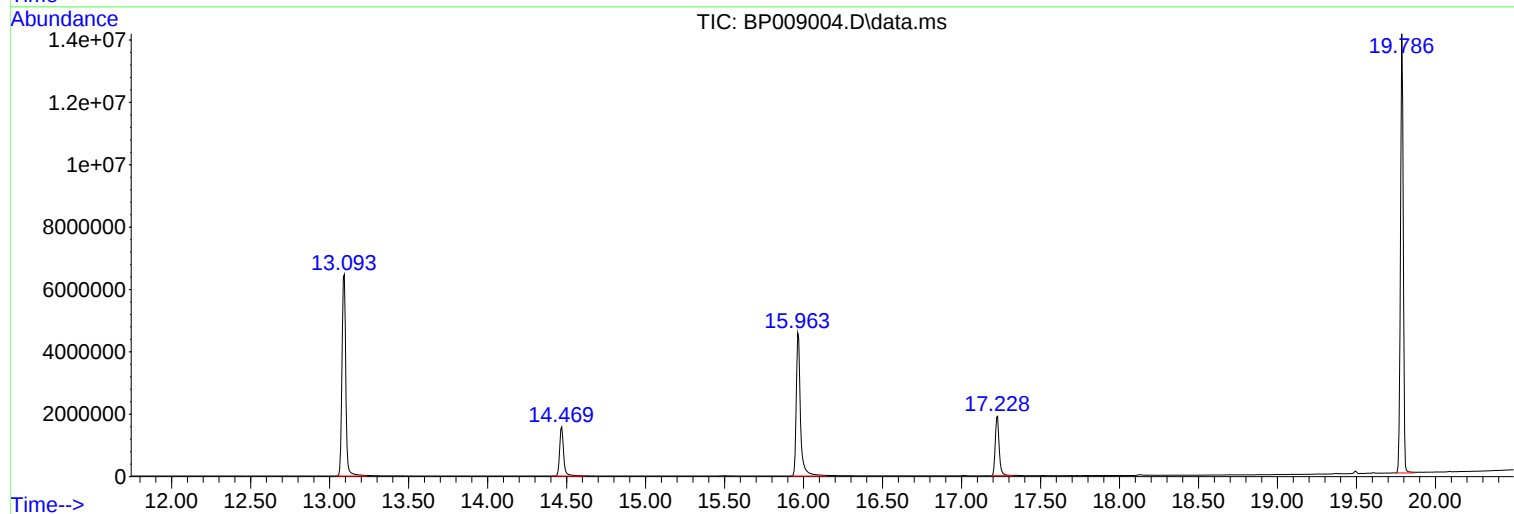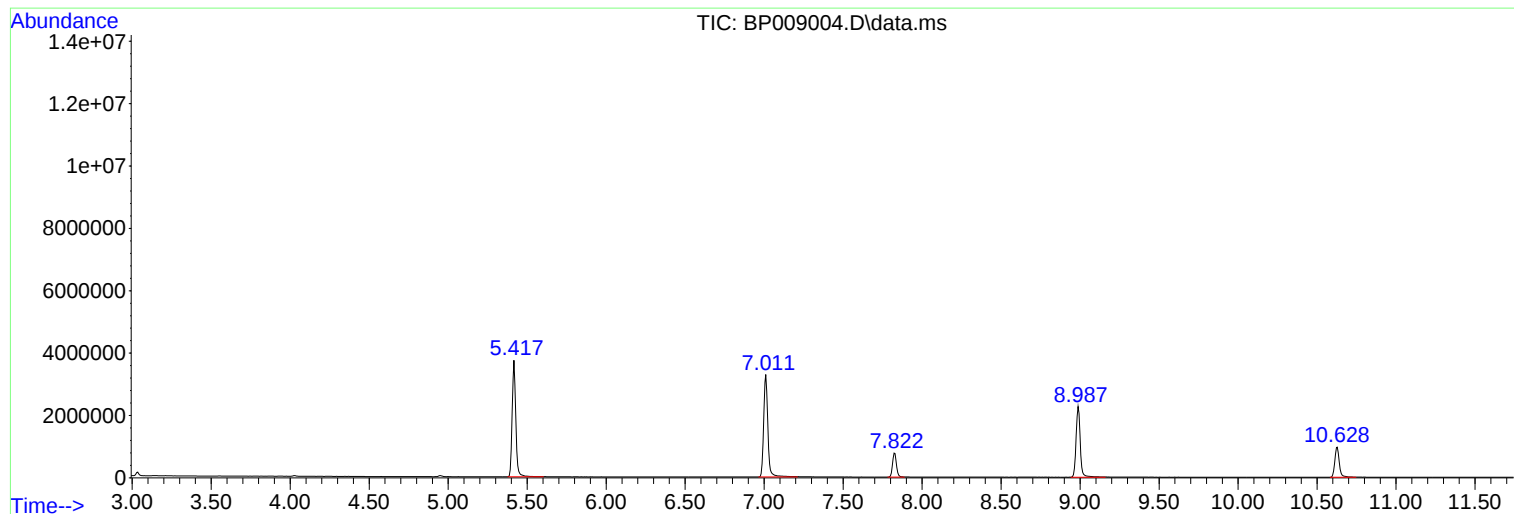

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009004.D
Acq On : 02 Feb 2022 13:48
Operator : CG/JU
Sample : PB142428BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142428BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP009004.D
Acq On : 02 Feb 2022 13:48
Operator : CG/JU
Sample : PB142428BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142428BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------