
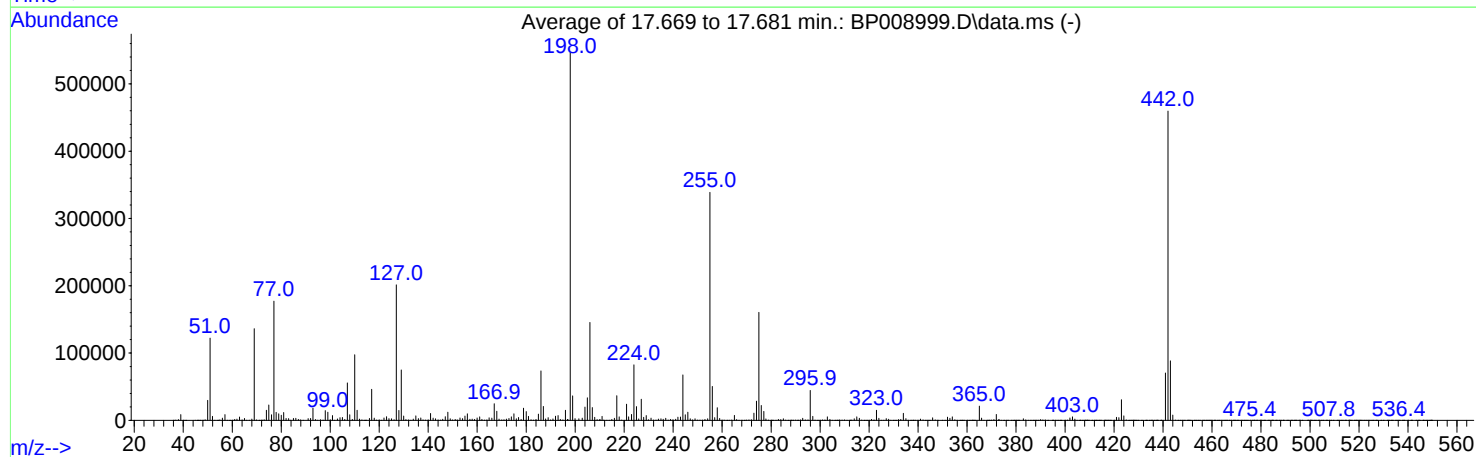


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
 Data File : BP008999.D
 Acq On : 02 Feb 2022 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 03 06:20:22 2022

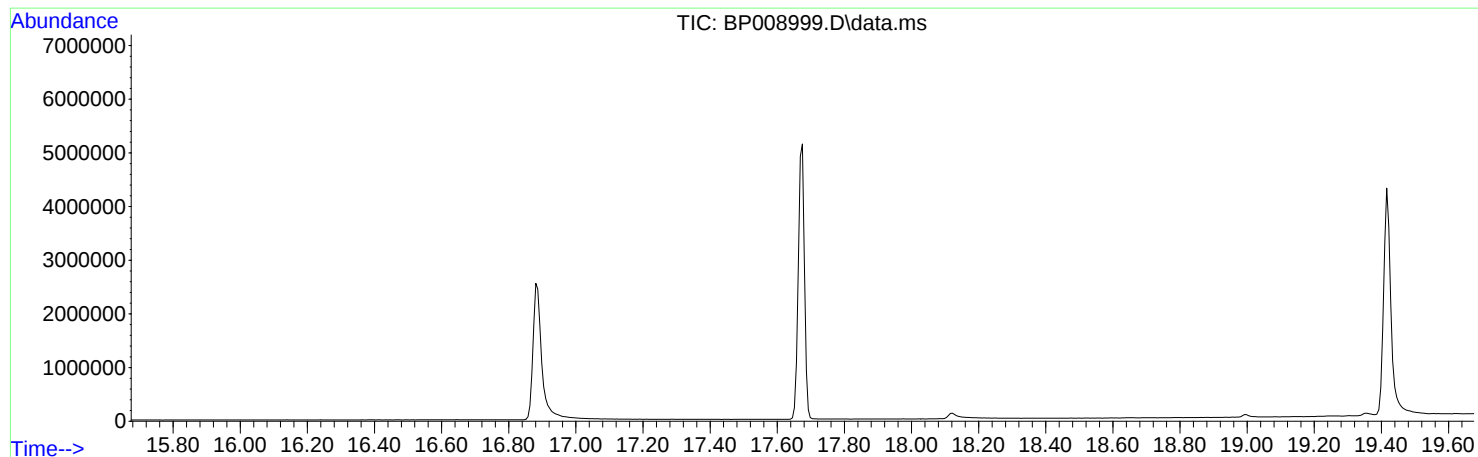




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	122360	PASS
68	69	0.00	2	1.5	1979	PASS
69	198	0.00	100	24.9	136199	PASS
70	69	0.00	2	0.6	835	PASS
127	198	10	80	36.8	201316	PASS
197	198	0.00	2	0.3	1526	PASS
198	198	100	100	100.0	546661	PASS
199	198	5	9	6.7	36358	PASS
275	198	10	60	29.4	160462	PASS
365	198	1	100	3.9	21160	PASS
441	198	0.01	100	12.9	70515	PASS
442	442	100	100	100.0	459627	PASS
443	442	15	24	19.2	88409	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP008999.D
Acq On : 02 Feb 2022 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 03 08:44:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 03 06:20:22 2022
Response via : Initial Calibration

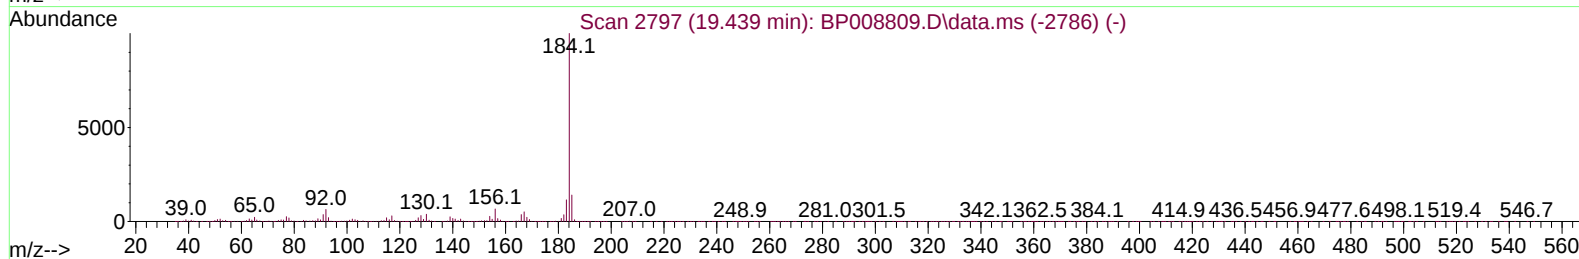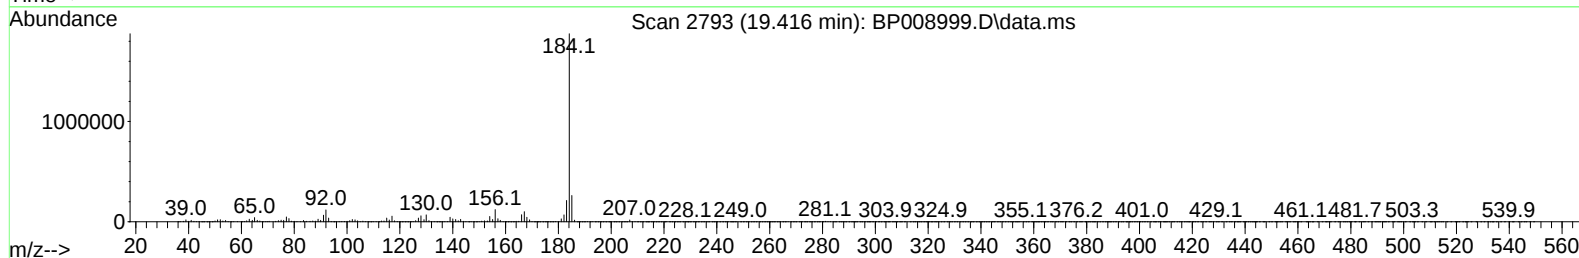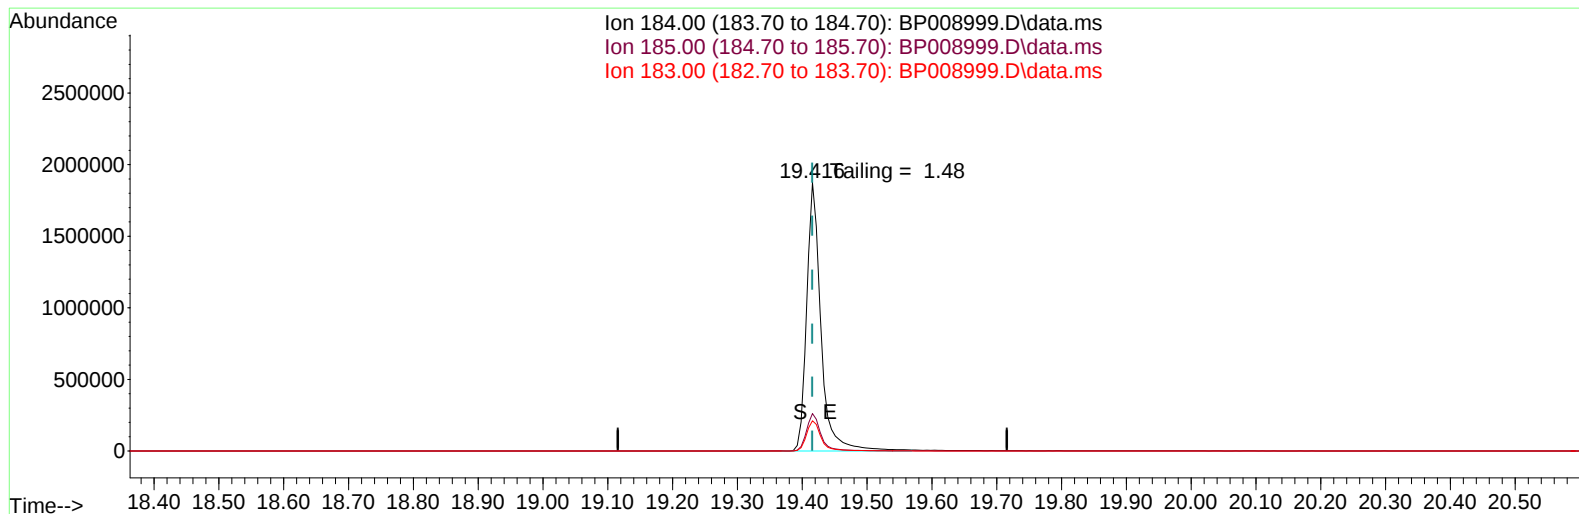

TIC: BP008999.D\data.ms

(77) Benzidine

19.416min (+ 0.000) 43285.86 ng




response 2879472

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.94
183.00	11.90	11.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020222\
Data File : BP008999.D
Acq On : 02 Feb 2022 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 03 08:44:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 03 06:20:22 2022
Response via : Initial Calibration

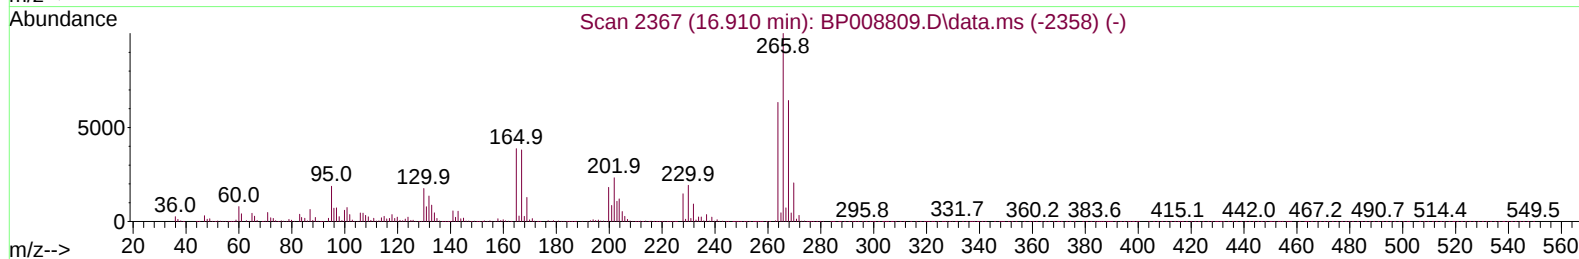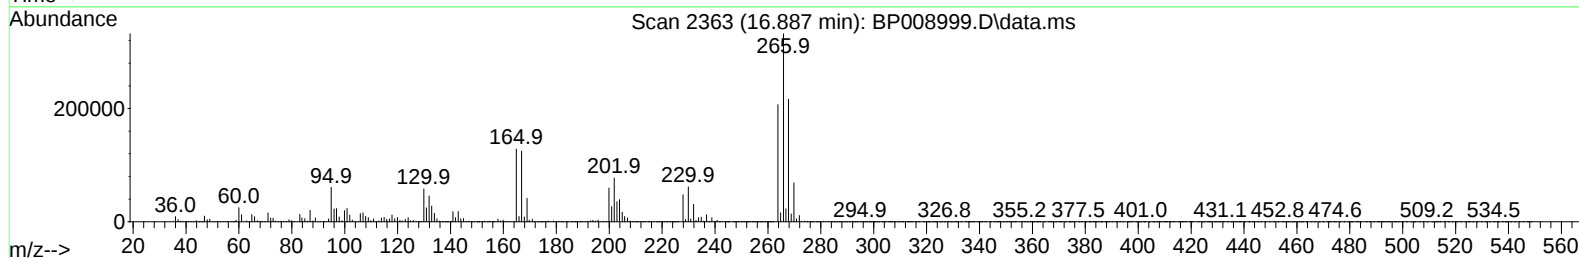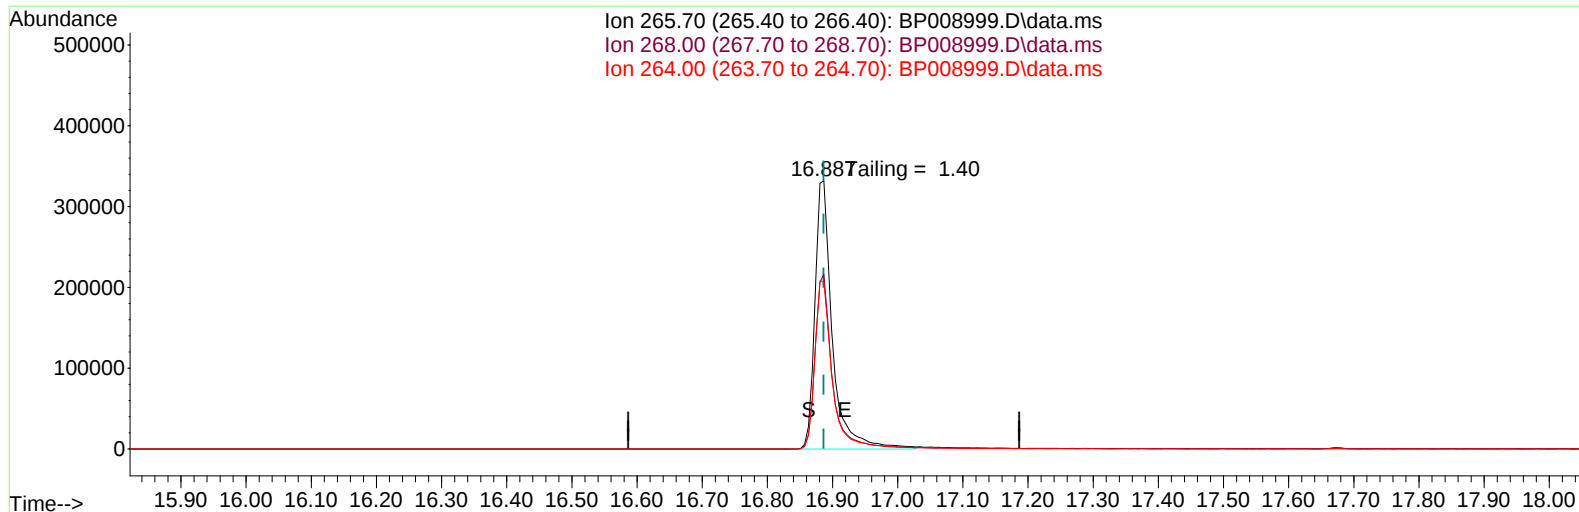

TIC: BP008999.D\data.ms

(70) Pentachlorophenol (C)

16.887min (+ 0.000) 562428.95 ng

response 621580

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	65.20
264.00	62.90	62.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2022	BNA_P	BP008999.D
Compound Name	Response	Retention Time
DDT	1807232	20.616
DDD	57072	20.192
DDE	5857	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
62929	1870161	3.36

Instrument :
BNA_P
ClientSampleId :
DFTPP