
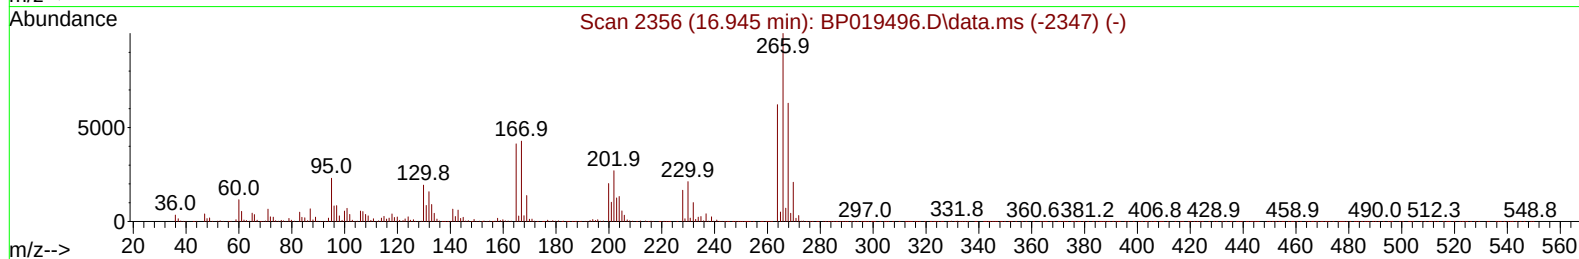
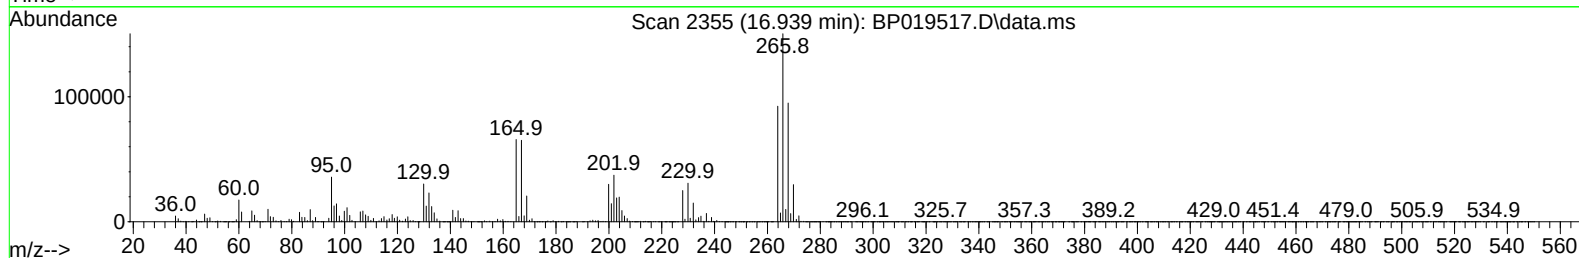


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020224\
Data File : BP019517.D
Acq On : 02 Feb 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 10:27:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

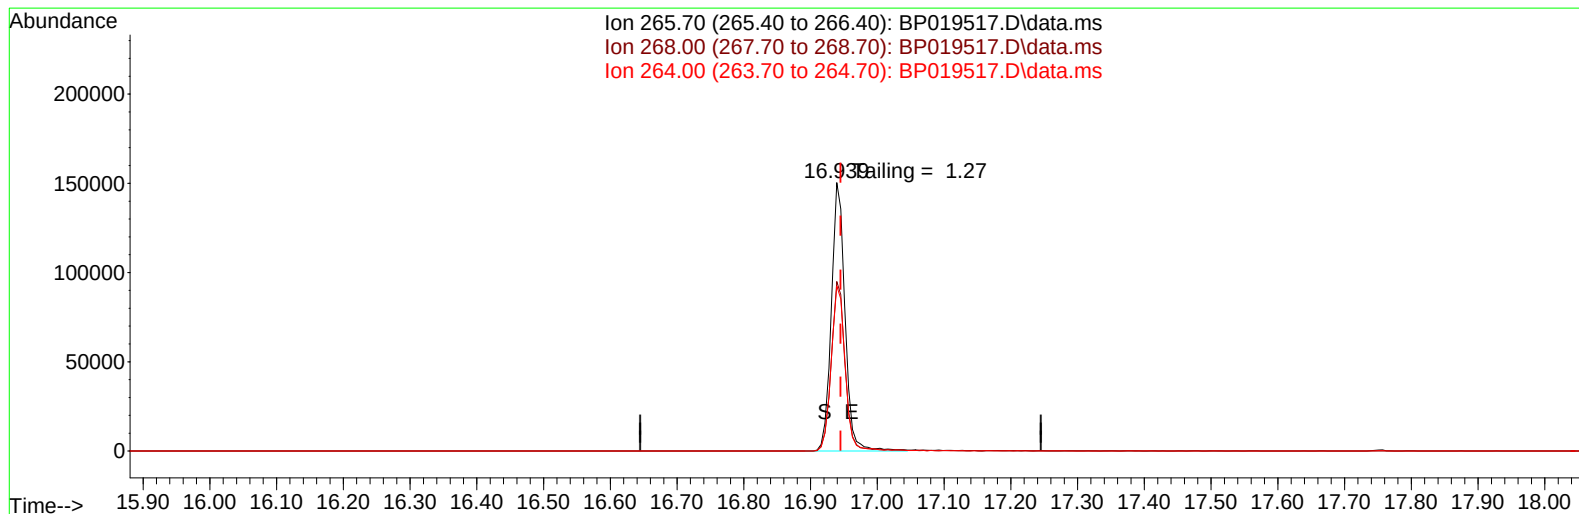

TIC: BP019517.D\data.ms

(70) Pentachlorophenol (C)




16.939min (-0.006) 3370138.65 ng

response 214470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.17
264.00	62.10	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020224\
Data File : BP019517.D
Acq On : 02 Feb 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 10:27:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

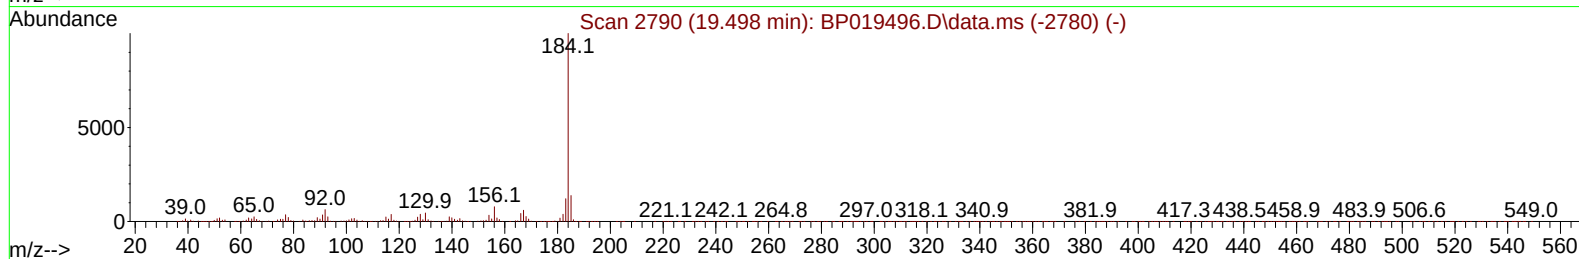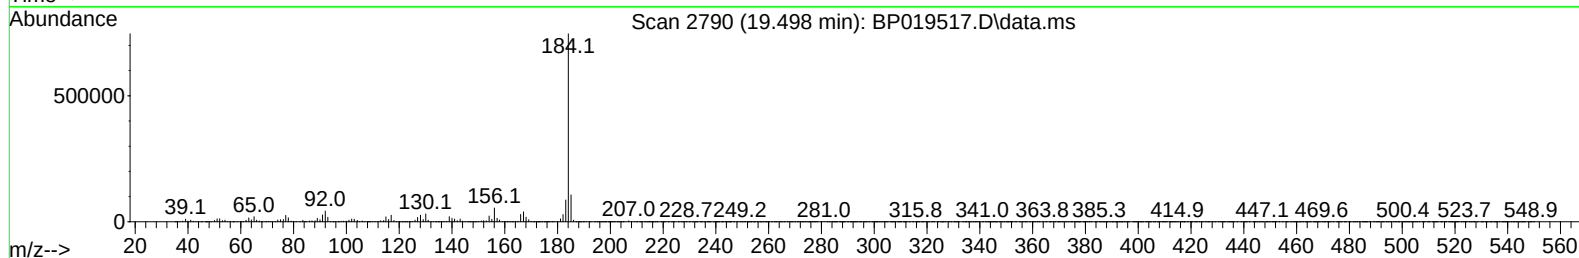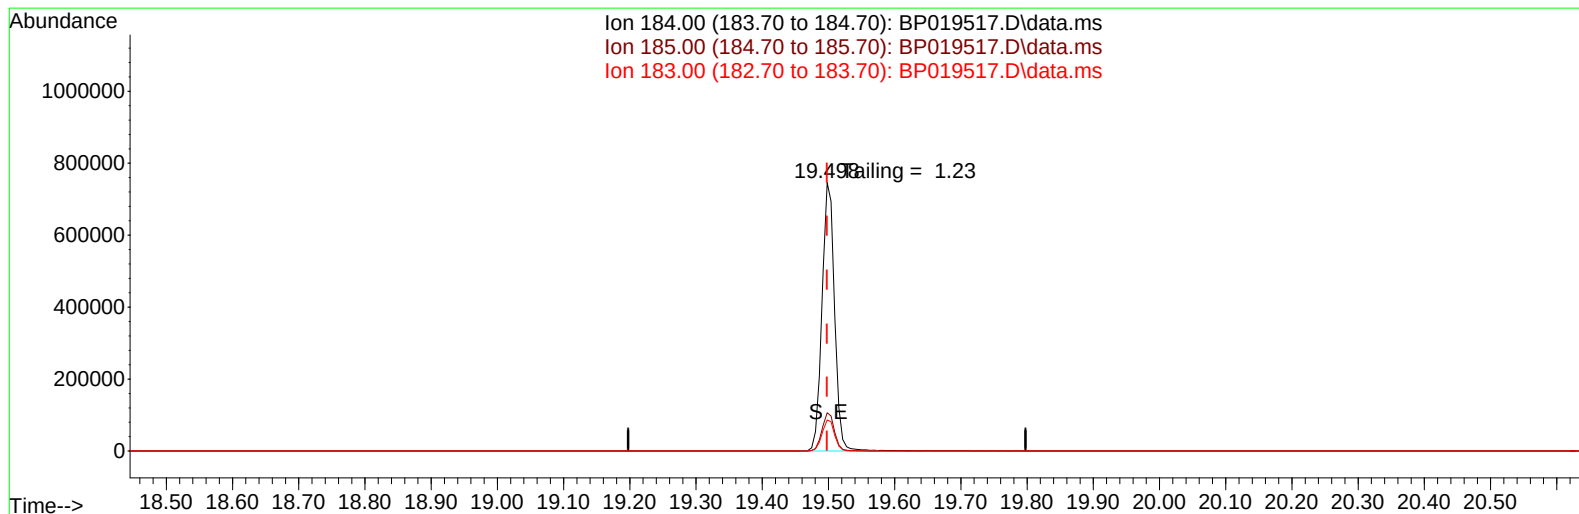

TIC: BP019517.D\data.ms

(77) Benzidine**19.498min (+ 0.000) 2048540.60 ng****response 985048**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.10	11.61
0.00	0.00	0.00