
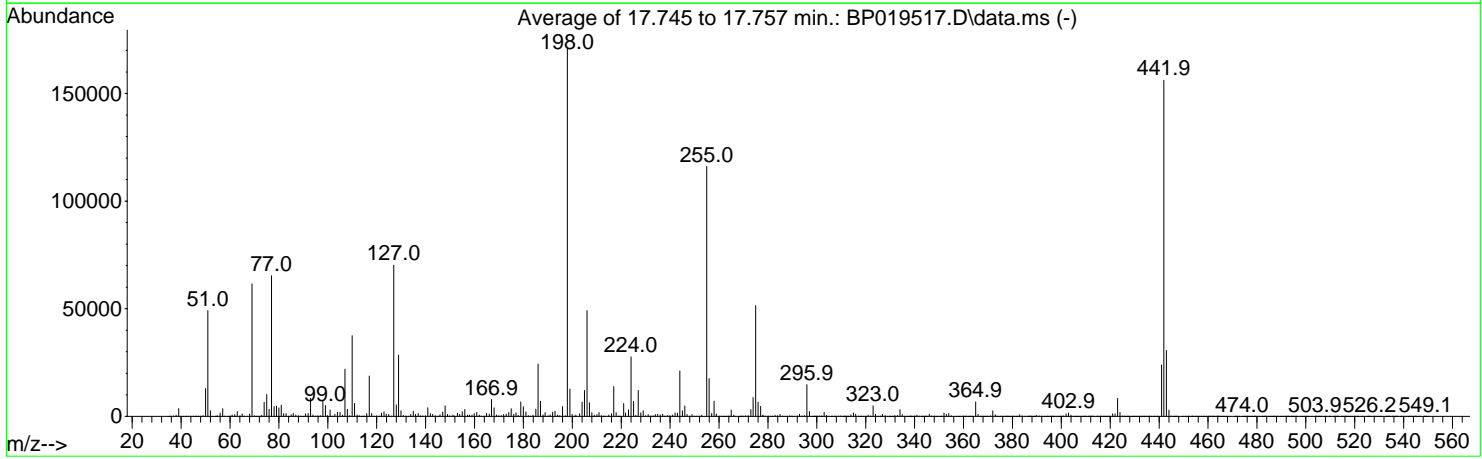


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020224\  
 Data File : BP019517.D  
 Acq On : 02 Feb 2024 08:34  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_P  
**ClientSampleId :**  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Feb 01 00:51:48 2024

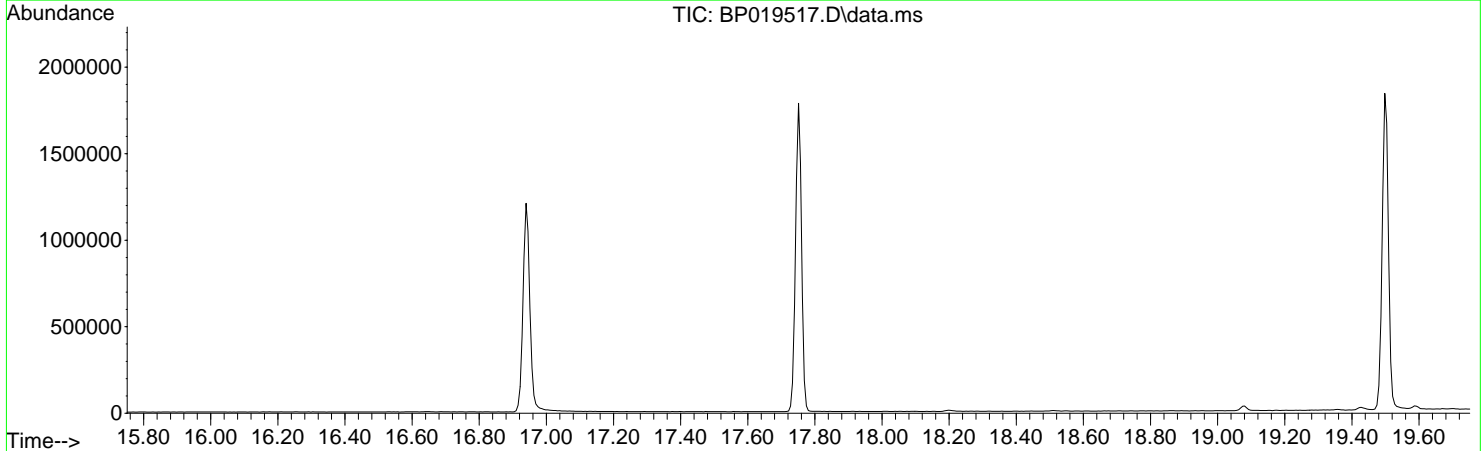




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	49137	PASS
68	69	0.00	2	1.7	1020	PASS
69	198	0.00	100	36.0	61544	PASS
70	69	0.00	2	0.5	316	PASS
127	198	10	80	41.1	70272	PASS
197	198	0.00	2	0.2	310	PASS
198	198	100	100	100.0	170919	PASS
199	198	5	9	7.5	12747	PASS
275	198	10	60	30.1	51427	PASS
365	198	1	100	3.9	6669	PASS
441	198	0.01	100	14.0	23860	PASS
442	442	100	100	100.0	156210	PASS
443	442	15	24	19.6	30637	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020224\  
 Data File : BP019517.D  
 Acq On : 02 Feb 2024 08:34  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_P  
**ClientSampleId :**  
 DFTPP

Quant Time: Feb 02 10:27:42 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 01 00:51:48 2024  
 Response via : Initial Calibration

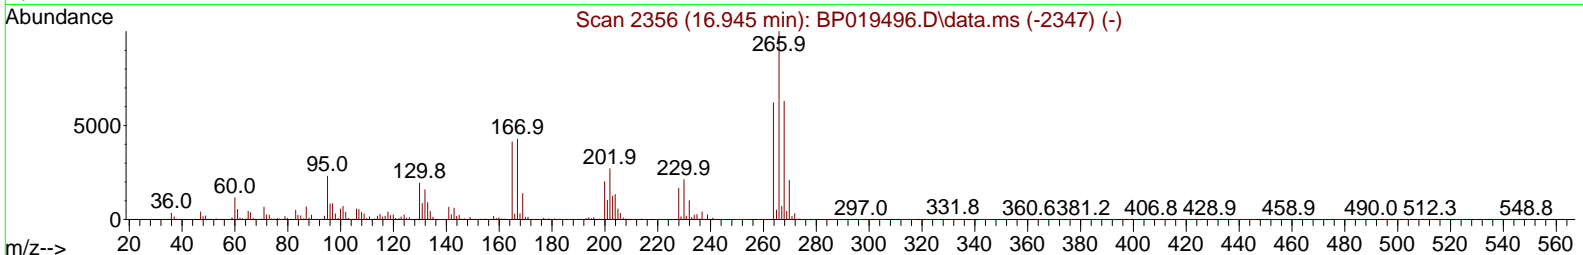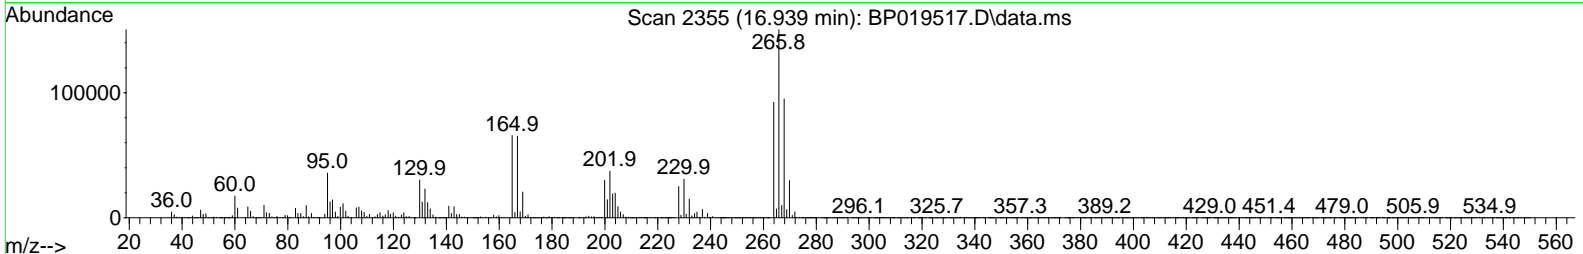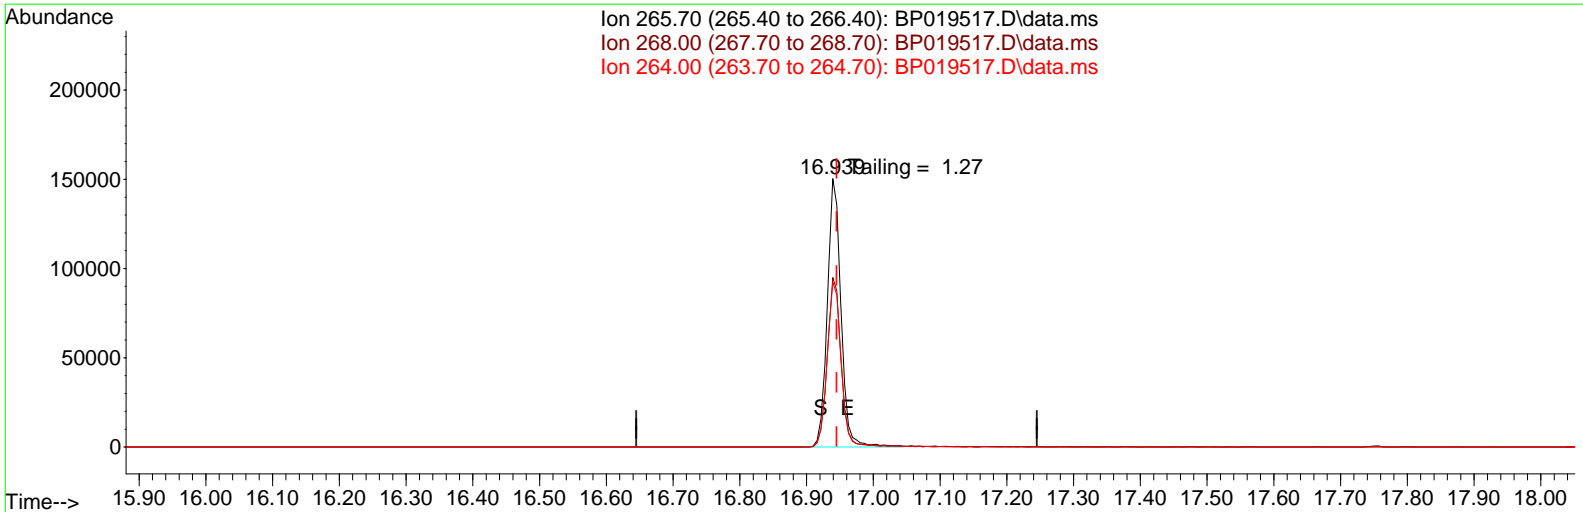

TIC: BP019517.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 3370138.65 ng




response 214470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.17
264.00	62.10	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020224\  
 Data File : BP019517.D  
 Acq On : 02 Feb 2024 08:34  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 02 10:27:42 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 01 00:51:48 2024  
 Response via : Initial Calibration

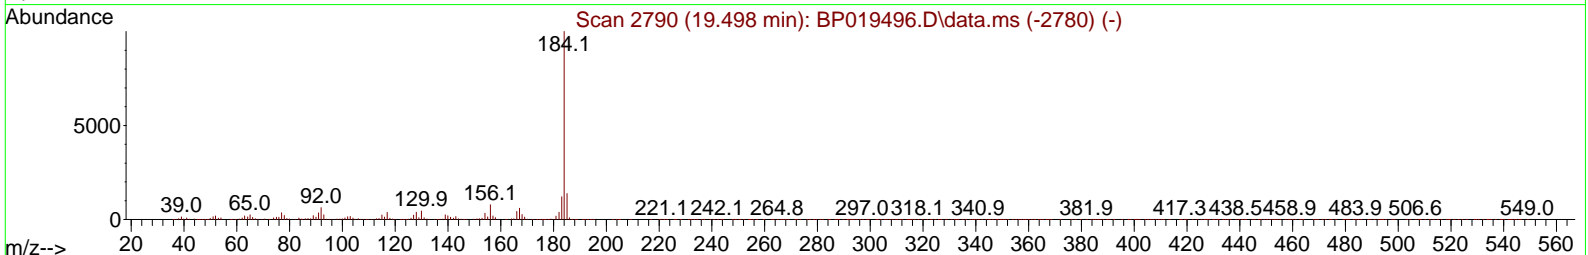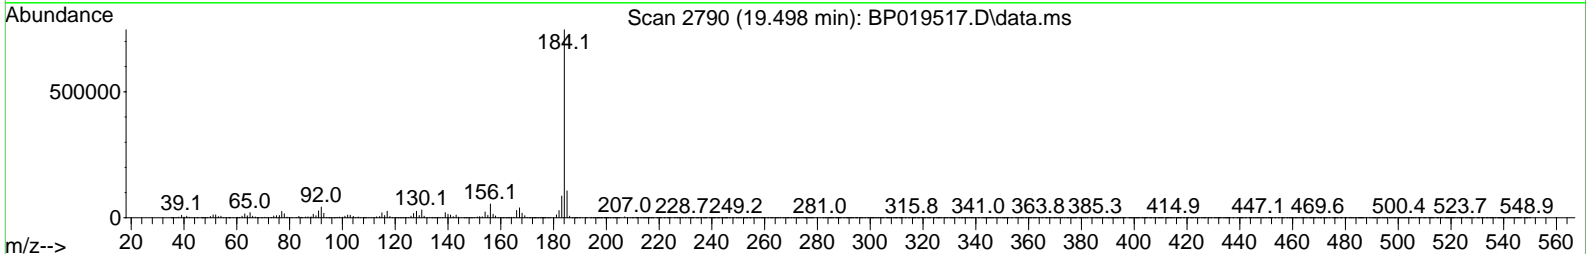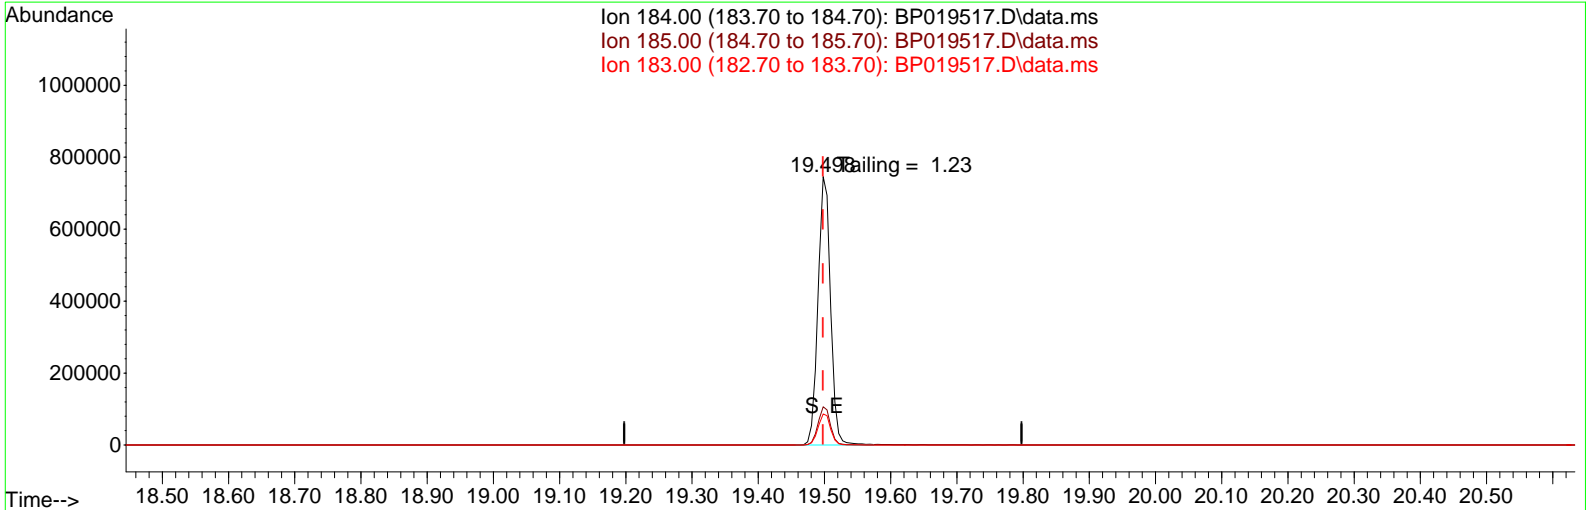

TIC: BP019517.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 2048540.60 ng

response 985048

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.10	11.61
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
2/2/2024	BNA_P	<u>BP019517.D</u>
Compound Name	Response	Retention Time
DDT	529862	20.704
DDD	11722	20.274
DDE	570	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12292	542154	2.27

Instrument :  
 BNA\_P  
 ClientSampled :  
 DFTPP