
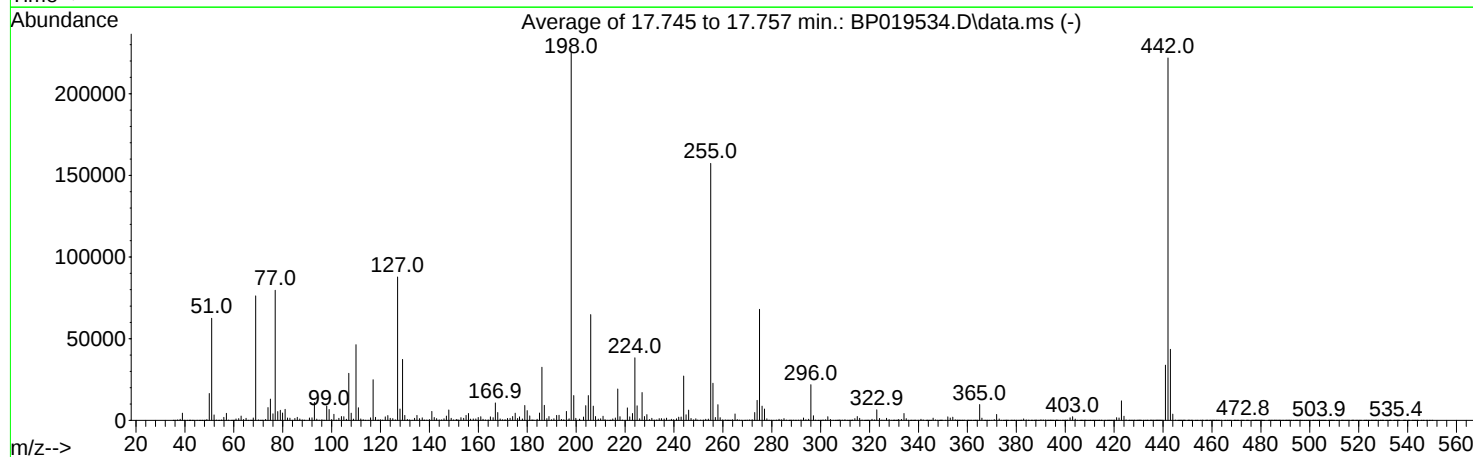


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020224\
Data File : BP019534.D
Acq On : 02 Feb 2024 19:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

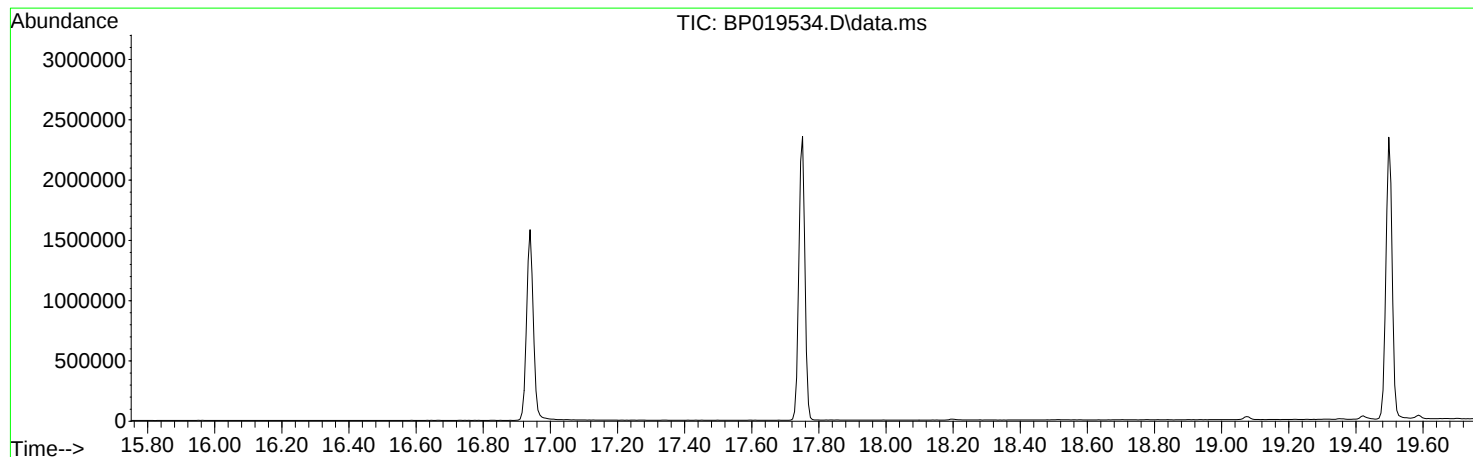




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	62464	PASS
68	69	0.00	2	2.0	1514	PASS
69	198	0.00	100	33.8	76221	PASS
70	69	0.00	2	0.4	310	PASS
127	198	10	80	39.0	87813	PASS
197	198	0.00	2	0.5	1016	PASS
198	198	100	100	100.0	225237	PASS
199	198	5	9	6.8	15212	PASS
275	198	10	60	30.2	68032	PASS
365	198	1	100	4.3	9740	PASS
441	198	0.01	100	15.0	33803	PASS
442	442	100	100	100.0	221908	PASS
443	442	15	24	19.6	43474	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020224\
Data File : BP019534.D
Acq On : 02 Feb 2024 19:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:51:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

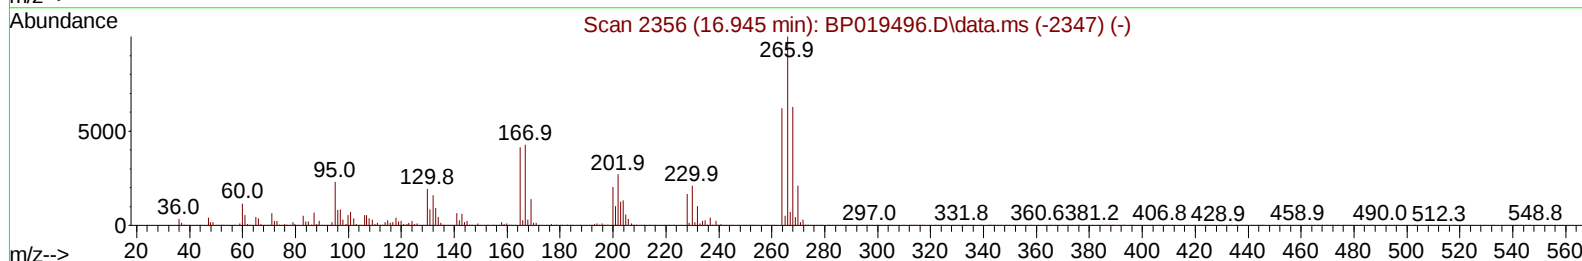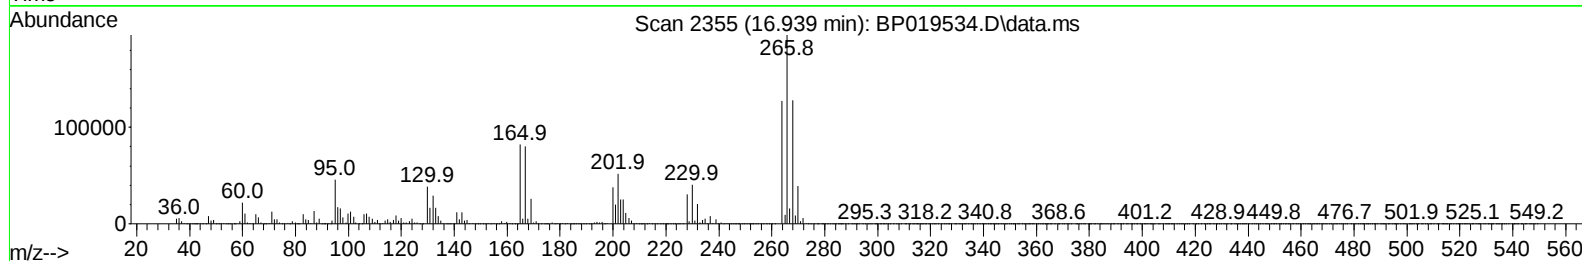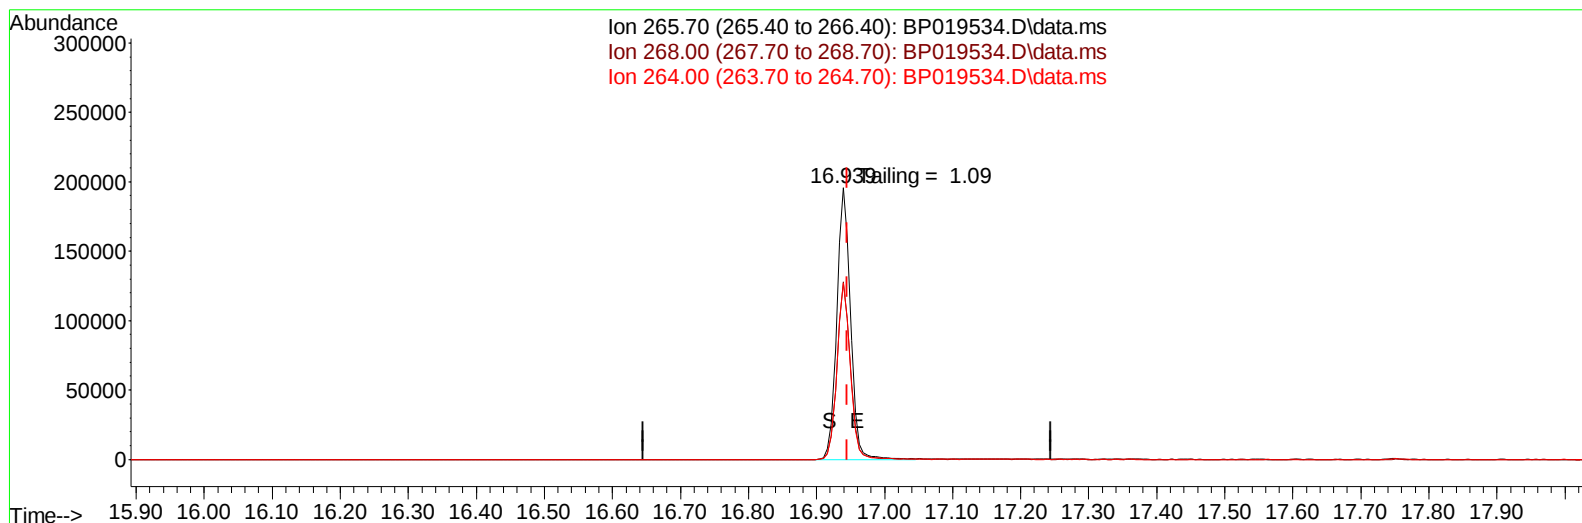

TIC: BP019534.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 1204269.16 ng




response 273706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.45
264.00	62.10	64.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020224\
Data File : BP019534.D
Acq On : 02 Feb 2024 19:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:51:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

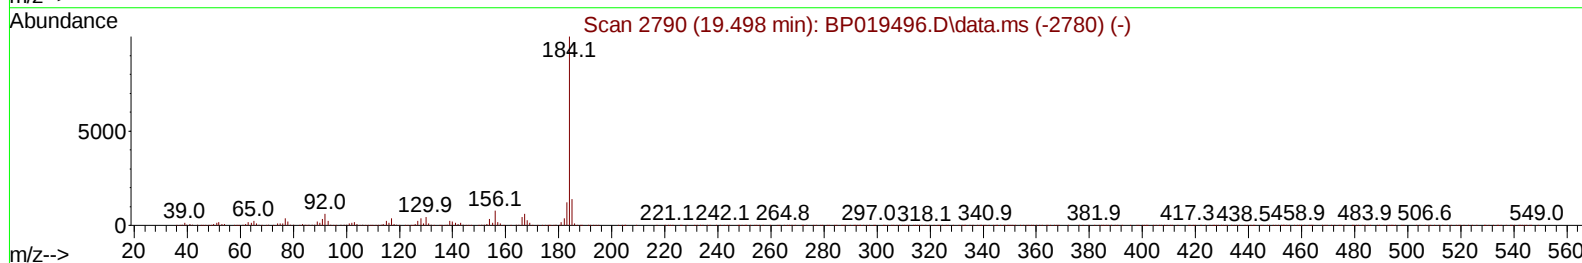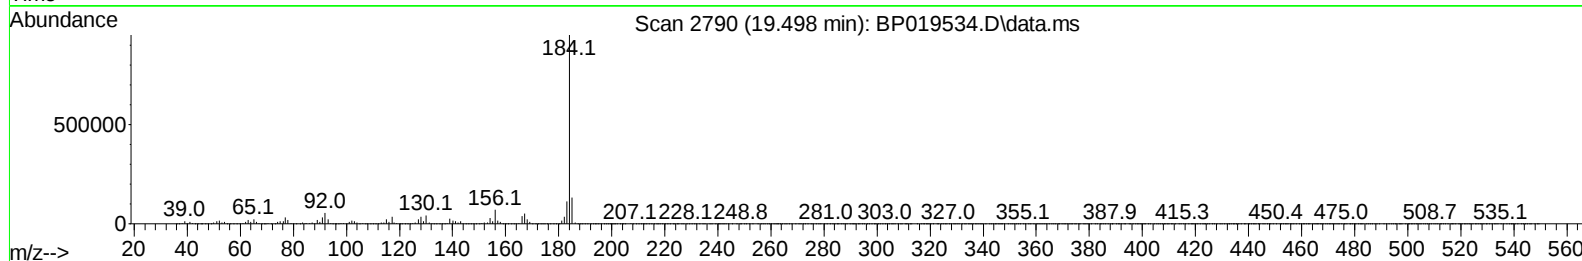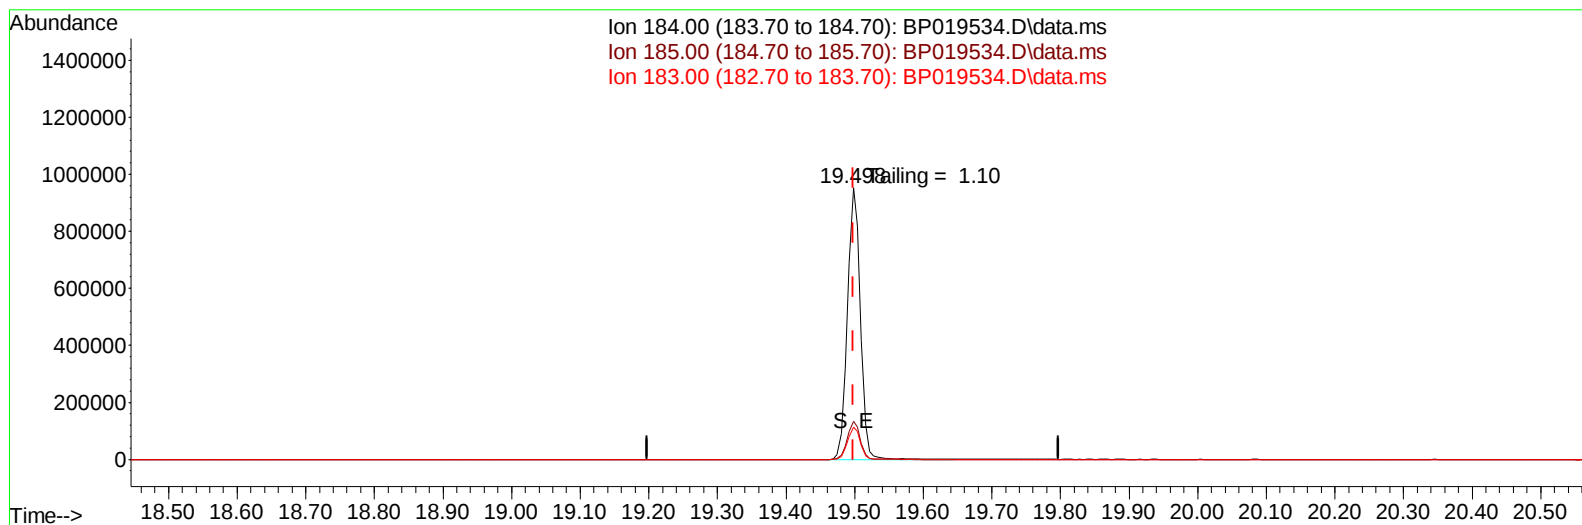

TIC: BP019534.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 2680457.45 ng

response 1232868

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.97
183.00	12.10	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2024	BNA_P	<u>BP019534.D</u>
Compound Name	Response	Retention Time
DDT	731956	20.698
DDD	15947	20.269
DDE	819	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16766	748722	2.24

Instrument :
BNA_P
ClientSampleId :
DFTPP